

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 11:19
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 20:51:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	67434655	137.2E6	47.504	57.374
28)	SA Decachlor...	9.112	7.932	91761619	123.8E6	45.597	46.485
Target Compounds							
23)	Chlordane-1	4.733	3.793	34375929	46858835	445.216	460.781
24)	Chlordane-2	5.263	4.369	36584107	54970599	441.934	448.480
25)	Chlordane-3	5.975	4.998	144.3E6	153.7E6	456.832	457.874
26)	Chlordane-4	6.058	5.062	173.3E6	142.8E6	455.252	449.338
27)	Chlordane-5	6.908	5.957	32089384	54064687	459.667	445.926



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 11:19
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 20:51:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

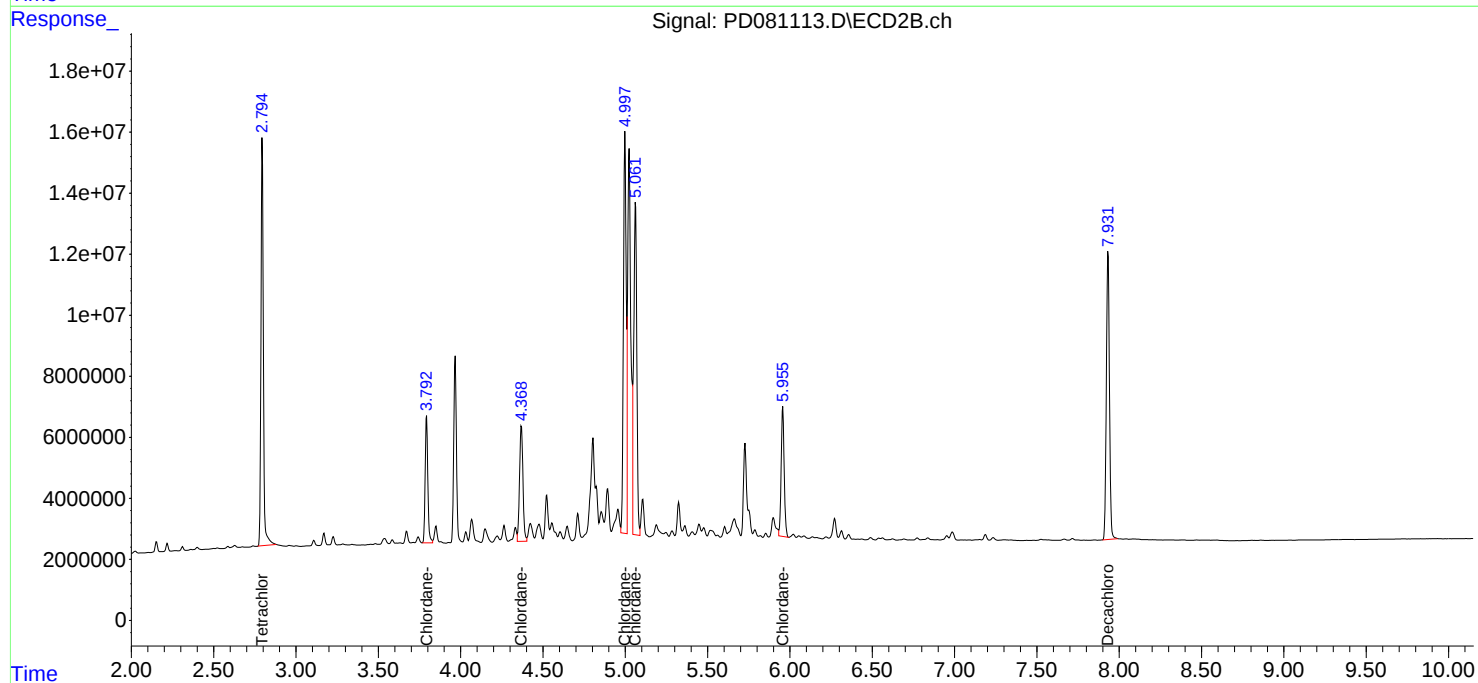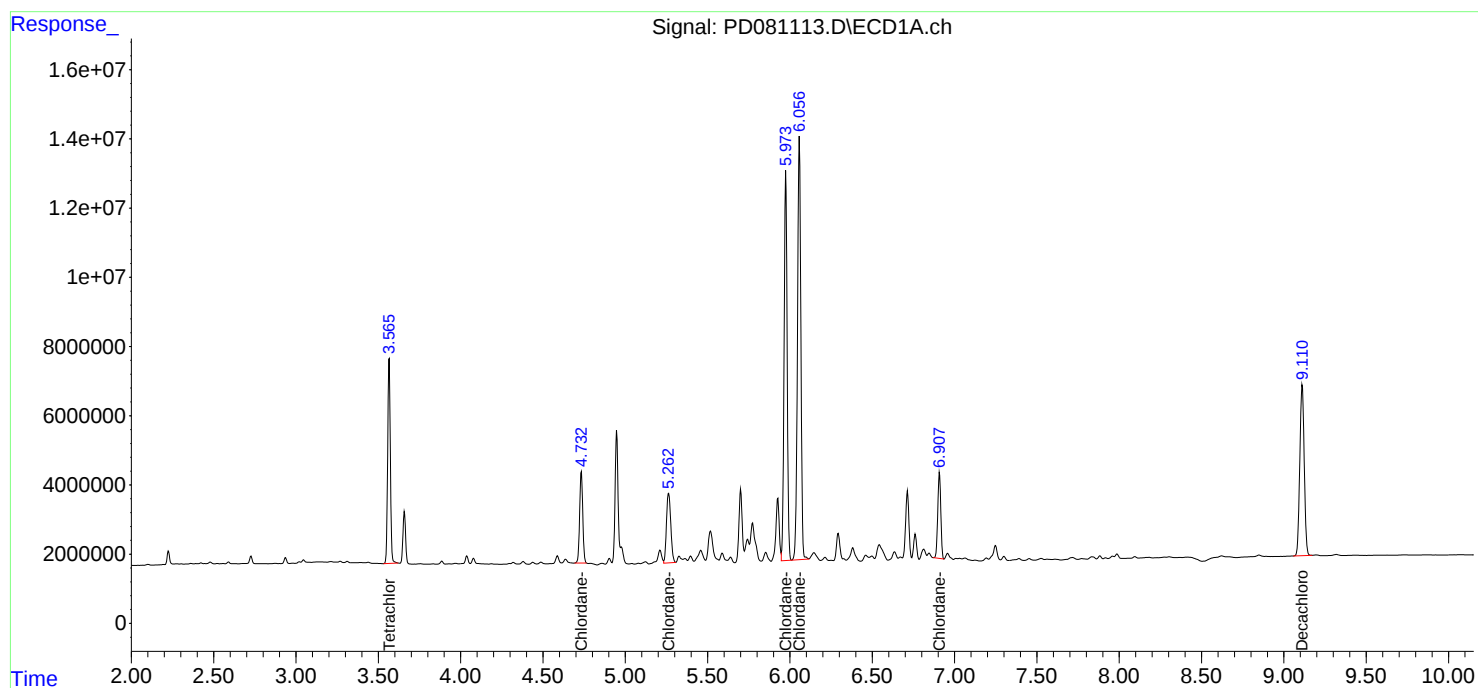


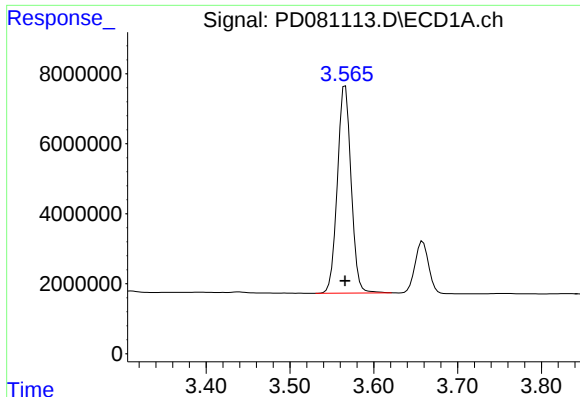

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 67434655
Conc: 47.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

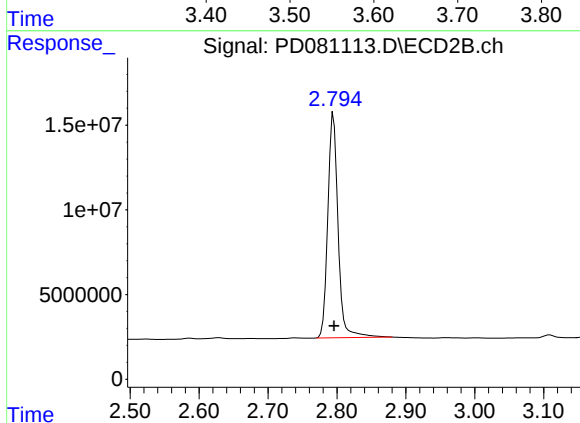


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 137248019
Conc: 57.37 ng/ml

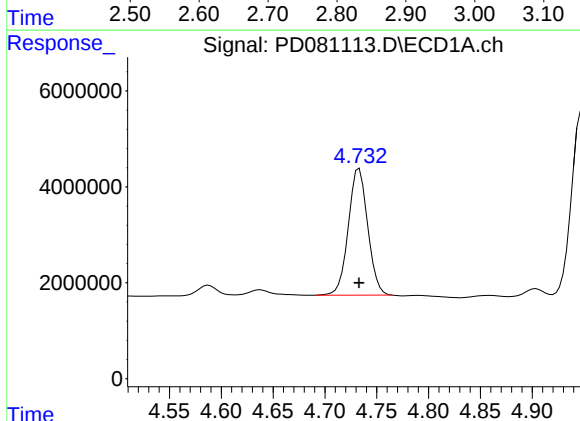


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 34375929
Conc: 445.22 ng/ml

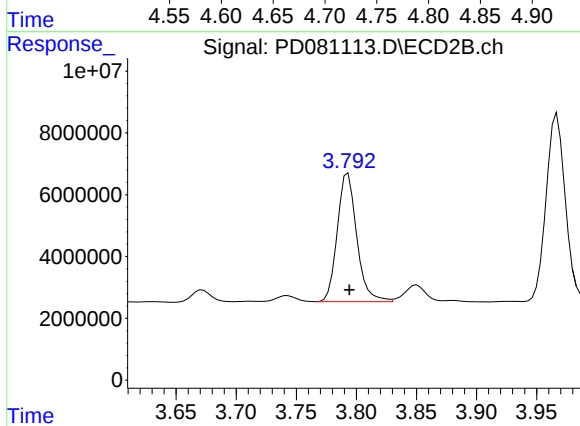

#23 Chlordane-1


R.T.: 3.793 min
Delta R.T.: -0.001 min
Response: 46858835
Conc: 460.78 ng/ml

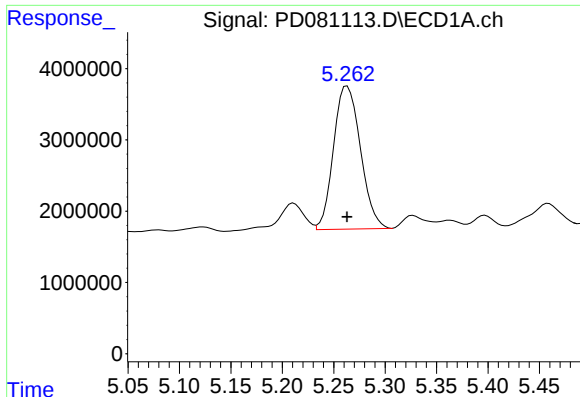

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 36584107
Conc: 441.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

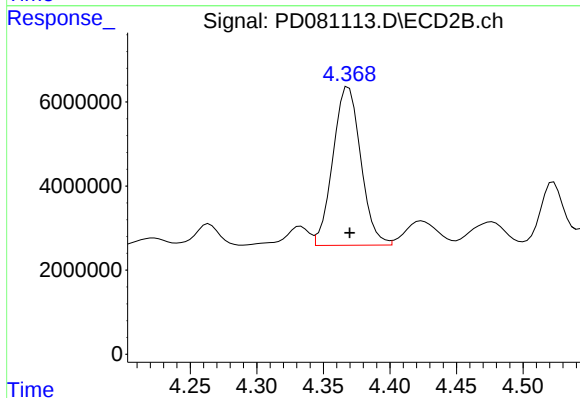


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 54970599
Conc: 448.48 ng/ml

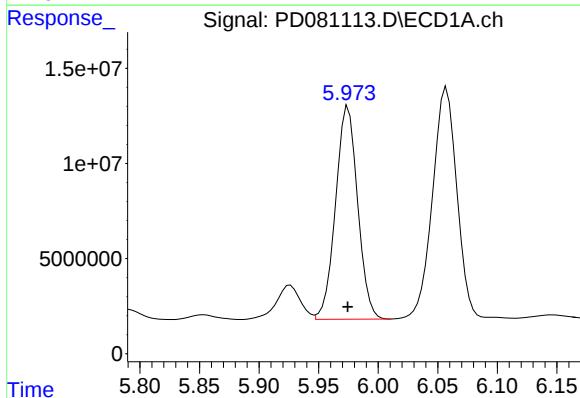


#25 Chlordane-3

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 144264698
Conc: 456.83 ng/ml

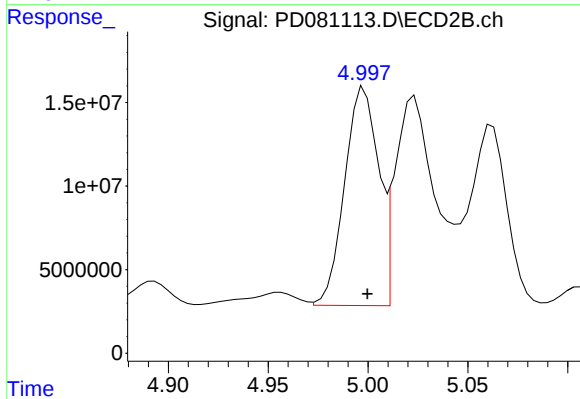

#25 Chlordane-3


R.T.: 4.998 min
Delta R.T.: -0.002 min
Response: 153669939
Conc: 457.87 ng/ml

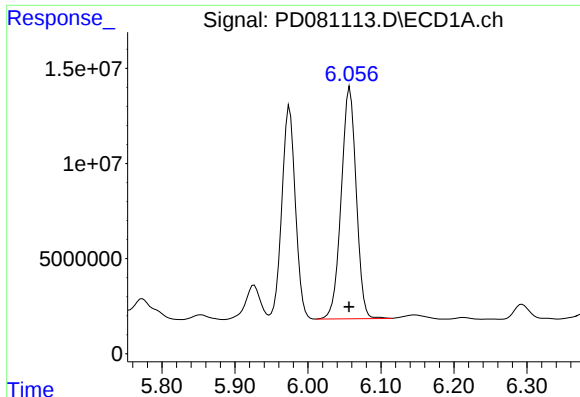

#26 Chlordane-4


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 173335058
Conc: 455.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

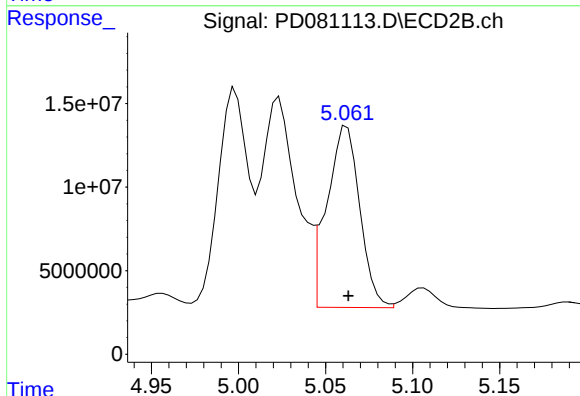


#26 Chlordane-4

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 142752683
Conc: 449.34 ng/ml

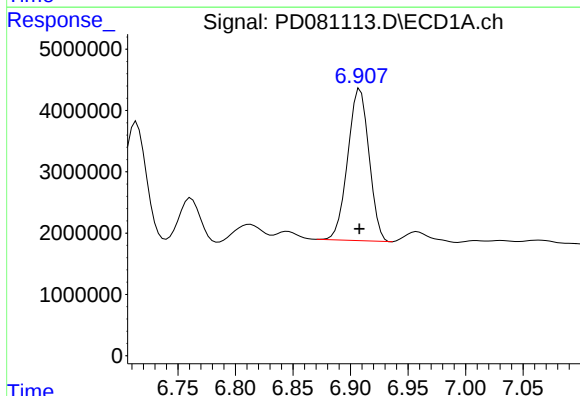


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 32089384
Conc: 459.67 ng/ml

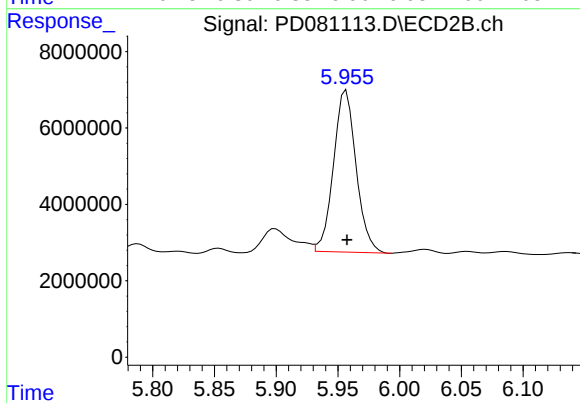

#27 Chlordane-5


R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 54064687
Conc: 445.93 ng/ml

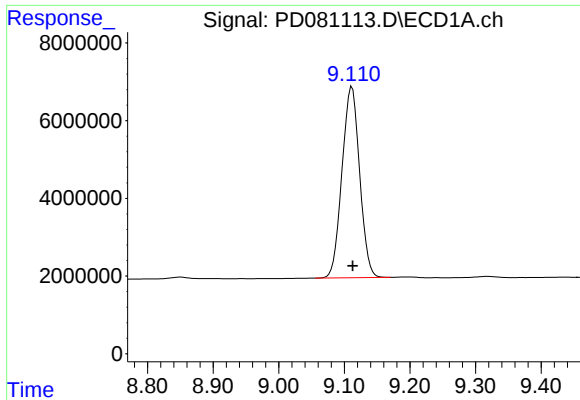

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.001 min
Response: 91761619
Conc: 45.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

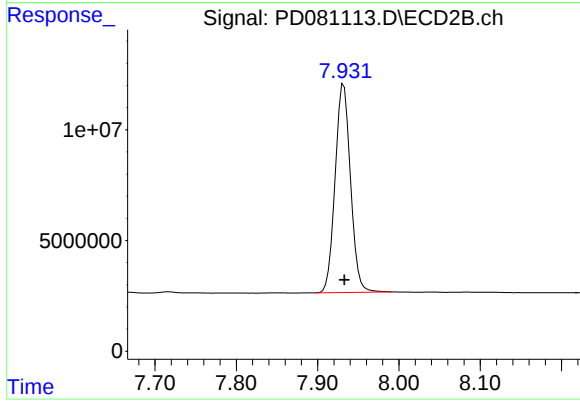

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 123818891
Conc: 46.49 ng/ml