

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 12:23
 Operator : AR\AJ
 Sample : PB158813BS
 Misc : CHLOR BS
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB158813BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 20:52:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.794	31940903	69770443	22.500	29.166 #
28)	SA Decachlor...	9.117	7.933	45428657	66087935	22.574	24.811
Target Compounds							
23)	Chlordane-1	4.738	3.792	16768619	23003327	217.177	226.201
24)	Chlordane-2	5.268	4.368	18745532	27939716	226.445	227.947
25)	Chlordane-3	5.979	4.998	67441885	75604917	213.563	225.272
26)	Chlordane-4	6.062	5.062	81457004	70498331	213.941	221.905
27)	Chlordane-5	6.913	5.956	15054631	27397311	215.651	225.973



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 12:23
Operator : AR\AJ
Sample : PB158813BS
Misc : CHLOR BS
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB158813BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 20:52:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

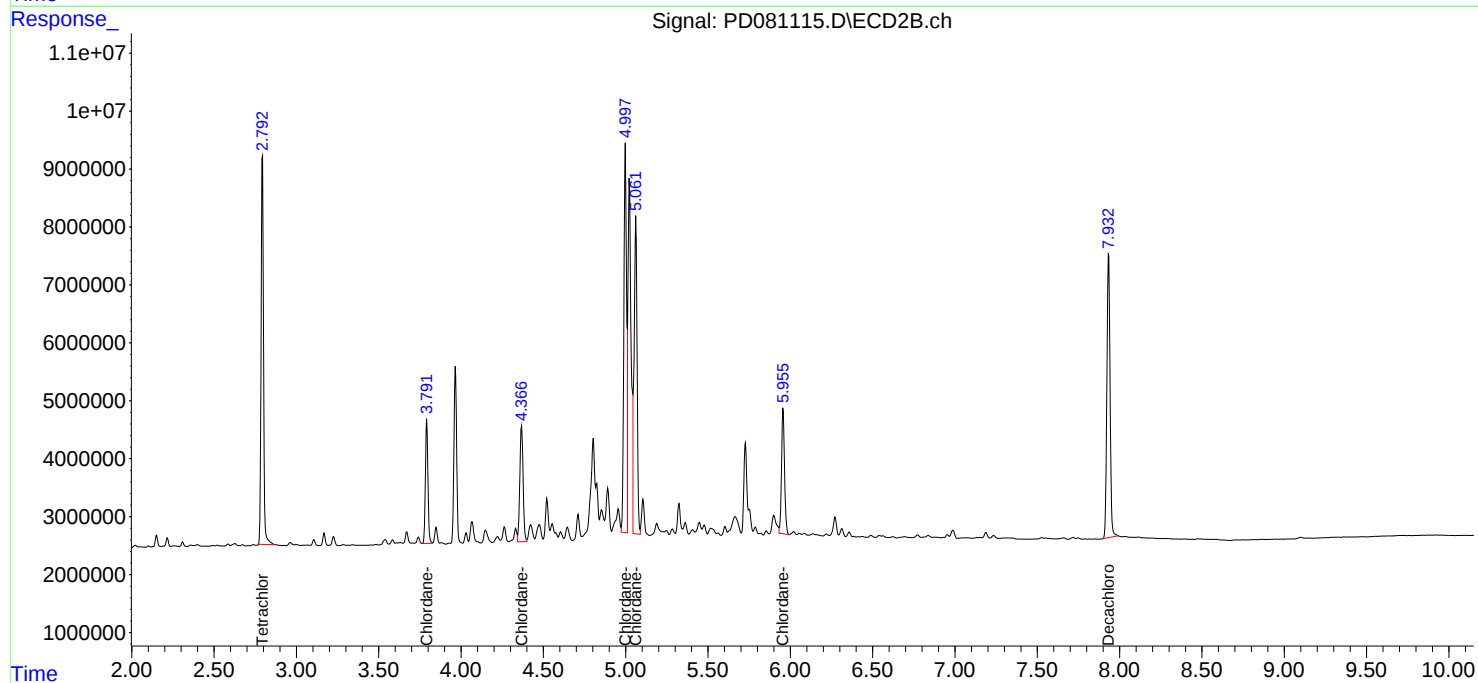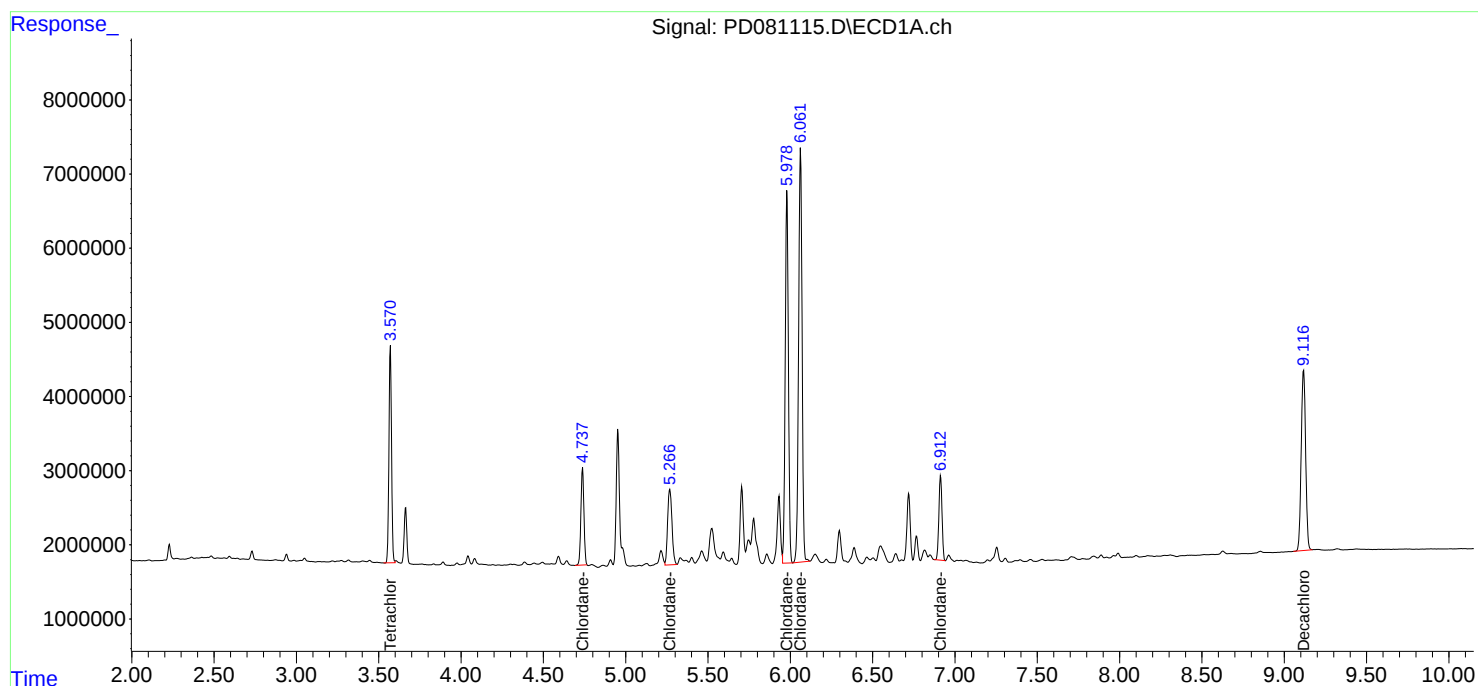


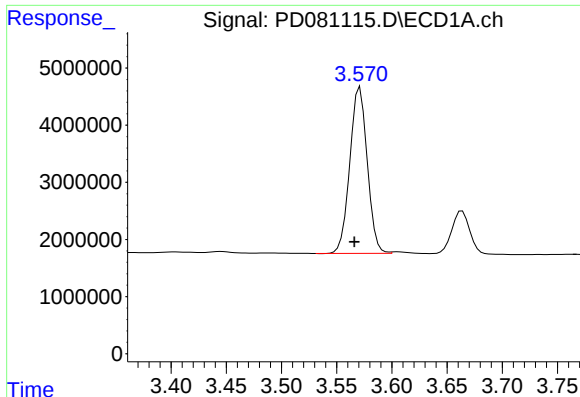

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.005 min
Response: 31940903
Conc: 22.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158813BS

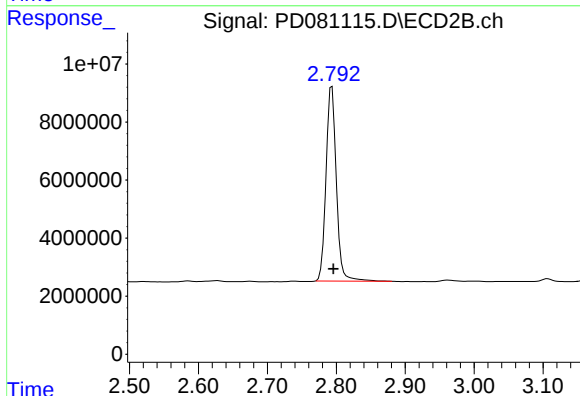


#1 Tetrachloro-m-xylene

R.T.: 2.794 min
Delta R.T.: -0.002 min
Response: 69770443
Conc: 29.17 ng/ml

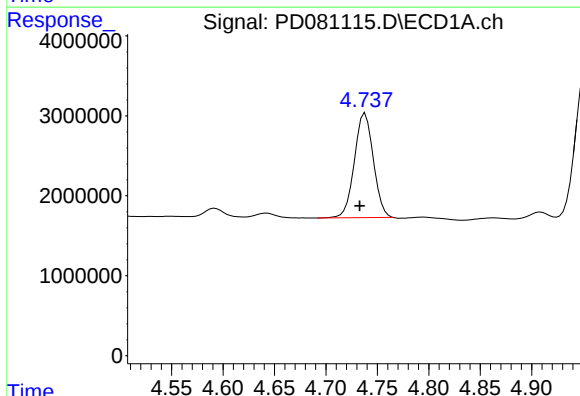


#23 Chlordane-1

R.T.: 4.738 min
Delta R.T.: 0.005 min
Response: 16768619
Conc: 217.18 ng/ml

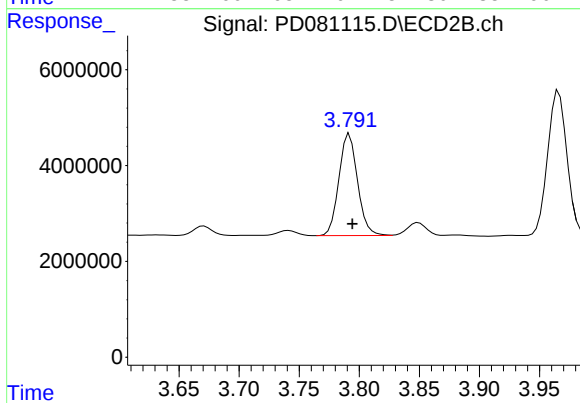

#23 Chlordane-1


R.T.: 3.792 min
Delta R.T.: -0.002 min
Response: 23003327
Conc: 226.20 ng/ml

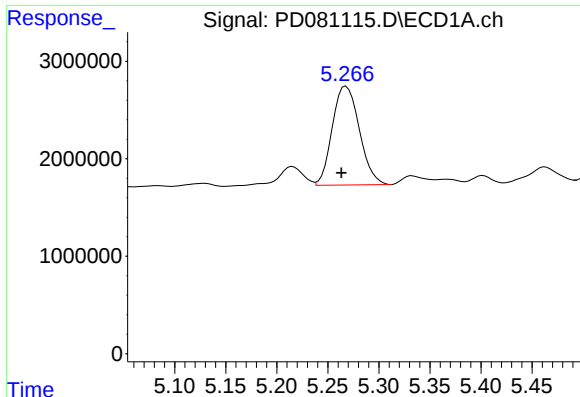

#24 Chlordane-2


R.T.: 5.268 min
Delta R.T.: 0.005 min
Response: 18745532
Conc: 226.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158813BS

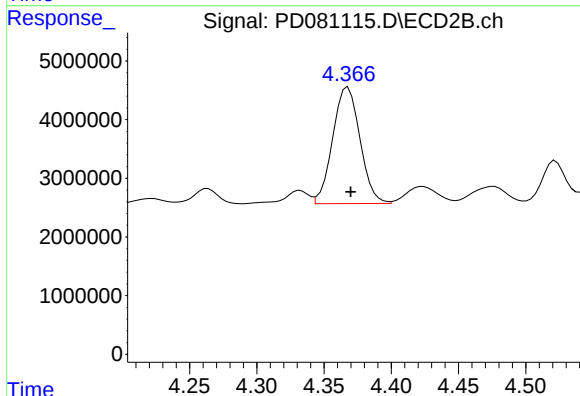


#24 Chlordane-2

R.T.: 4.368 min
Delta R.T.: -0.002 min
Response: 27939716
Conc: 227.95 ng/ml

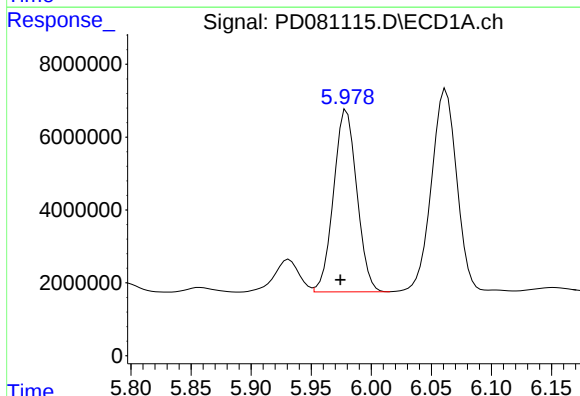


#25 Chlordane-3

R.T.: 5.979 min
Delta R.T.: 0.005 min
Response: 67441885
Conc: 213.56 ng/ml

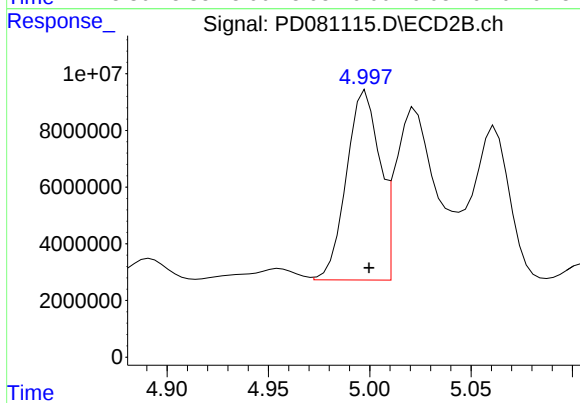

#25 Chlordane-3


R.T.: 4.998 min
Delta R.T.: -0.002 min
Response: 75604917
Conc: 225.27 ng/ml

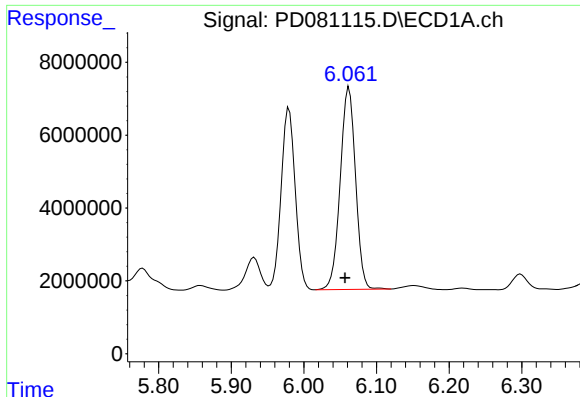

#26 Chlordane-4


R.T.: 6.062 min
Delta R.T.: 0.006 min
Response: 81457004
Conc: 213.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158813BS

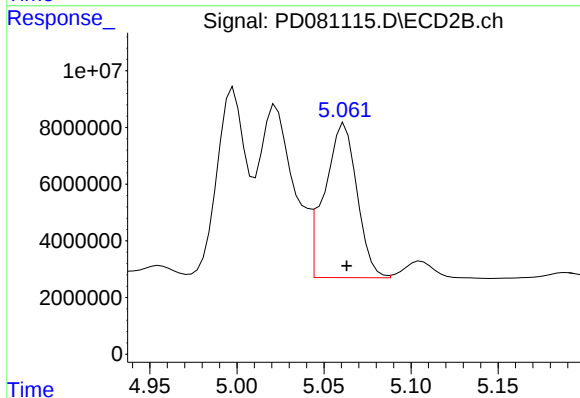


#26 Chlordane-4

R.T.: 5.062 min
Delta R.T.: -0.001 min
Response: 70498331
Conc: 221.91 ng/ml

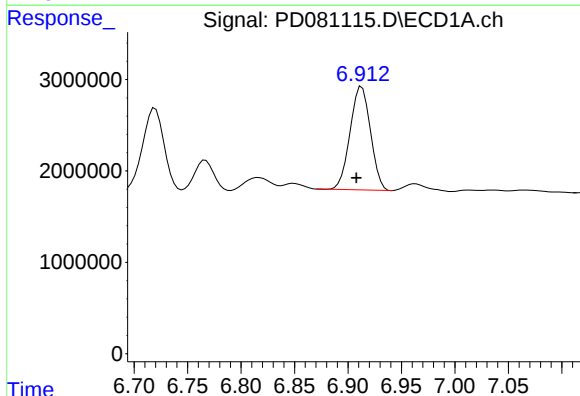


#27 Chlordane-5

R.T.: 6.913 min
Delta R.T.: 0.005 min
Response: 15054631
Conc: 215.65 ng/ml

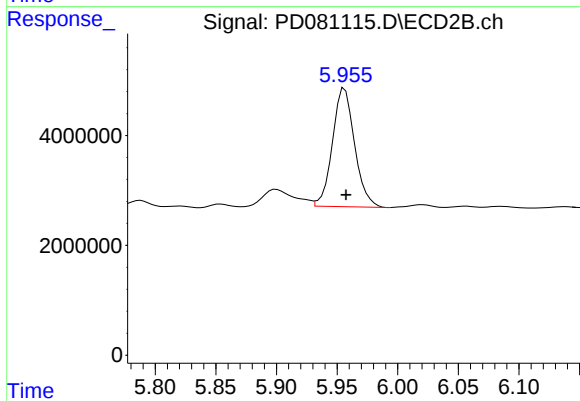

#27 Chlordane-5


R.T.: 5.956 min
Delta R.T.: -0.001 min
Response: 27397311
Conc: 225.97 ng/ml

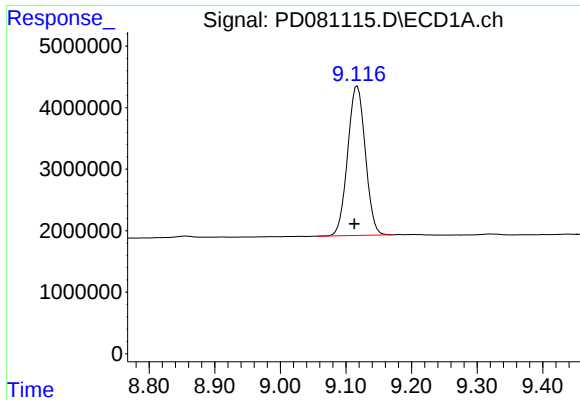

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.004 min
Response: 45428657
Conc: 22.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158813BS

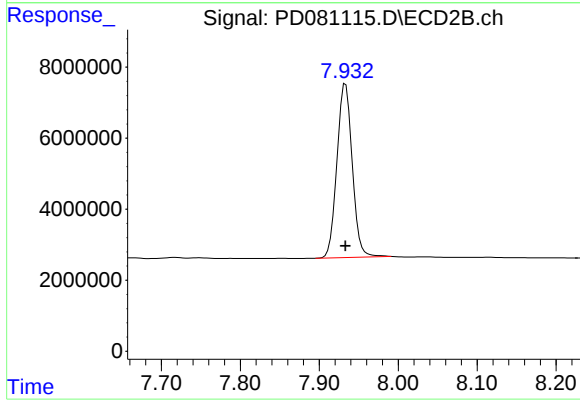

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 66087935
Conc: 24.81 ng/ml