

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 16:39
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:04:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.795	61710777	138.9E6	43.472	58.083 #
28)	SA Decachlor...	9.116	7.933	81826154	120.9E6	40.660	45.396
Target Compounds							
23)	Chlordane-1	4.737	3.794	32785342	45789412	424.616	450.265
24)	Chlordane-2	5.267	4.370	35338647	53733509	426.889	438.387
25)	Chlordane-3	5.978	4.999	130.6E6	151.5E6	413.651	451.396
26)	Chlordane-4	6.061	5.063	157.9E6	142.9E6	414.621	449.688
27)	Chlordane-5	6.912	5.958	29938092	53750358	428.850	443.333



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 16:39
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:04:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

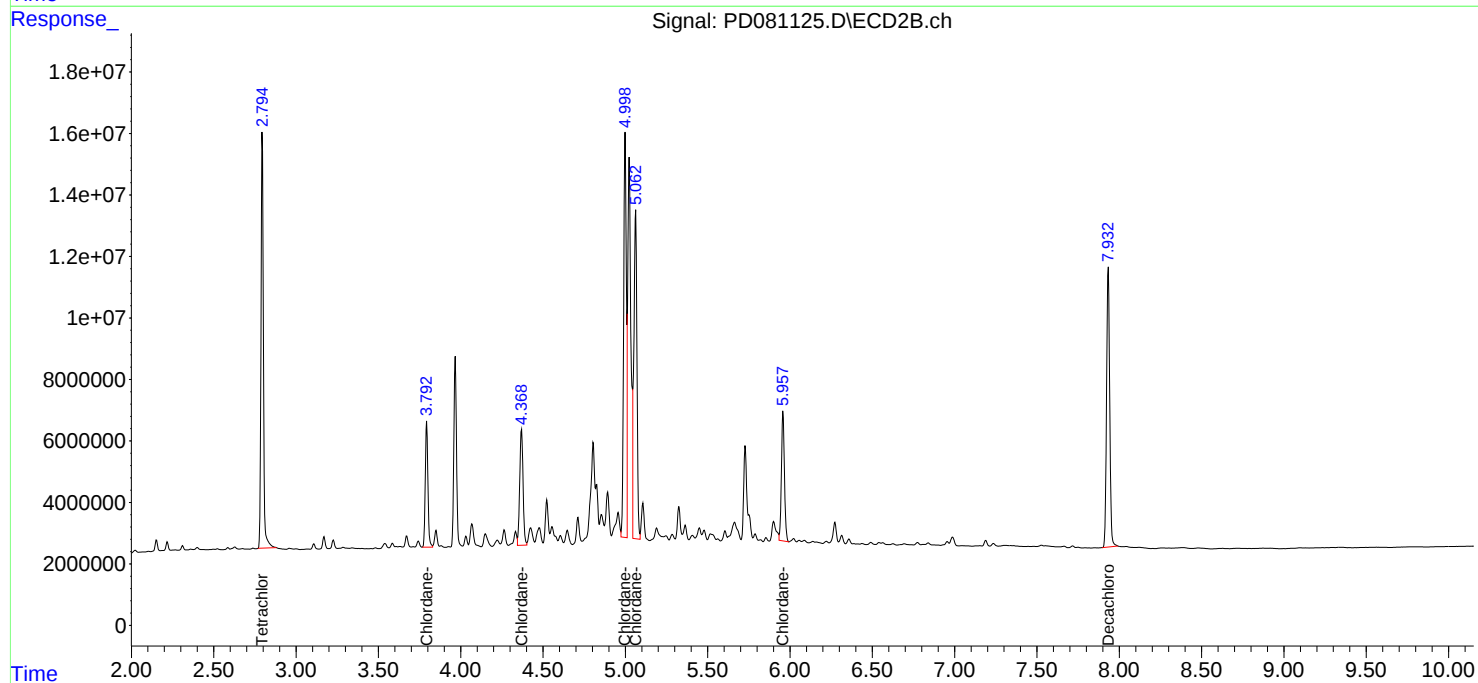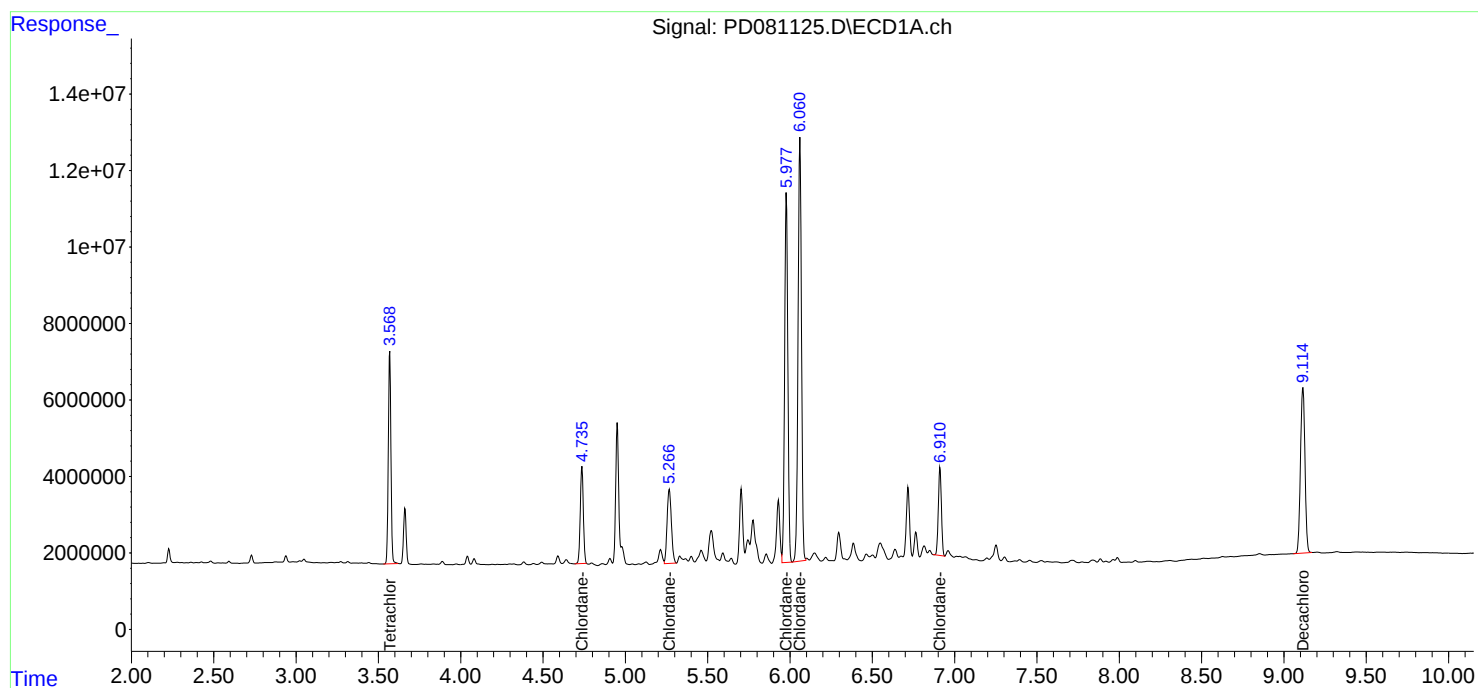


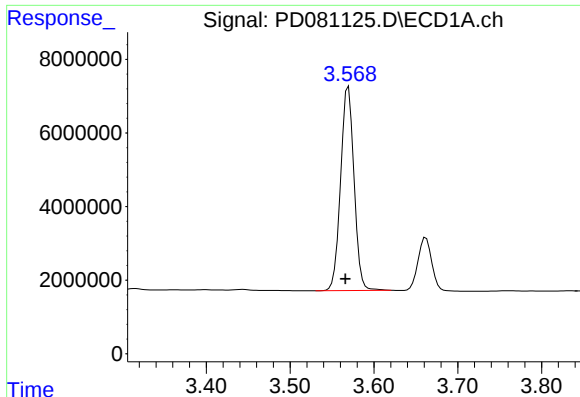

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.004 min
Response: 61710777
Conc: 43.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

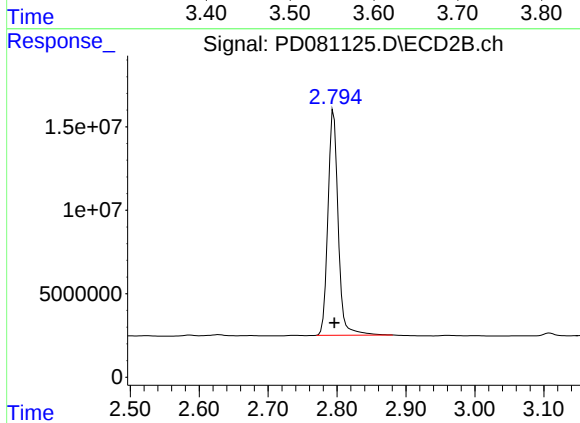


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 138943720
Conc: 58.08 ng/ml

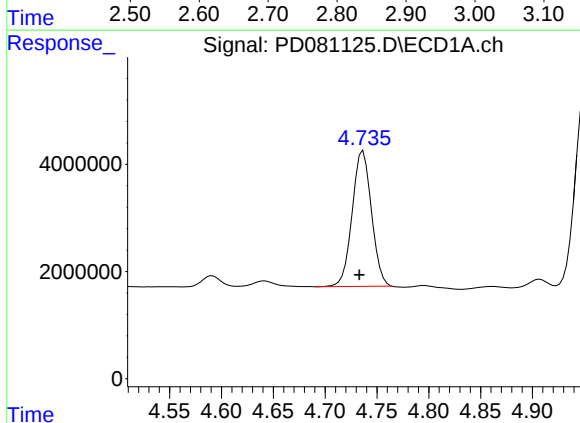


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.004 min
Response: 32785342
Conc: 424.62 ng/ml

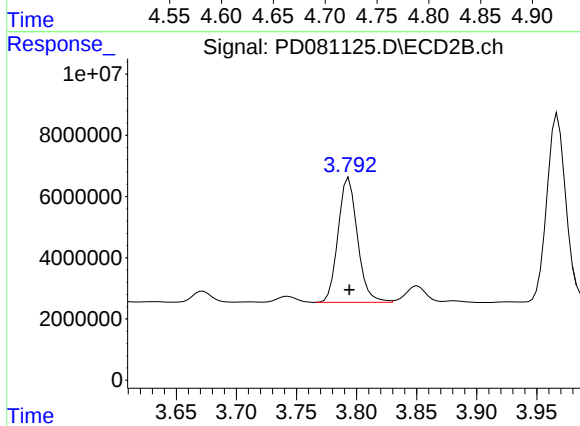

#23 Chlordane-1


R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 45789412
Conc: 450.26 ng/ml

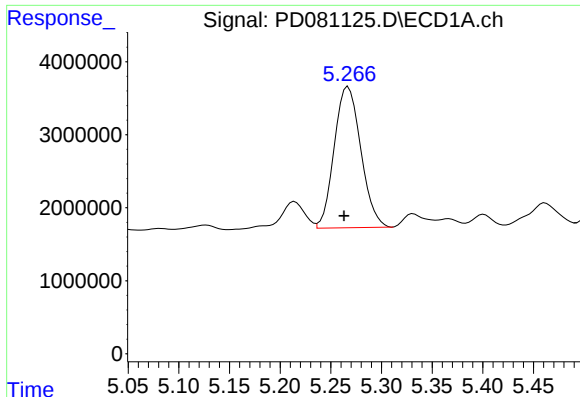

#24 Chlordane-2


R.T.: 5.267 min
Delta R.T.: 0.004 min
Response: 35338647
Conc: 426.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

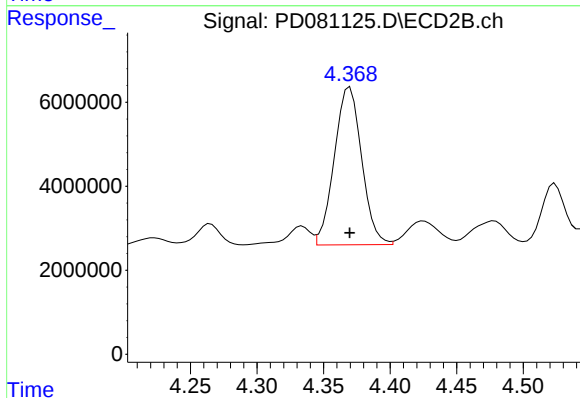


#24 Chlordane-2

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 53733509
Conc: 438.39 ng/ml

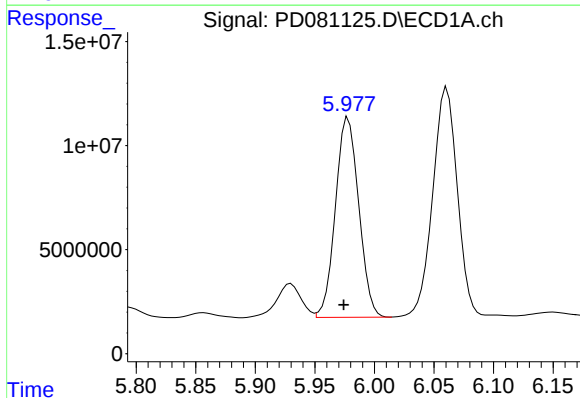


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.004 min
Response: 130628368
Conc: 413.65 ng/ml

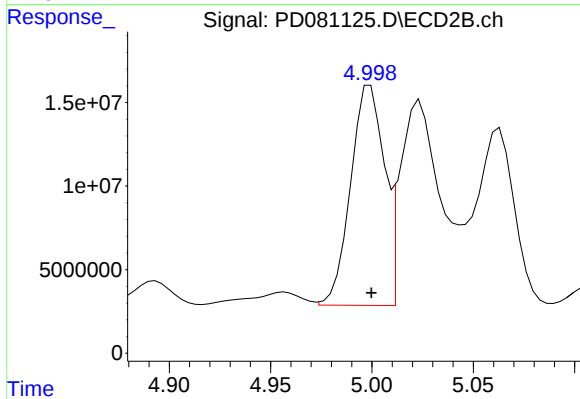

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 151495626
Conc: 451.40 ng/ml

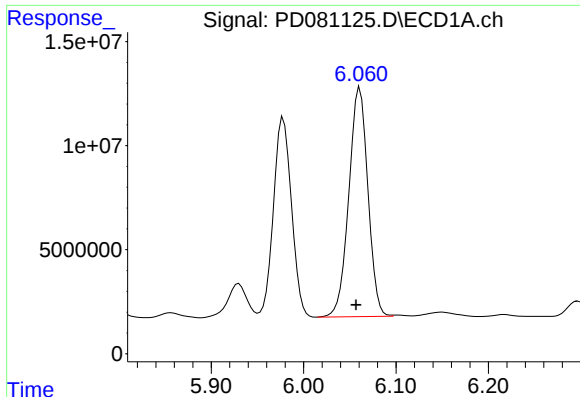

#26 Chlordane-4


R.T.: 6.061 min
Delta R.T.: 0.004 min
Response: 157864950
Conc: 414.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

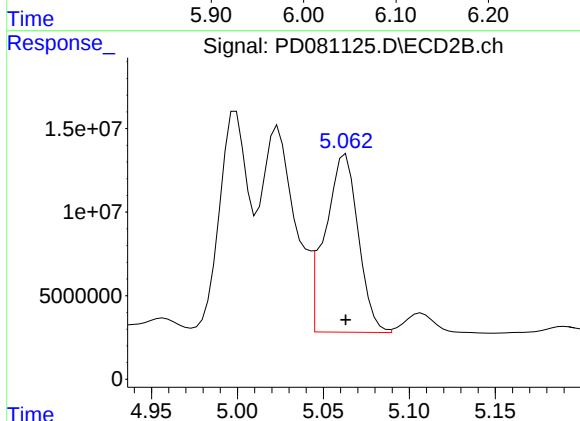


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 142863660
Conc: 449.69 ng/ml

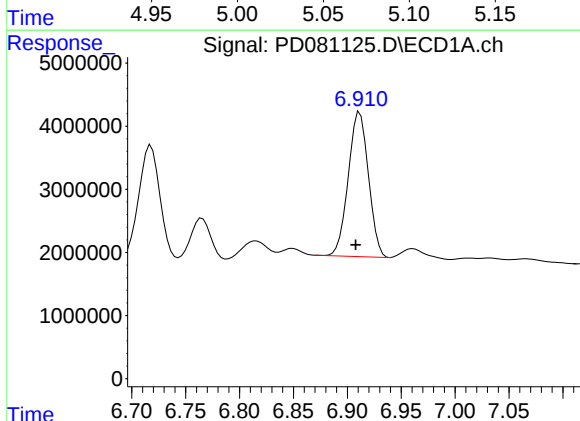


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.004 min
Response: 29938092
Conc: 428.85 ng/ml

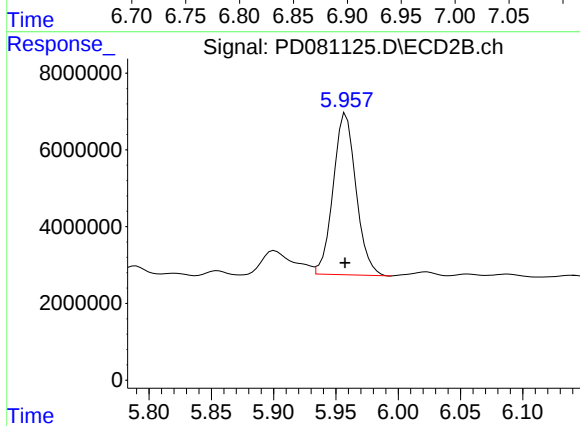

#27 Chlordane-5


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 53750358
Conc: 443.33 ng/ml

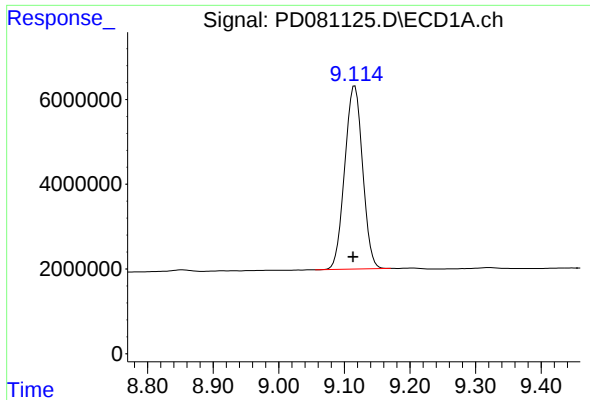

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.003 min
Response: 81826154
Conc: 40.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

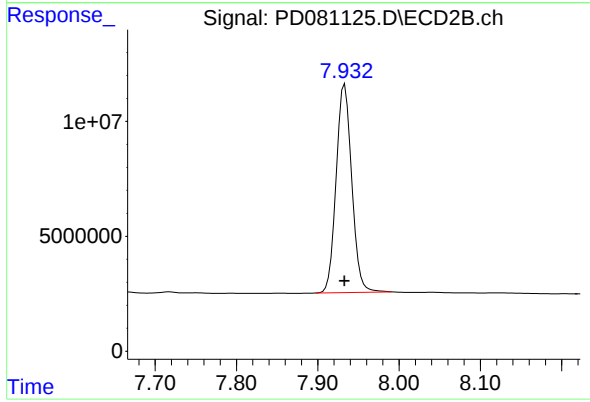

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 120918274
Conc: 45.40 ng/ml