

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 17:07
 Operator : AR\AJ
 Sample : P1327-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MANHOLE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/08/2024
 Supervised By : Ankita Jodhani 02/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 16:23:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.564	2.795	22969041	42469557	16.180m	17.754
28) SA Decachlor...	9.110	7.932	12554712	17491193	6.239m	6.567
Target Compounds						
7) B delta-BHC	4.791	4.154	10055329	18002616	4.008m	4.797m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 17:07
Operator : AR\AJ
Sample : P1327-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MANHOLE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/08/2024
Supervised By : Ankita Jodhani 02/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 16:23:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

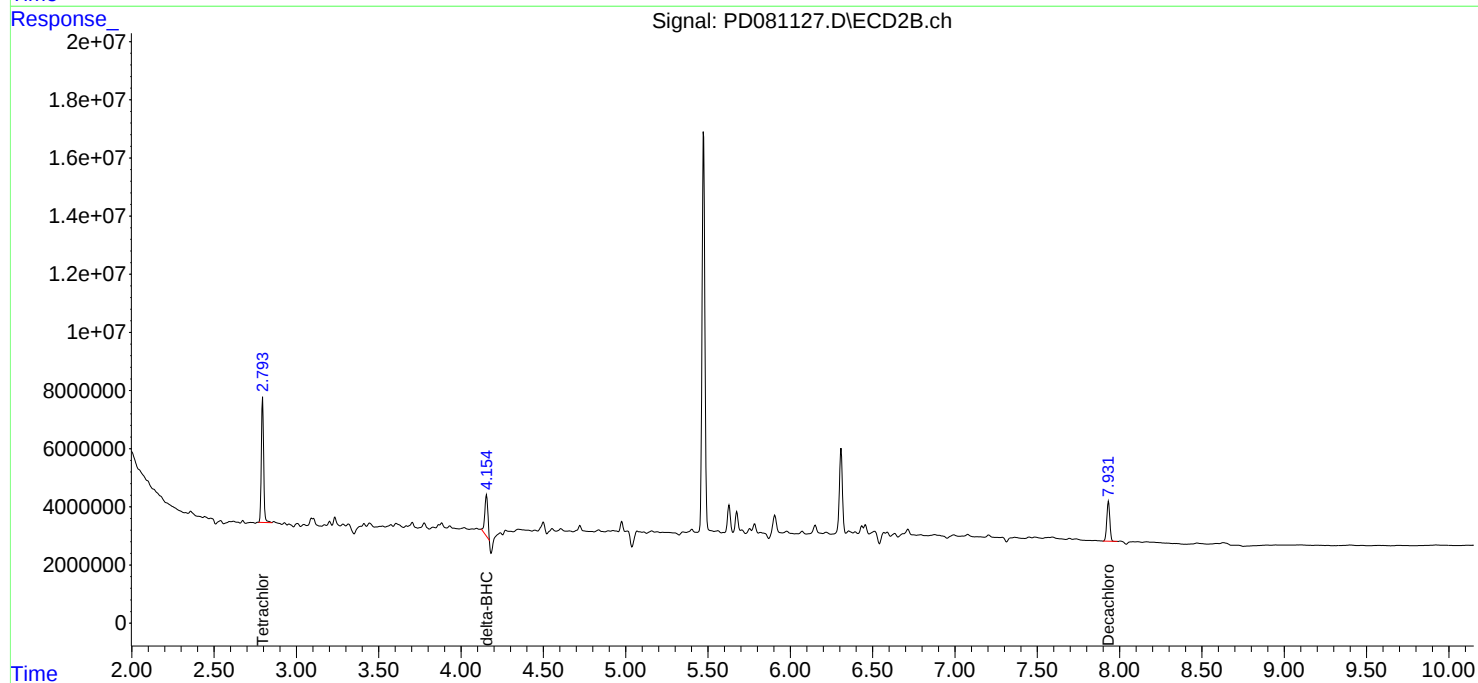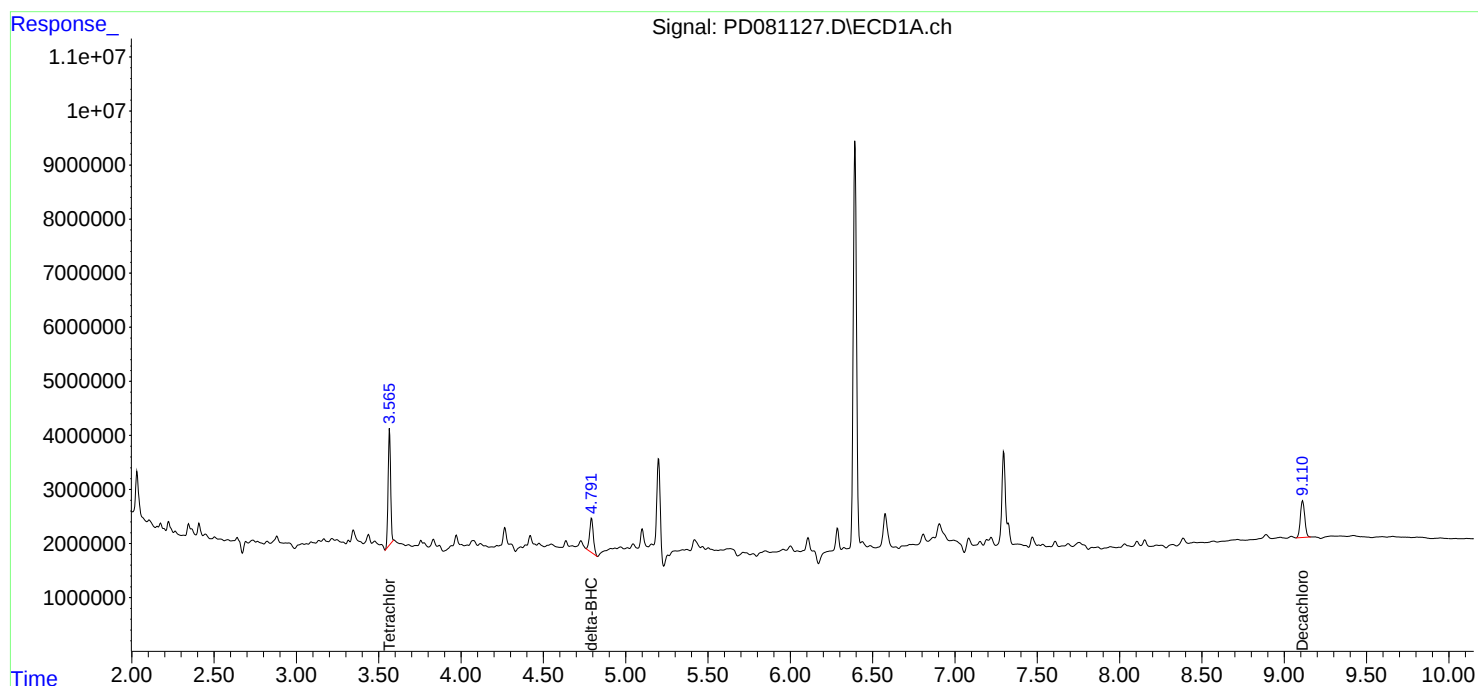

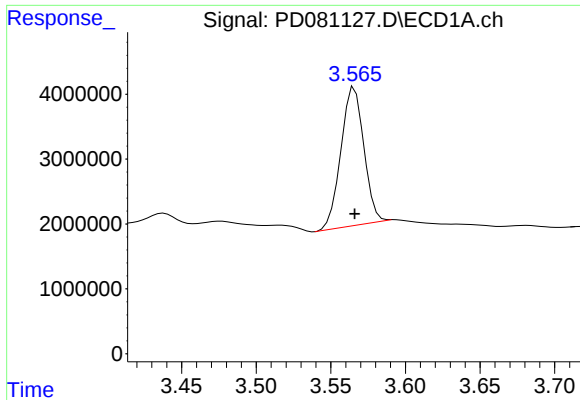


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.002 min
Response: 22969041
Conc: 16.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
MANHOLE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/08/2024
Supervised By :Ankita Jodhani 02/08/2024

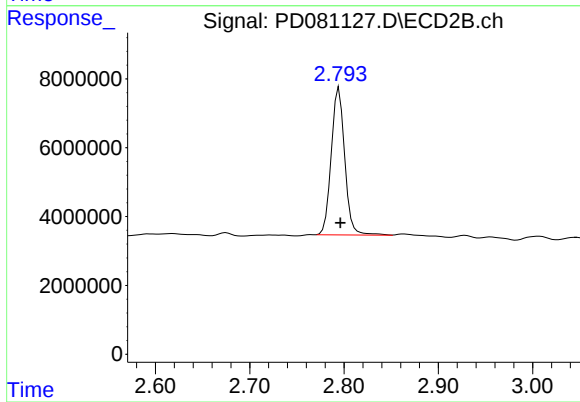


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.001 min
Response: 42469557
Conc: 17.75 ng/ml

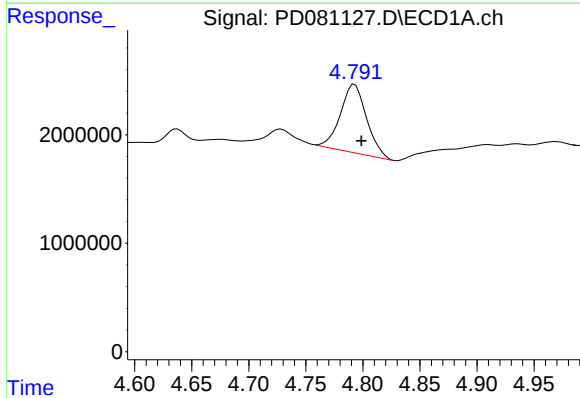


#7 delta-BHC

R.T.: 4.791 min
Delta R.T.: -0.007 min
Response: 10055329
Conc: 4.01 ng/ml m

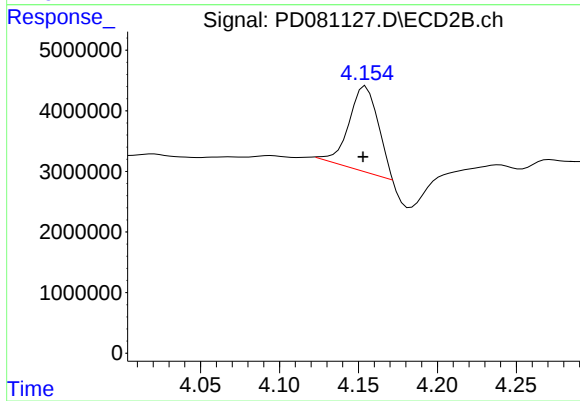

#7 delta-BHC

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 18002616
Conc: 4.80 ng/ml m

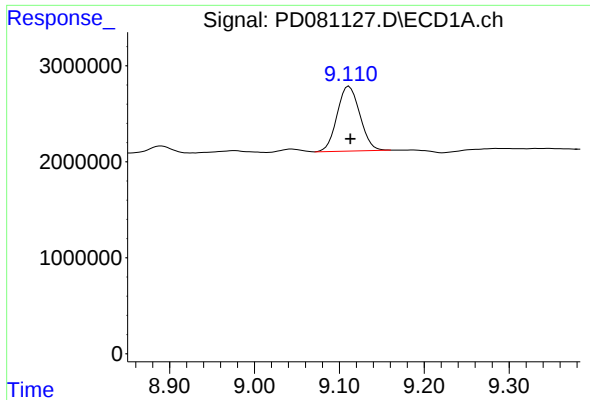


#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.003 min
Response: 12554712
Conc: 6.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
MANHOLE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/08/2024
Supervised By :Ankita Jodhani 02/08/2024

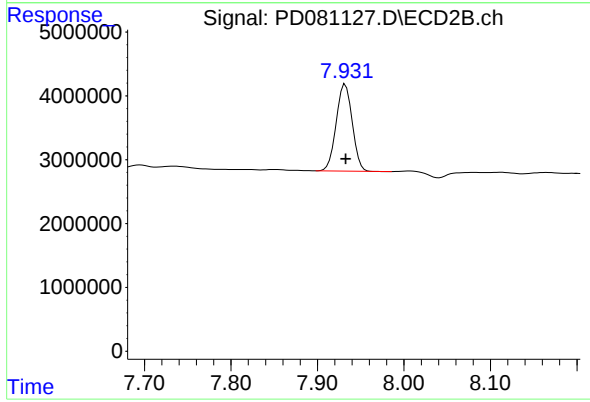

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 17491193
Conc: 6.57 ng/ml