

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020724\
 Data File : PD081157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 10:59
 Operator : AR\AJ
 Sample : PB158860BL
 Misc : CHLOR BS
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB158860BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 20:57:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.795	27997233	47759277	19.722	19.965
28)	SA Decachlor...	9.110	7.931	37318516	45673078	18.544	17.147
Target Compounds							
2)	A alpha-BHC	0.000	3.310	0	72351	N.D.	0.019 #
3)	MA gamma-BHC...	0.000	3.643f	0	311304	N.D.	0.083 #
5)	MB Aldrin	0.000	4.269f	0	134198	N.D.	0.037 #
7)	B delta-BHC	4.791	0.000	775797	0	0.309	N.D. #
10)	B gamma-Chl...	5.944f	0.000	275520	0	0.126	N.D. #
14)	MA Endrin	0.000	5.676f	0	136260	N.D.	0.046 #
15)	B Endosulfa...	6.801f	0.000	1183012	0	0.611	N.D. #
18)	B Endrin al...	0.000	6.147f	0	312456	N.D.	0.139 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020724\
Data File : PD081157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 10:59
Operator : AR\AJ
Sample : PB158860BL
Misc : CHLOR BS
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB158860BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 20:57:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

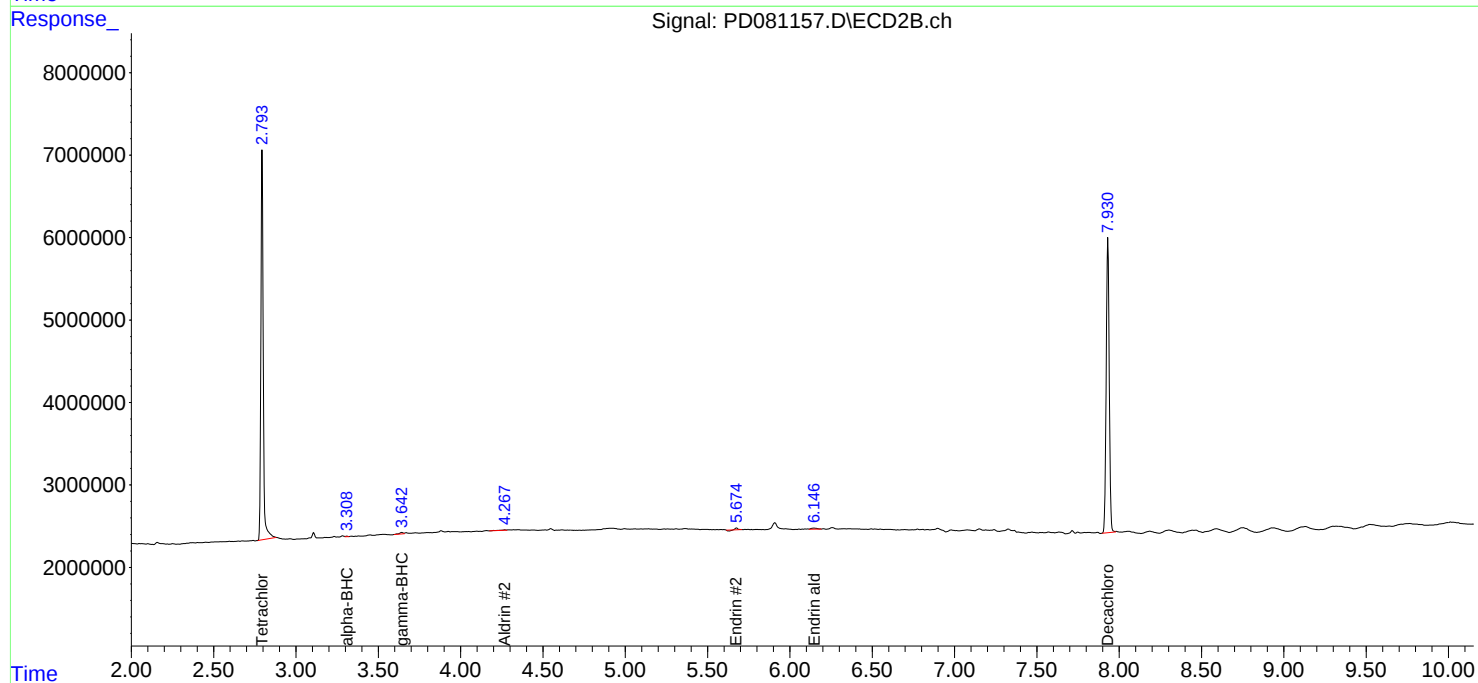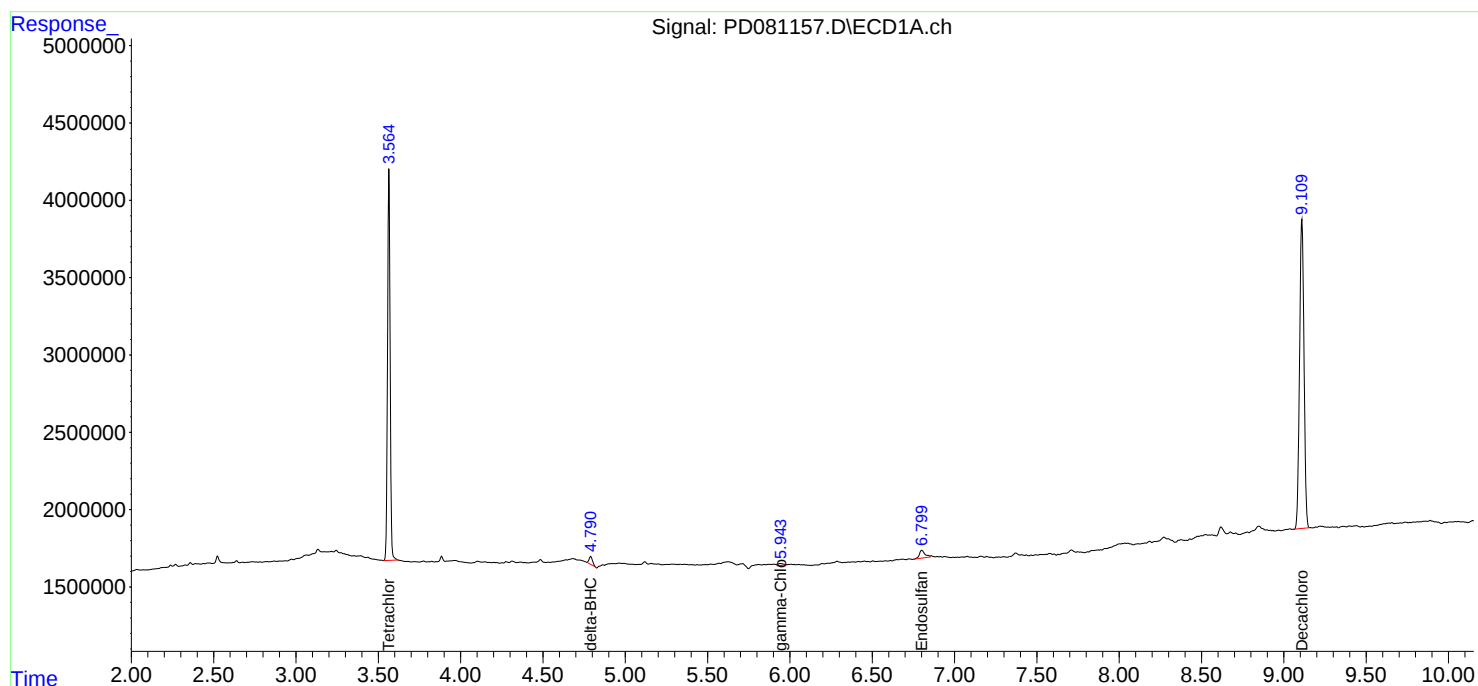


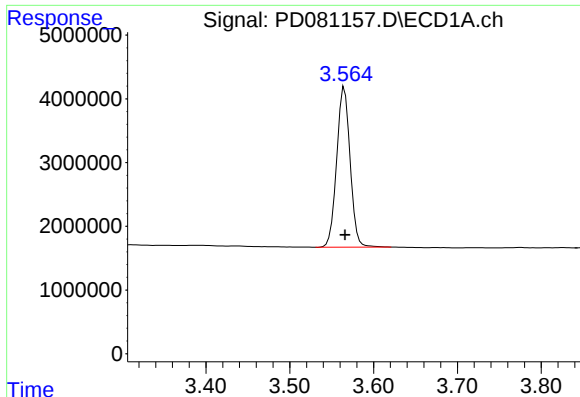

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 27997233
Conc: 19.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158860BL

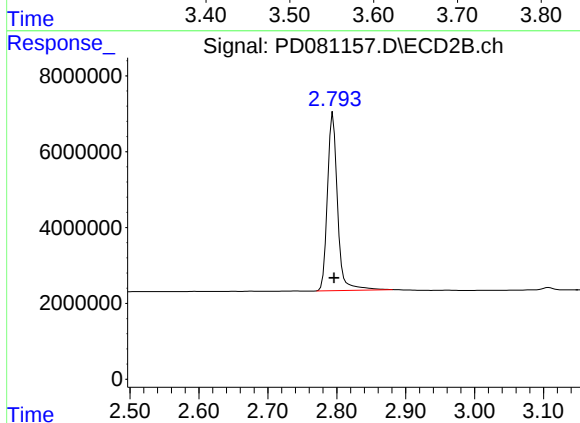


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.001 min
Response: 47759277
Conc: 19.96 ng/ml

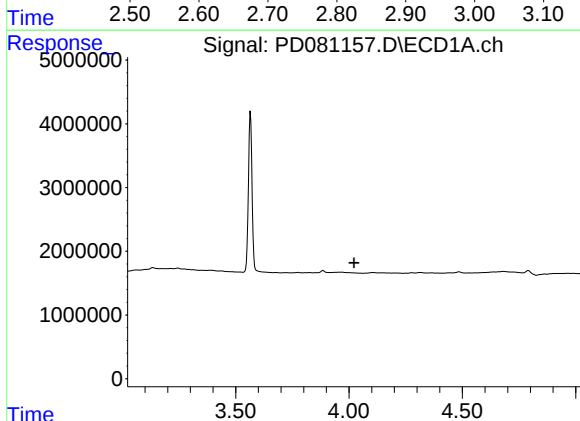


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

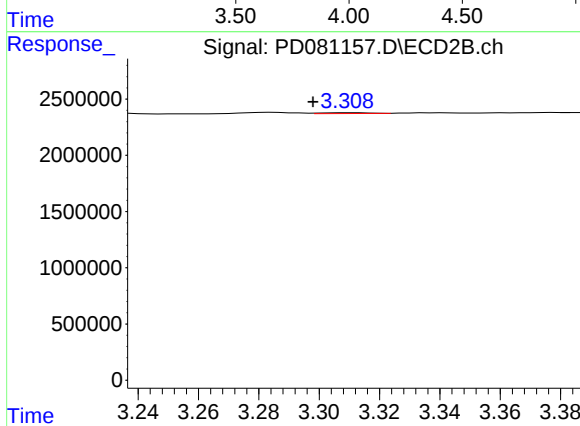

#2 alpha-BHC


R.T.: 3.310 min
Delta R.T.: 0.012 min
Response: 72351
Conc: 0.02 ng/ml

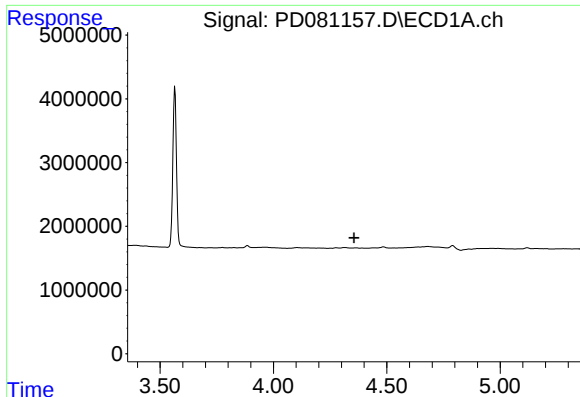

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158860BL

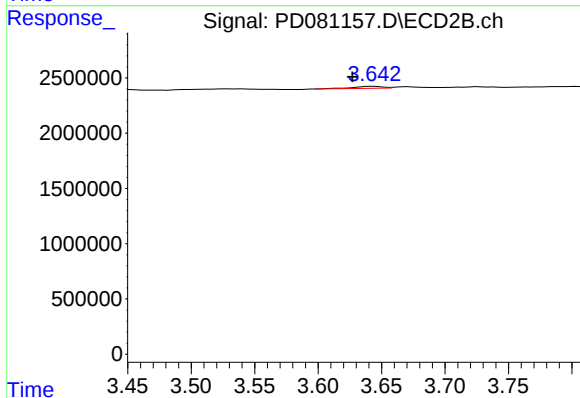


#3 gamma-BHC (Lindane)

R.T.: 3.643 min
Delta R.T.: 0.016 min
Response: 311304
Conc: 0.08 ng/ml

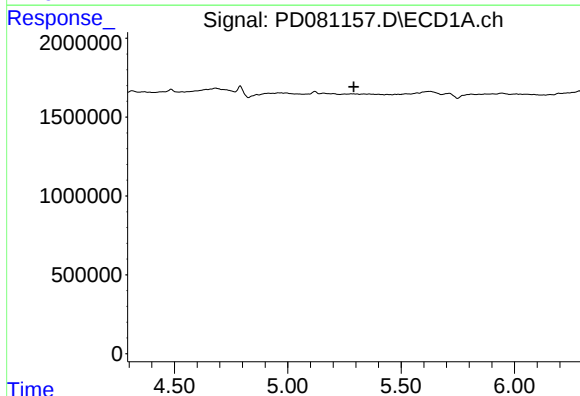


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.292 min
Response: 0
Conc: N.D.

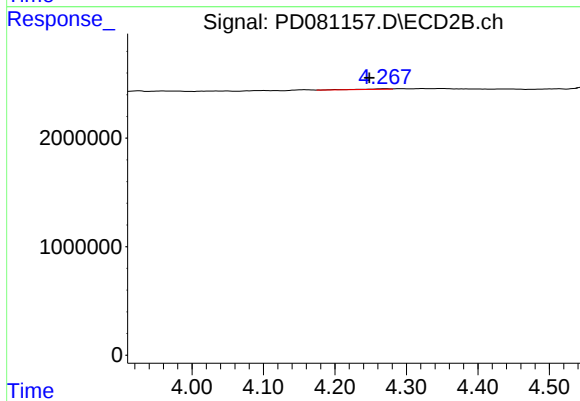

#5 Aldrin


R.T.: 4.269 min
Delta R.T.: 0.020 min
Response: 134198
Conc: 0.04 ng/ml

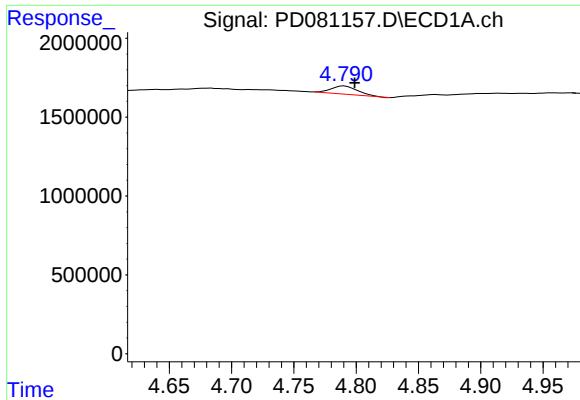

#7 delta-BHC


R.T.: 4.791 min
Delta R.T.: -0.008 min
Response: 775797
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158860BL

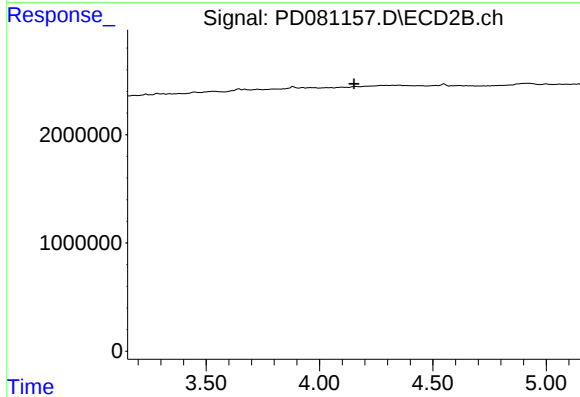


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

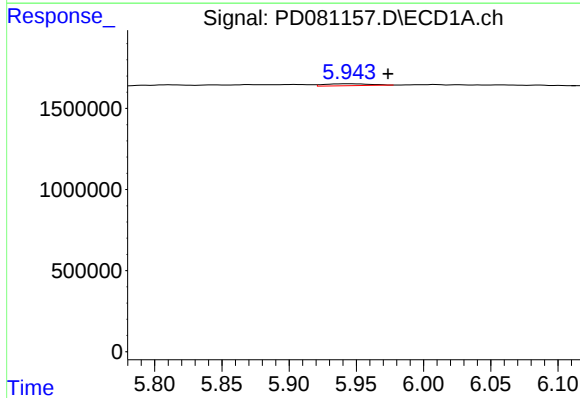


#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.030 min
Response: 275520
Conc: 0.13 ng/ml

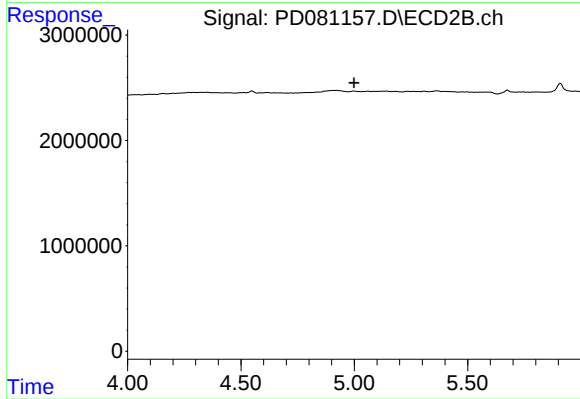

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

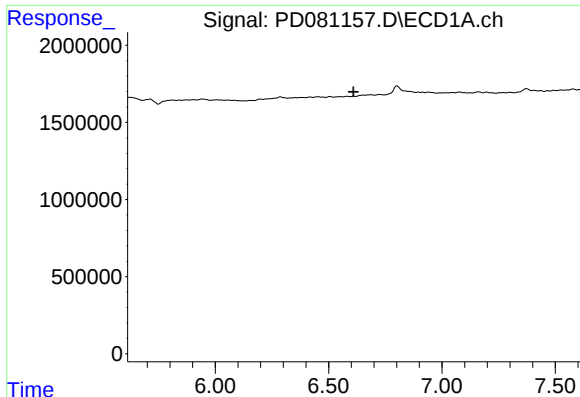

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158860BL

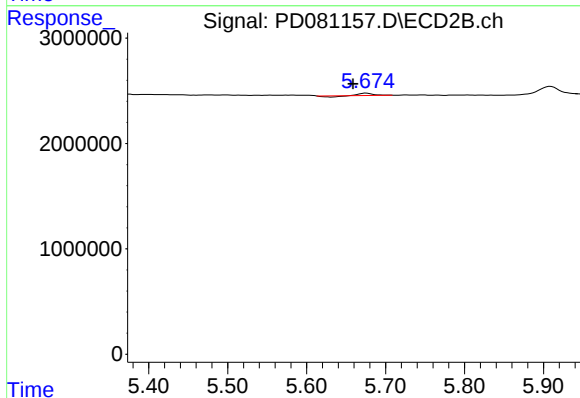


#14 Endrin

R.T.: 5.676 min
Delta R.T.: 0.017 min
Response: 136260
Conc: 0.05 ng/ml

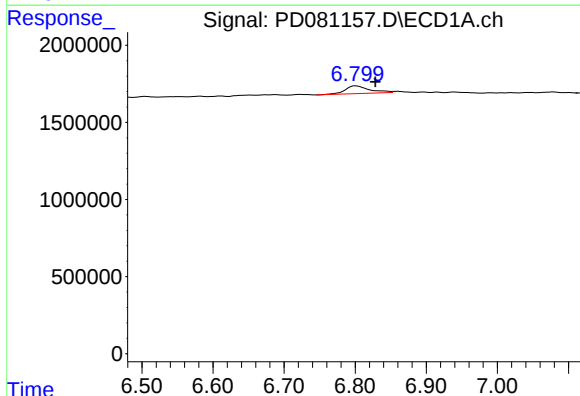


#15 Endosulfan II

R.T.: 6.801 min
Delta R.T.: -0.027 min
Response: 1183012
Conc: 0.61 ng/ml

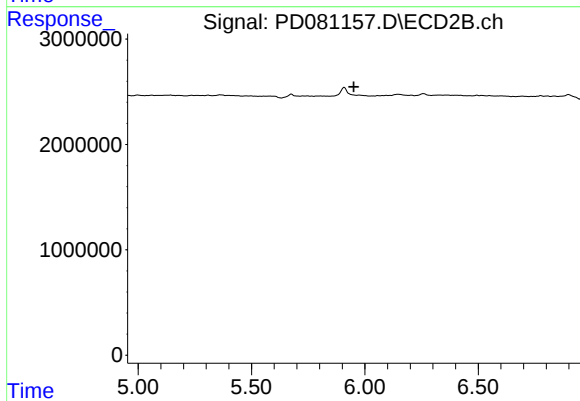

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

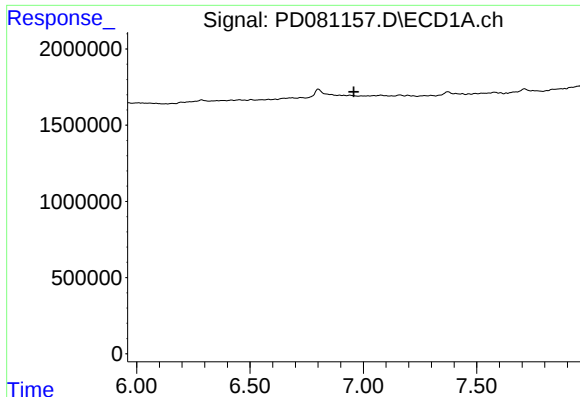

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158860BL

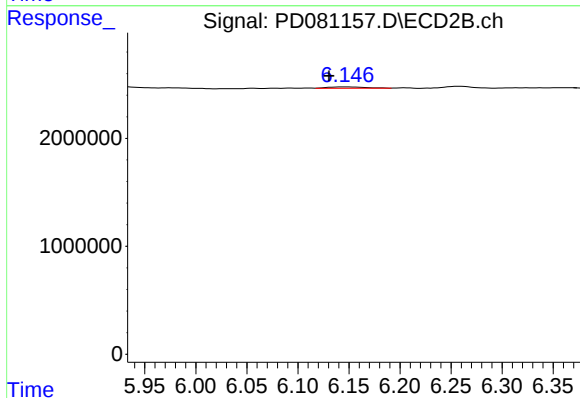


#18 Endrin aldehyde

R.T.: 6.147 min
Delta R.T.: 0.017 min
Response: 312456
Conc: 0.14 ng/ml

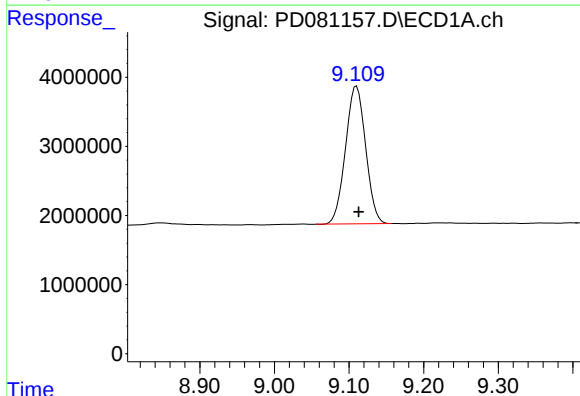

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.003 min
Response: 37318516
Conc: 18.54 ng/ml

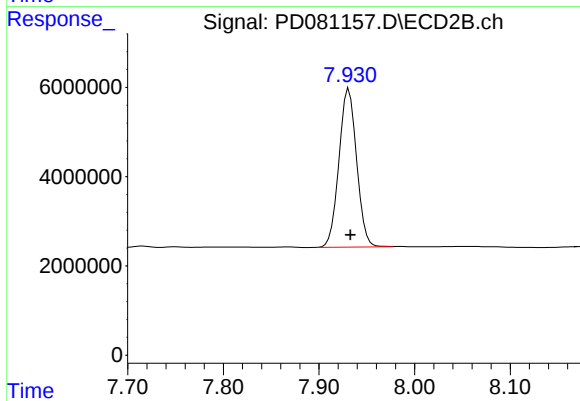

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: -0.002 min
Response: 45673078
Conc: 17.15 ng/ml