

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
 Data File : PD051251.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2019 12:10
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:47:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
 Quant Title : GC Extractables
 QLast Update : Sat Feb 09 00:01:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.225	4.045	29425466	638.5E6	21.278	21.942
28) SA	Decachlor...	7.828	9.159	25872131	408.6E6	22.534	23.134
Target Compounds							
2) A	alpha-BHC	3.667f	4.446	373249	498777	0.177	0.012 #
3) MA	gamma-BHC...	3.926	4.741f	2241714	115830	1.051	0.003 #
4) MA	Heptachlor	0.000	5.246	0	574390	N.D.	0.015 #
8) B	Heptachlo...	0.000	5.922	0	3904135	N.D.	0.128 #
10) B	gamma-Chl...	0.000	6.173	0	1023826	N.D.	0.032 #
25)	Chlordane-3	0.000	6.173	0	1023826	N.D.	0.234 #
27)	Chlordane-5	0.000	7.064	0	501886	N.D.	0.477 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
Data File : PD051251.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2019 12:10
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:47:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
Quant Title : GC Extractables
QLast Update : Sat Feb 09 00:01:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

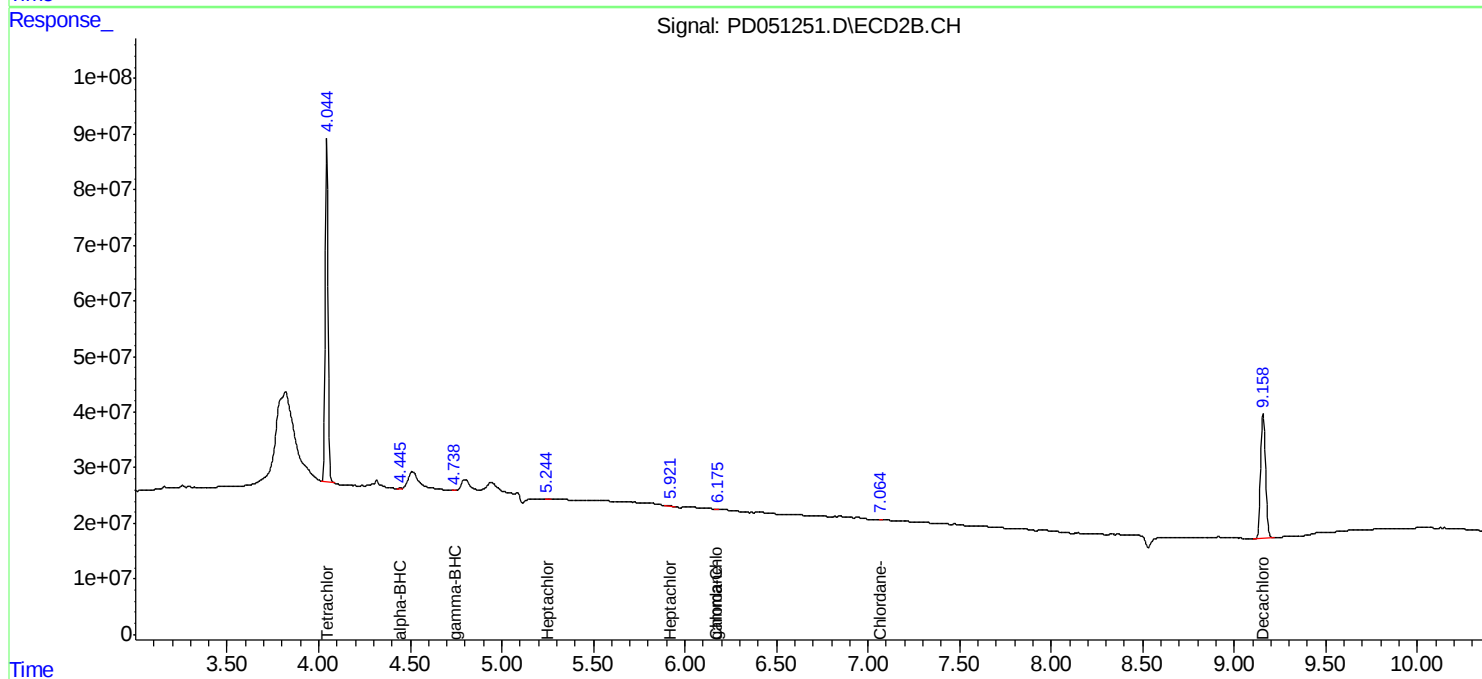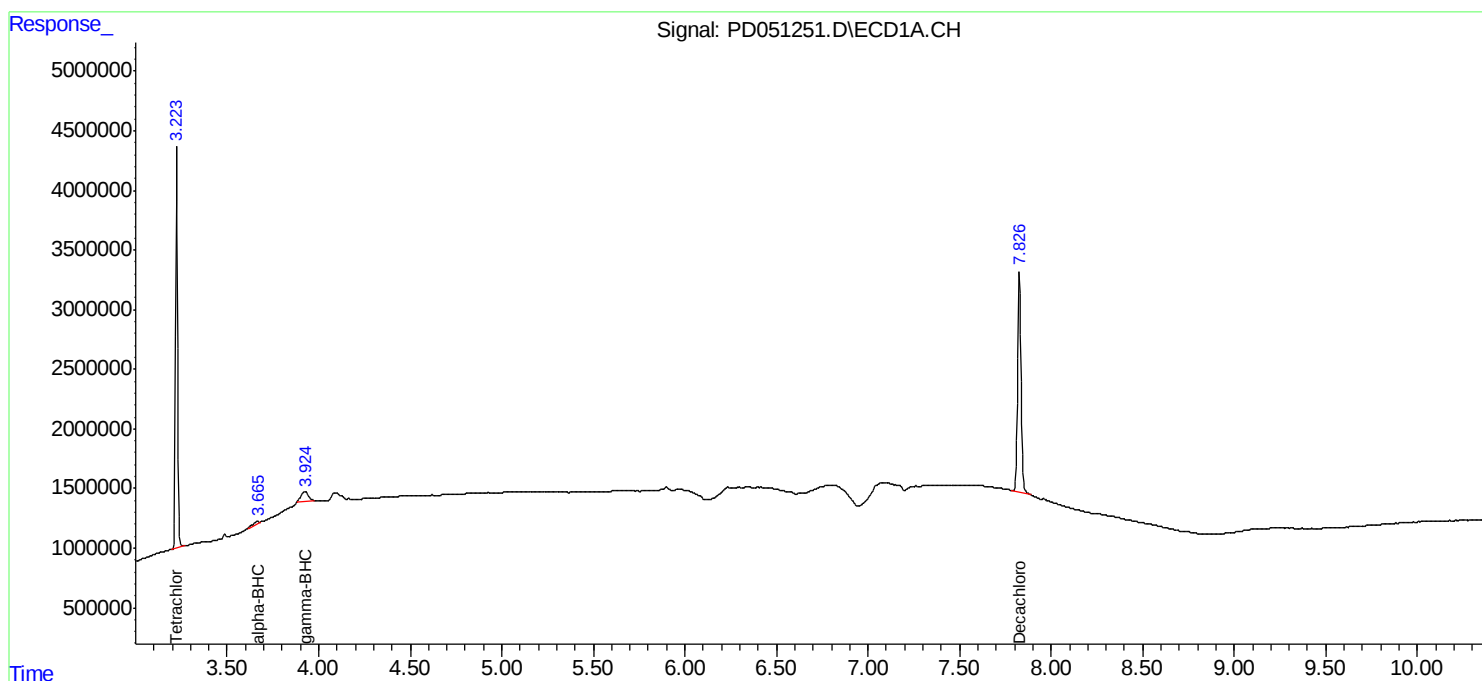


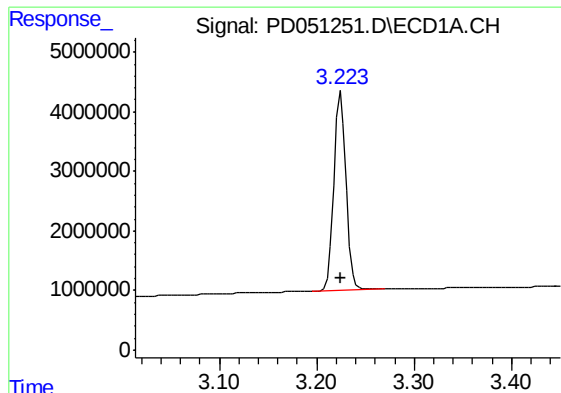

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 29425466
Conc: 21.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

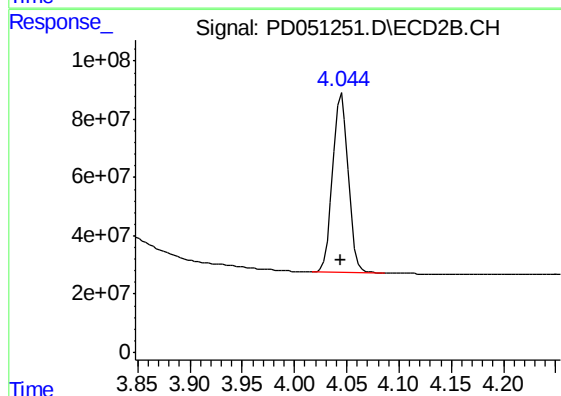


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 638541460
Conc: 21.94 ng/ml

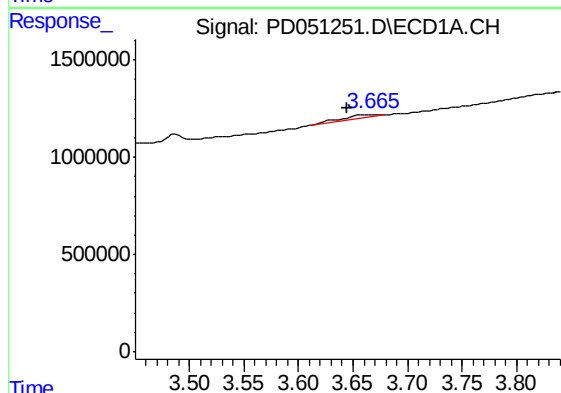


#2 alpha-BHC

R.T.: 3.667 min
Delta R.T.: 0.022 min
Response: 373249
Conc: 0.18 ng/ml

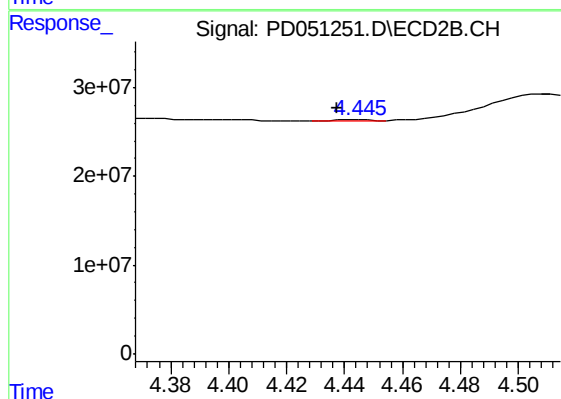

#2 alpha-BHC


R.T.: 4.446 min
Delta R.T.: 0.009 min
Response: 498777
Conc: 0.01 ng/ml

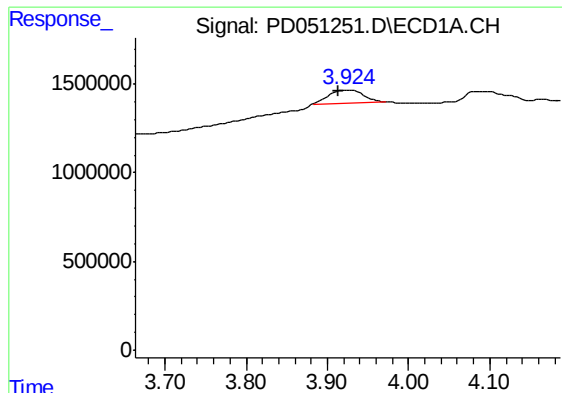

#3 gamma-BHC (Lindane)


R.T.: 3.926 min
Delta R.T.: 0.013 min
Response: 2241714
Conc: 1.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

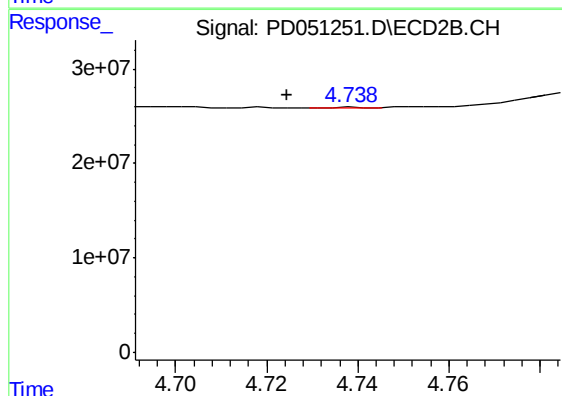


#3 gamma-BHC (Lindane)

R.T.: 4.741 min
Delta R.T.: 0.016 min
Response: 115830
Conc: 0.00 ng/ml

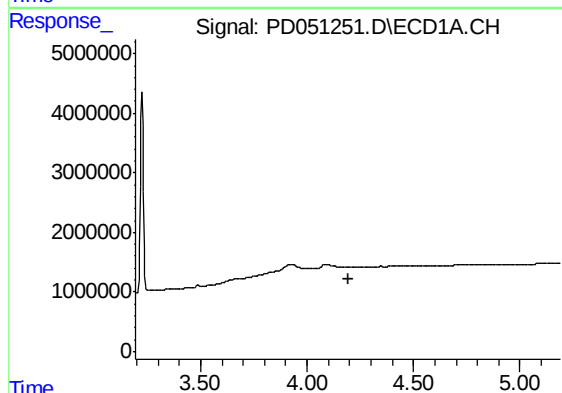


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.192 min
Response: 0
Conc: N.D.

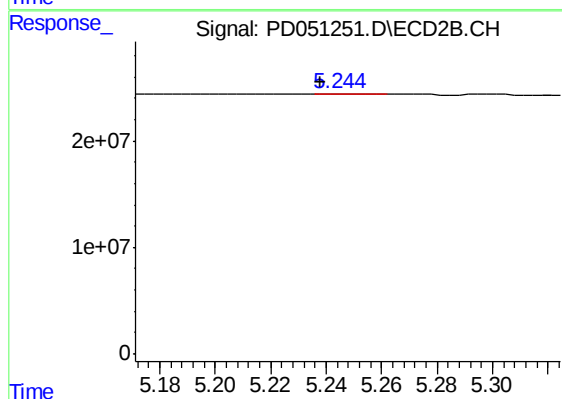

#4 Heptachlor


R.T.: 5.246 min
Delta R.T.: 0.008 min
Response: 574390
Conc: 0.02 ng/ml

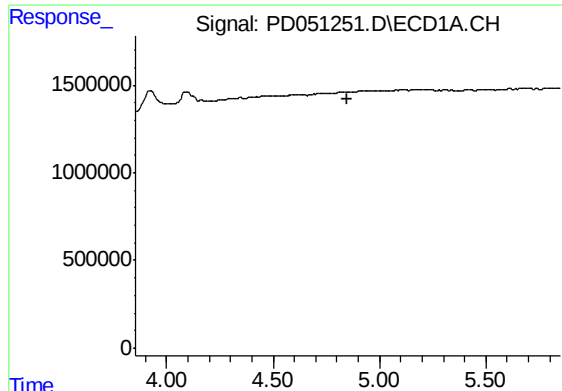

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

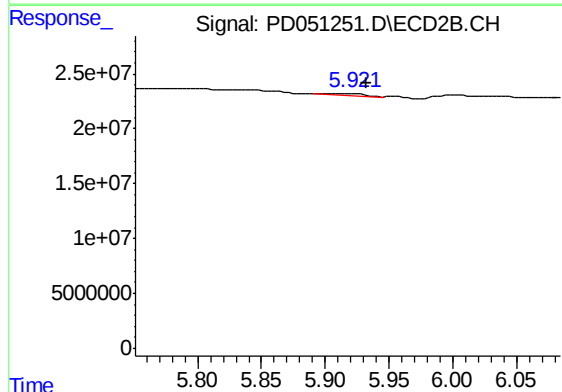


#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.011 min
Response: 3904135
Conc: 0.13 ng/ml

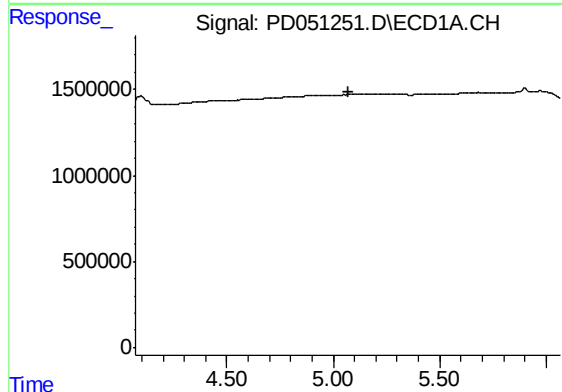


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.069 min
Response: 0
Conc: N.D.

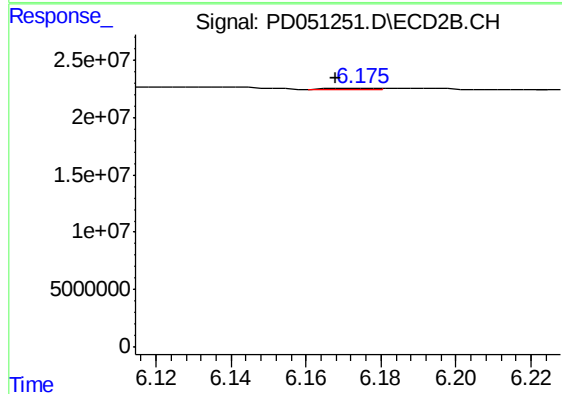

#10 gamma-Chlordane


R.T.: 6.173 min
Delta R.T.: 0.006 min
Response: 1023826
Conc: 0.03 ng/ml

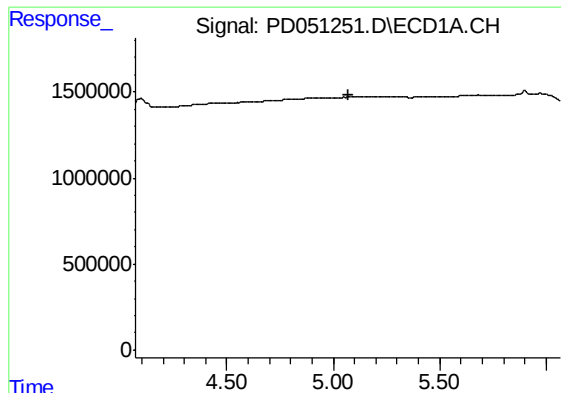

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

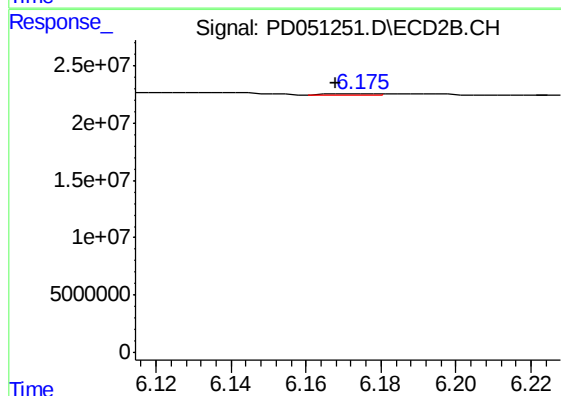


#25 Chlordane-3

R.T.: 6.173 min
Delta R.T.: 0.006 min
Response: 1023826
Conc: 0.23 ng/ml

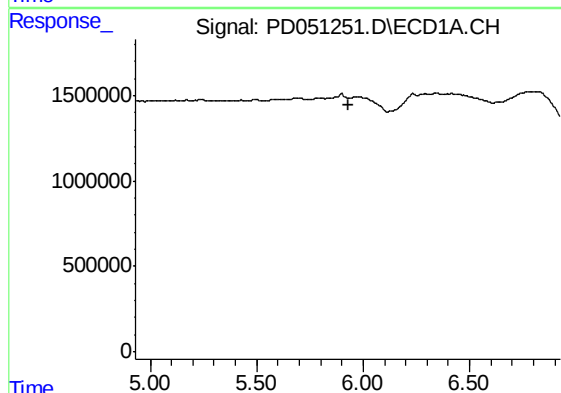


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.930 min
Response: 0
Conc: N.D.

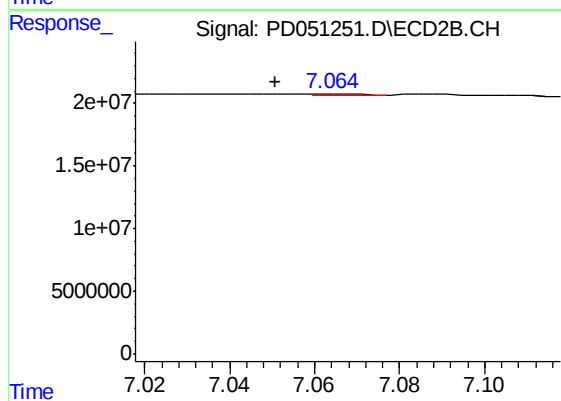

#27 Chlordane-5


R.T.: 7.064 min
Delta R.T.: 0.014 min
Response: 501886
Conc: 0.48 ng/ml

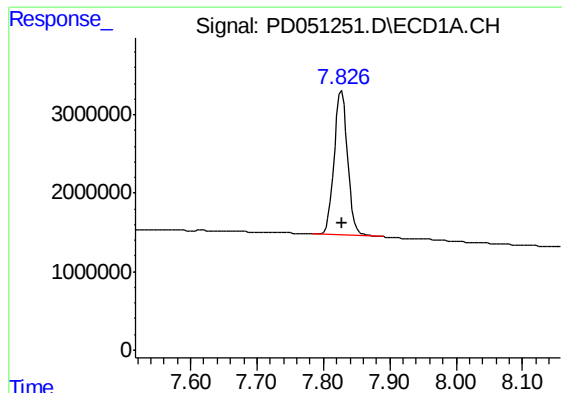

#28 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 25872131
Conc: 22.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

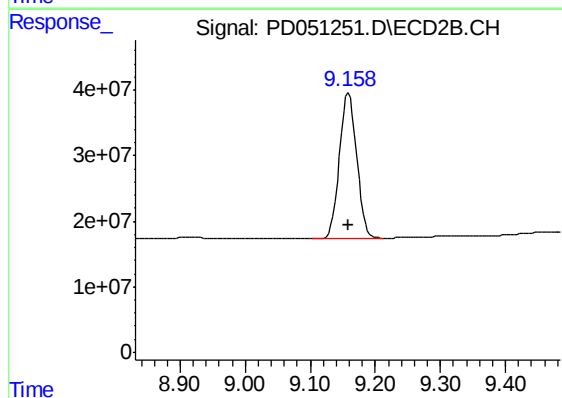

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.000 min
Response: 408590013
Conc: 23.13 ng/ml