

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
 Data File : PD051279.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2019 19:17
 Operator : AJ\SJ
 Sample : PB116942BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB116942BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:56:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
 Quant Title : GC Extractables
 QLast Update : Sat Feb 09 00:01:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	31220092	635.7E6	22.576	21.845
28)	SA Decachlor...	7.827	9.158	26144064	394.9E6	22.771	22.358
Target Compounds							
3)	MA gamma-BHC...	3.920	0.000	2017599	0	0.946	N.D. #
8)	B Heptachlo...	0.000	5.917f	0	3915389	N.D.	0.129 #
10)	B gamma-Chl...	0.000	6.175	0	9271689	N.D.	0.289 #
15)	B Endosulfa...	0.000	6.981	0	10662067	N.D.	0.422 #
18)	B Endrin al...	0.000	7.077f	0	6396753	N.D.	0.301 #
25)	Chlordane-3	0.000	6.175	0	9271689	N.D.	2.115 #
27)	Chlordane-5	0.000	7.055	0	2930090	N.D.	2.788 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
Data File : PD051279.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2019 19:17
Operator : AJ\SJ
Sample : PB116942BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB116942BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:56:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
Quant Title : GC Extractables
QLast Update : Sat Feb 09 00:01:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

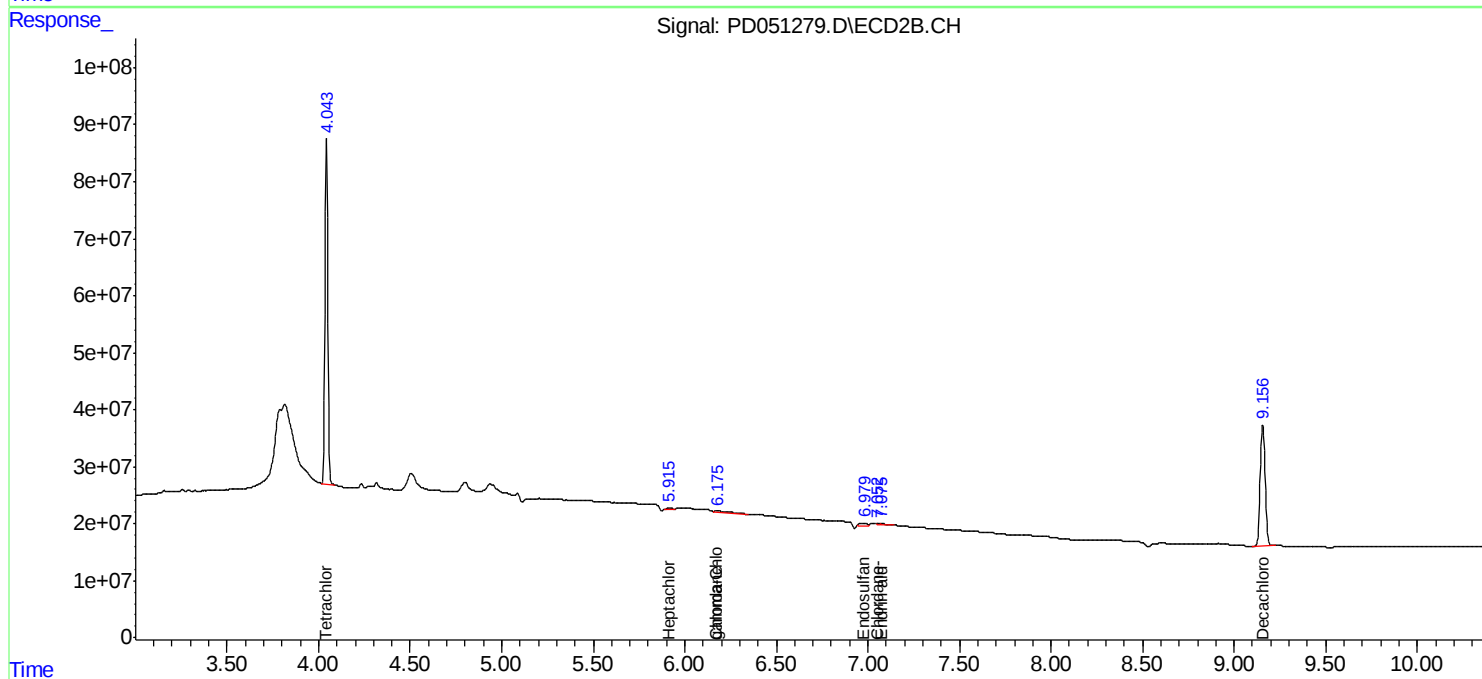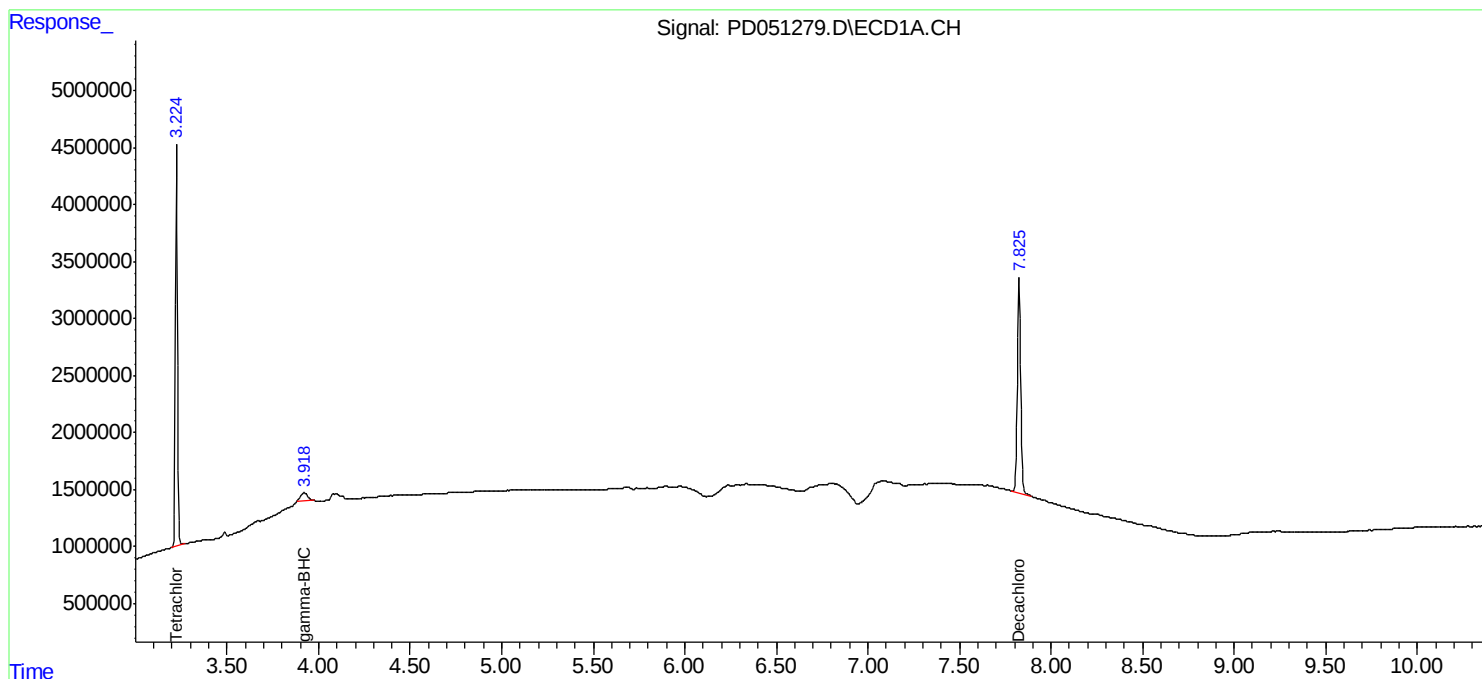


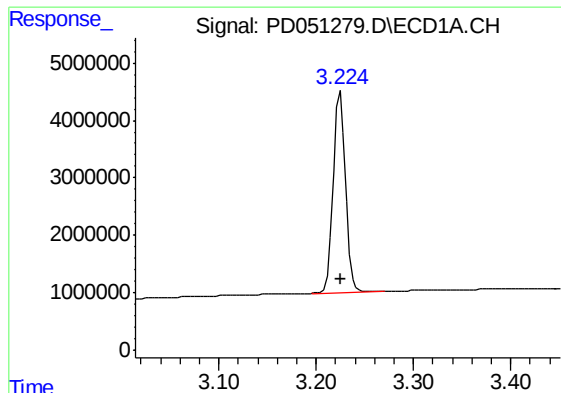

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 31220092
Conc: 22.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB116942BL

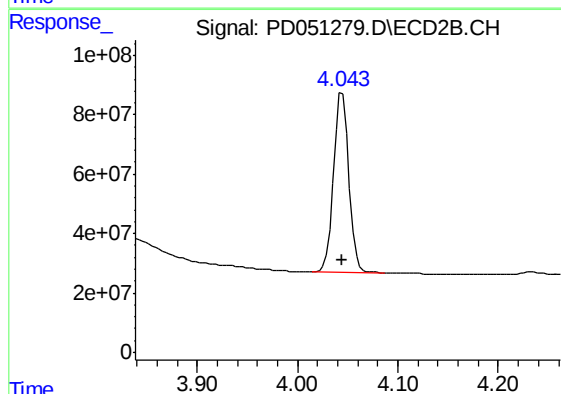


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 635713462
Conc: 21.85 ng/ml

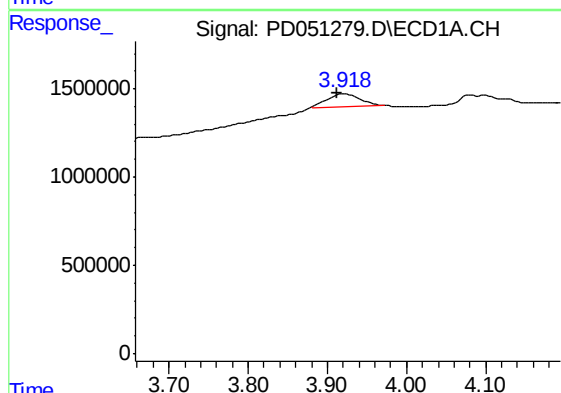


#3 gamma-BHC (Lindane)

R.T.: 3.920 min
Delta R.T.: 0.007 min
Response: 2017599
Conc: 0.95 ng/ml

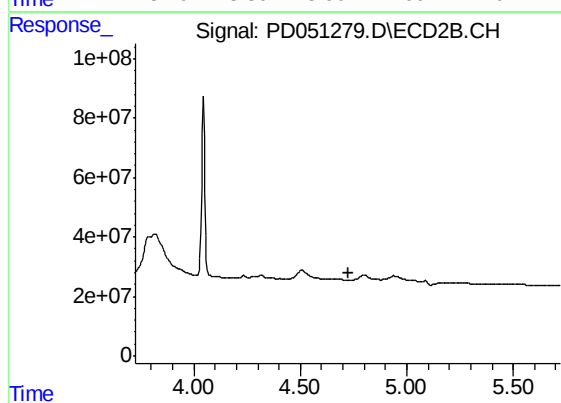

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

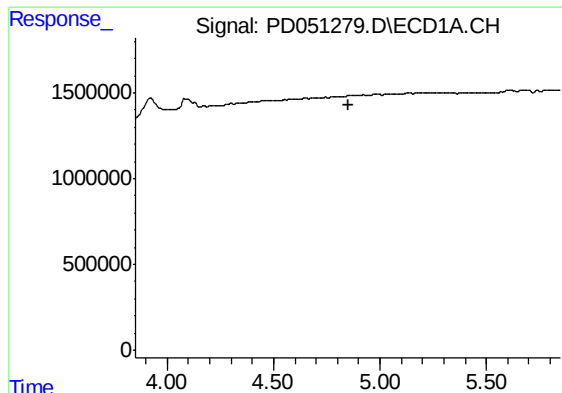

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB116942BL

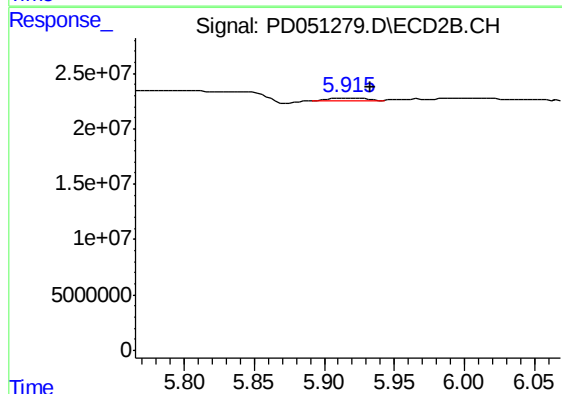


#8 Heptachlor epoxide

R.T.: 5.917 min
Delta R.T.: -0.015 min
Response: 3915389
Conc: 0.13 ng/ml

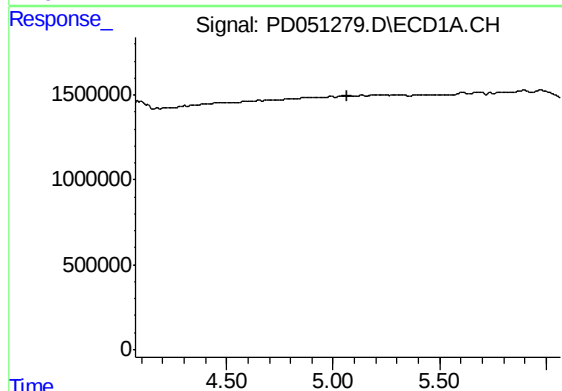


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.069 min
Response: 0
Conc: N.D.

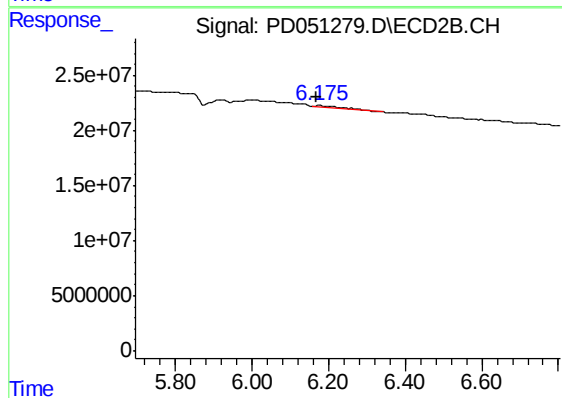

#10 gamma-Chlordane


R.T.: 6.175 min
Delta R.T.: 0.008 min
Response: 9271689
Conc: 0.29 ng/ml

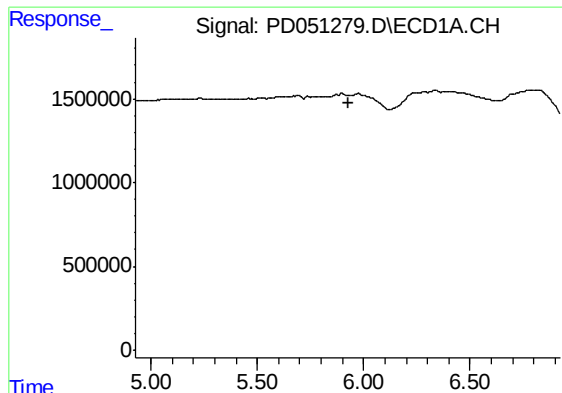

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.926 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB116942BL

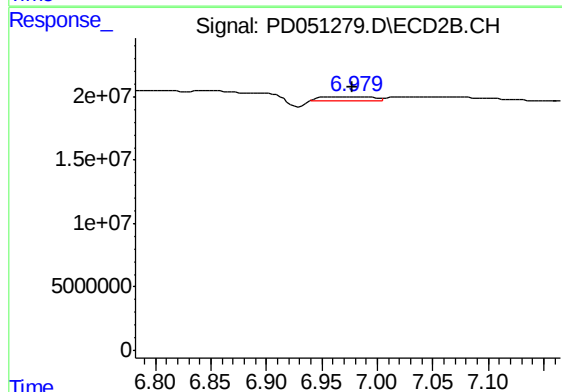


#15 Endosulfan II

R.T.: 6.981 min
Delta R.T.: 0.003 min
Response: 10662067
Conc: 0.42 ng/ml

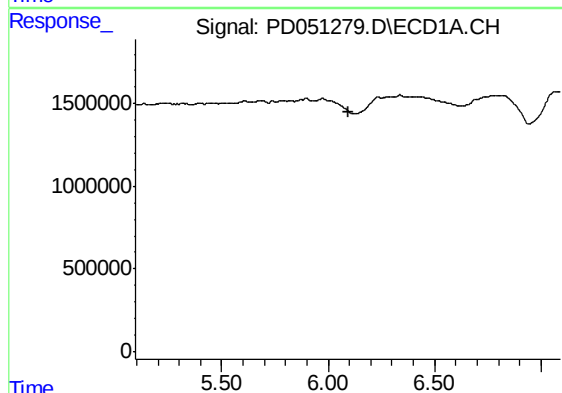


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.093 min
Response: 0
Conc: N.D.

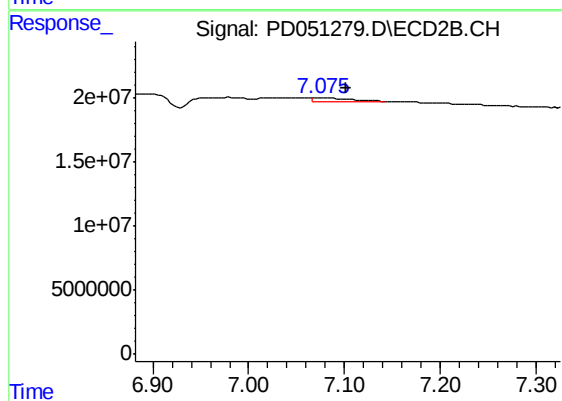

#18 Endrin aldehyde


R.T.: 7.077 min
Delta R.T.: -0.025 min
Response: 6396753
Conc: 0.30 ng/ml

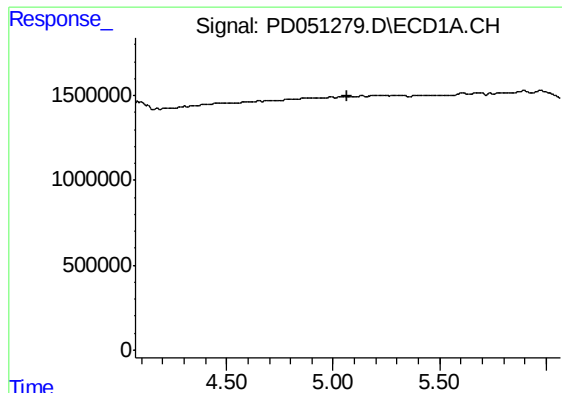

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB116942BL

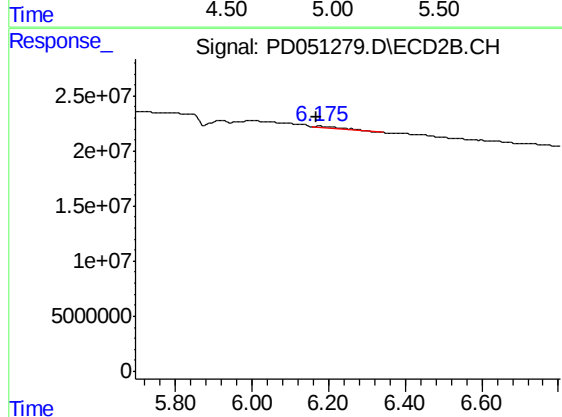


#25 Chlordane-3

R.T.: 6.175 min
Delta R.T.: 0.008 min
Response: 9271689
Conc: 2.11 ng/ml

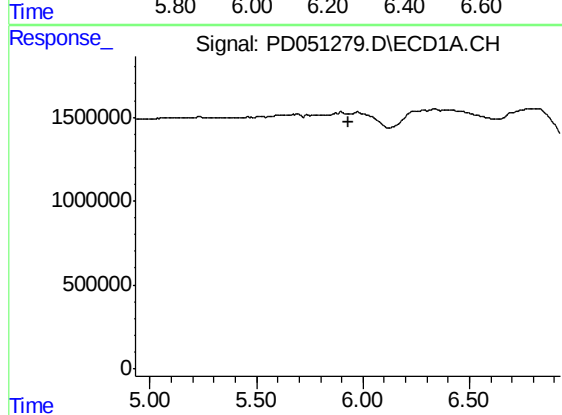


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.930 min
Response: 0
Conc: N.D.

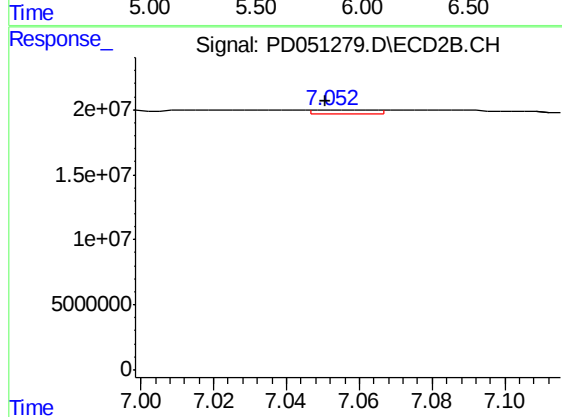

#27 Chlordane-5


R.T.: 7.055 min
Delta R.T.: 0.004 min
Response: 2930090
Conc: 2.79 ng/ml

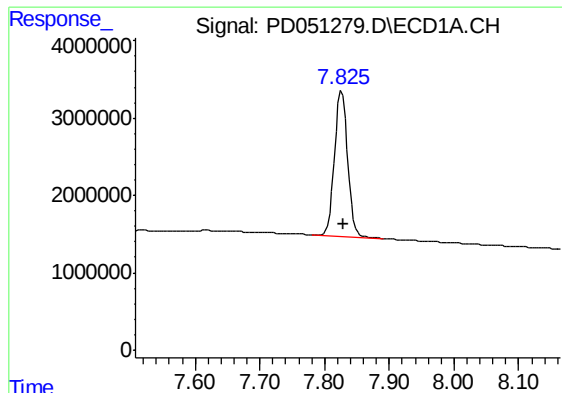

#28 Decachlorobiphenyl

R.T.: 7.827 min
Delta R.T.: -0.002 min
Response: 26144064
Conc: 22.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB116942BL

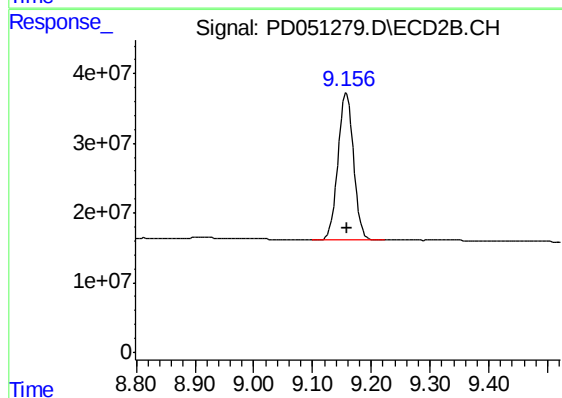

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.000 min
Response: 394879177
Conc: 22.36 ng/ml