

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
 Data File : PD051242.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2019 10:04
 Operator : AJ\SJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:36:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
 Quant Title : GC Extractables
 QLast Update : Sat Feb 09 00:01:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	33987614	724.4E6	24.577	24.894
28)	SA Decachlor...	7.828	9.159	29920840	477.3E6	26.061	27.026
Target Compounds							
9)	A Endosulfan I	5.173	6.292	22984514	402.2E6	12.192	13.935
10)	B gamma-Chl...	5.068	6.168	24435972	437.2E6	11.882	13.609
12)	B 4,4'-DDE	5.294	6.397	47532558	795.7E6	24.735	26.468
13)	MA Dieldrin	5.409	6.551	53104787	824.3E6	25.575	27.125
19)	B Endosulfa...	6.301	7.326	41085946	603.4E6	25.876	26.963
20)	A Methoxychlor	6.574	7.648	108.1E6	1282.4E6	121.601	115.072
21)	B Endrin ke...	6.776	7.801	41972881	526.0E6	21.873	23.054



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
Data File : PD051242.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2019 10:04
Operator : AJ\SJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:36:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
Quant Title : GC Extractables
QLast Update : Sat Feb 09 00:01:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

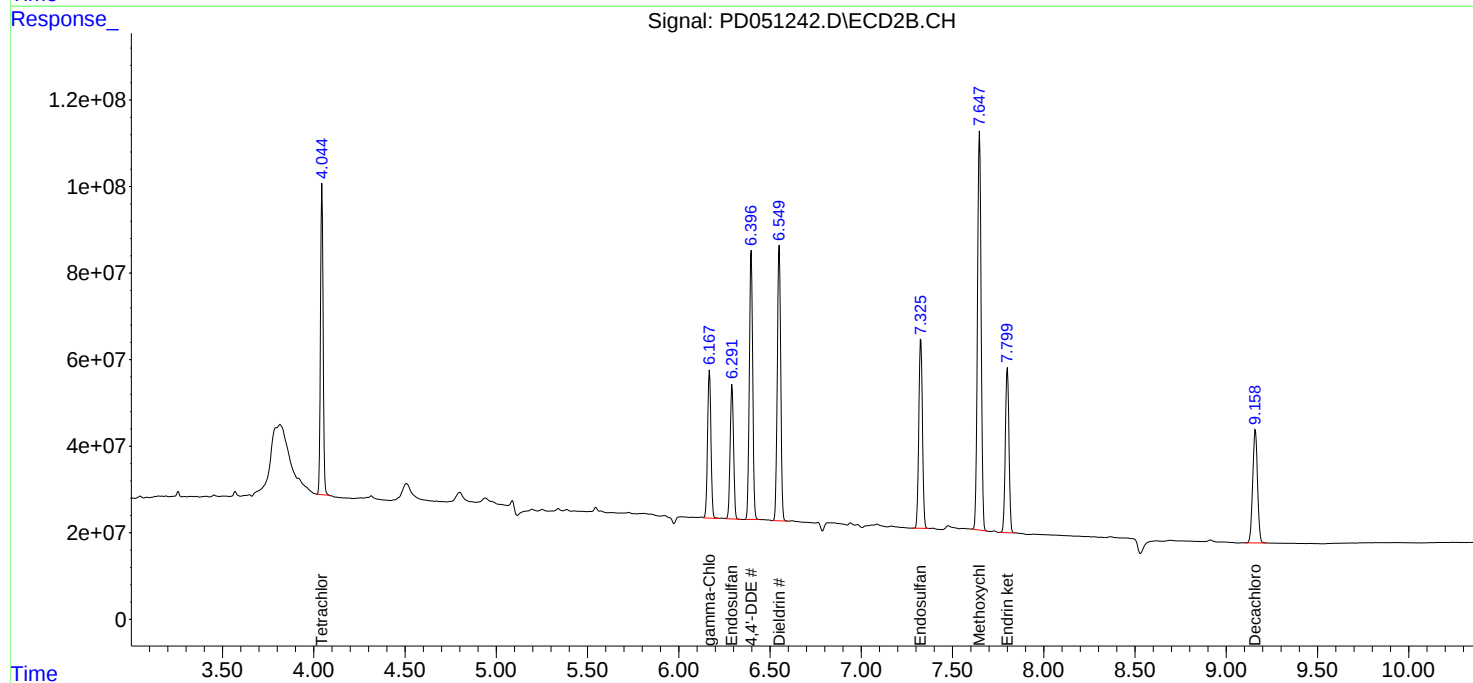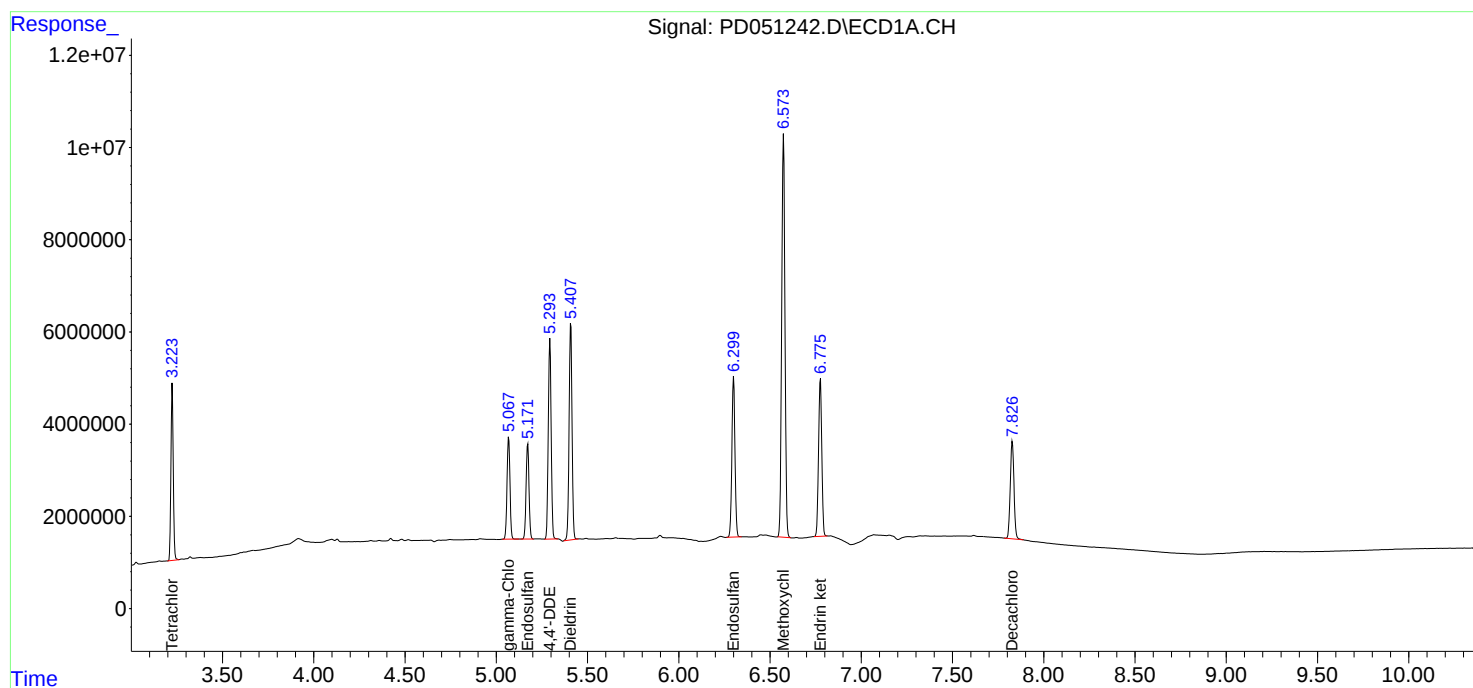


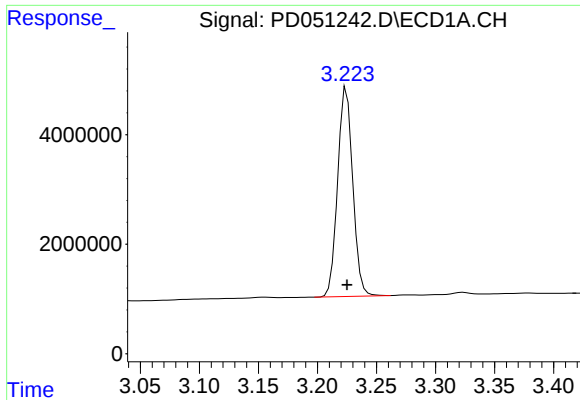

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 33987614
Conc: 24.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

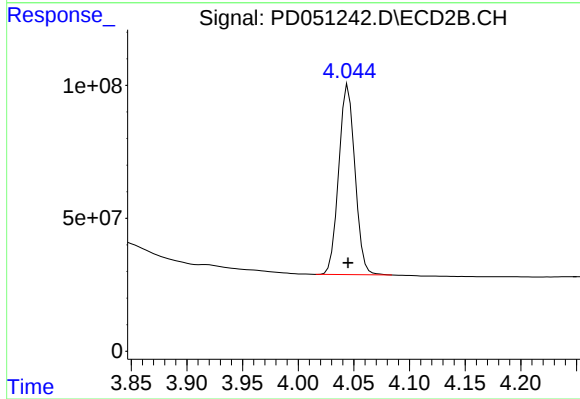


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 724433686
Conc: 24.89 ng/ml

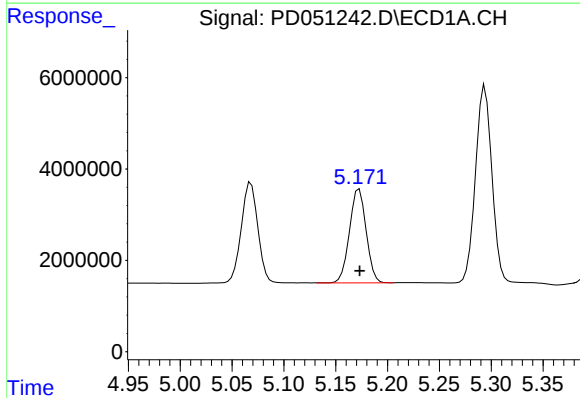


#9 Endosulfan I

R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 22984514
Conc: 12.19 ng/ml

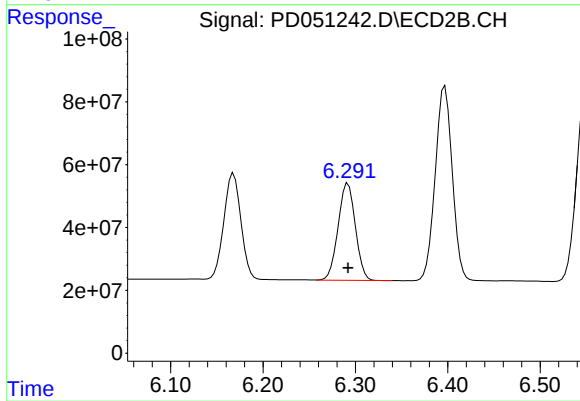

#9 Endosulfan I


R.T.: 6.292 min
Delta R.T.: 0.000 min
Response: 402248372
Conc: 13.94 ng/ml

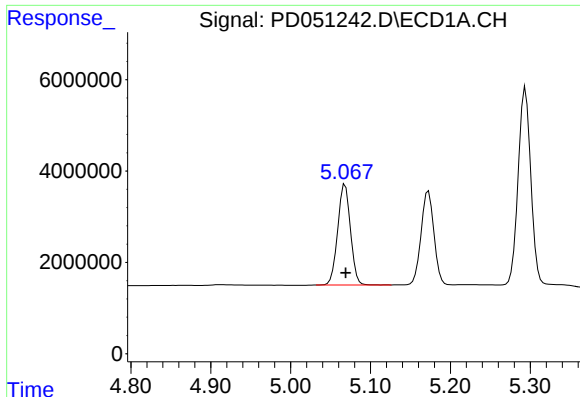

#10 gamma-Chlordane


R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 24435972
Conc: 11.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

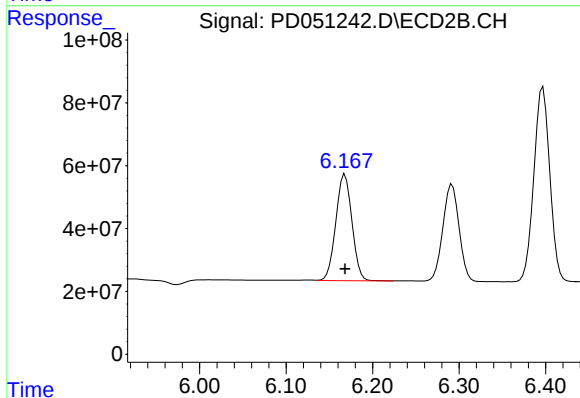


#10 gamma-Chlordane

R.T.: 6.168 min
Delta R.T.: 0.000 min
Response: 437156705
Conc: 13.61 ng/ml

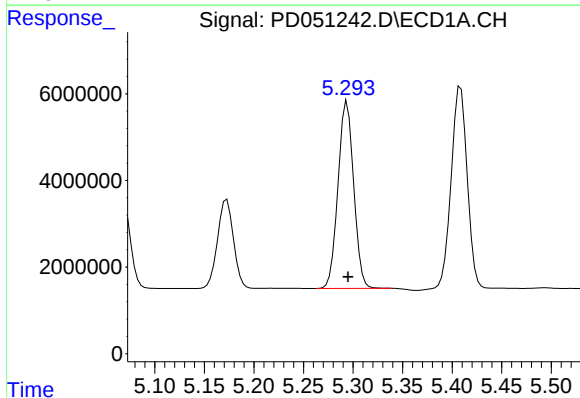


#12 4,4'-DDE

R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 47532558
Conc: 24.74 ng/ml

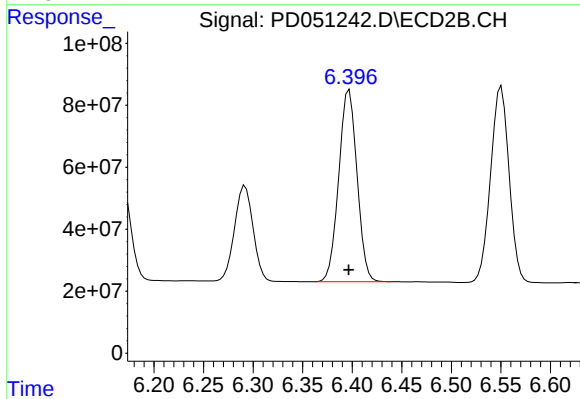

#12 4,4'-DDE


R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 795741100
Conc: 26.47 ng/ml

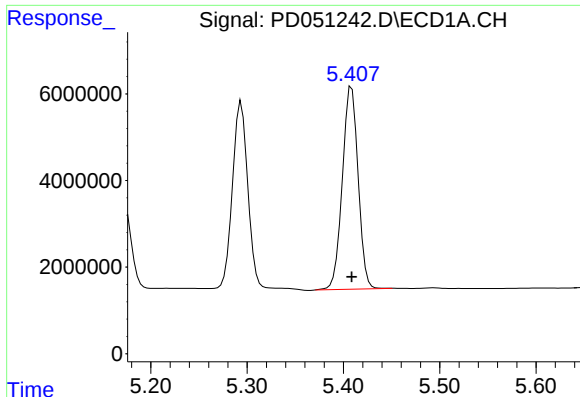

#13 Dieldrin


R.T.: 5.409 min
Delta R.T.: 0.000 min
Response: 53104787
Conc: 25.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

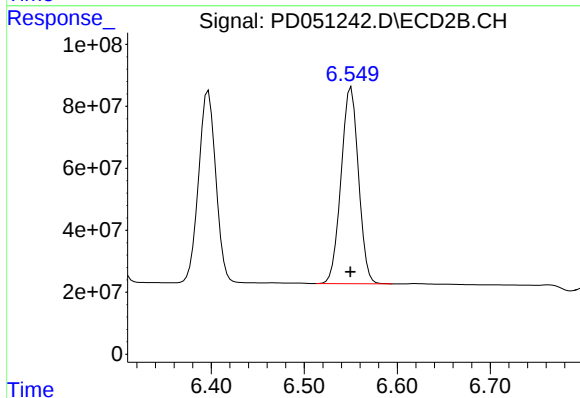


#13 Dieldrin

R.T.: 6.551 min
Delta R.T.: 0.000 min
Response: 824301229
Conc: 27.13 ng/ml

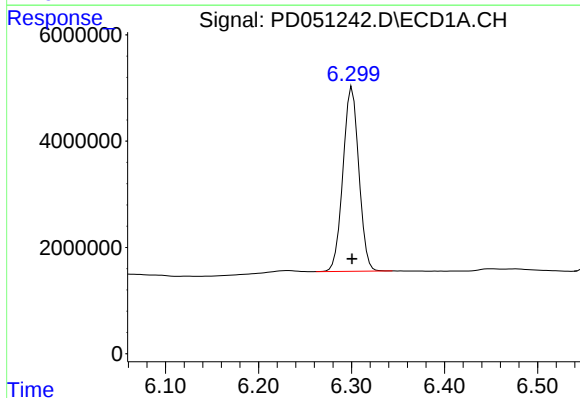


#19 Endosulfan Sulfate

R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 41085946
Conc: 25.88 ng/ml

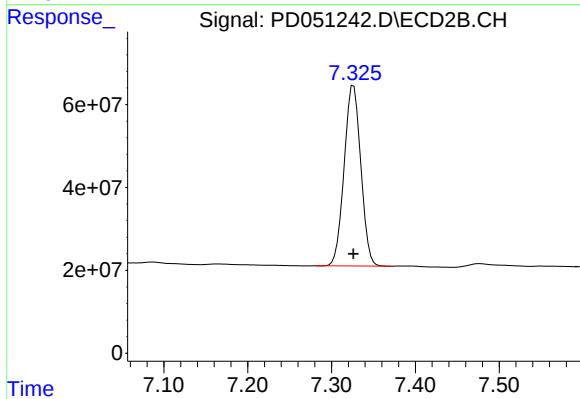

#19 Endosulfan Sulfate


R.T.: 7.326 min
Delta R.T.: 0.000 min
Response: 603378261
Conc: 26.96 ng/ml

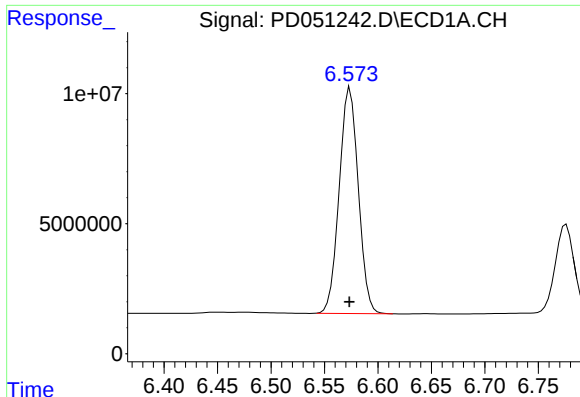

#20 Methoxychlor


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 108080172
Conc: 121.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

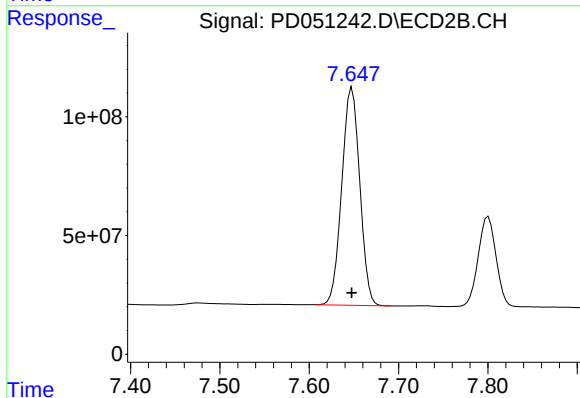


#20 Methoxychlor

R.T.: 7.648 min
Delta R.T.: 0.000 min
Response: 1282363519
Conc: 115.07 ng/ml

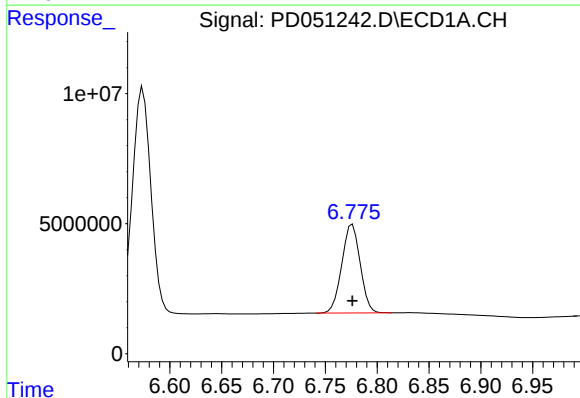


#21 Endrin ketone

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 41972881
Conc: 21.87 ng/ml

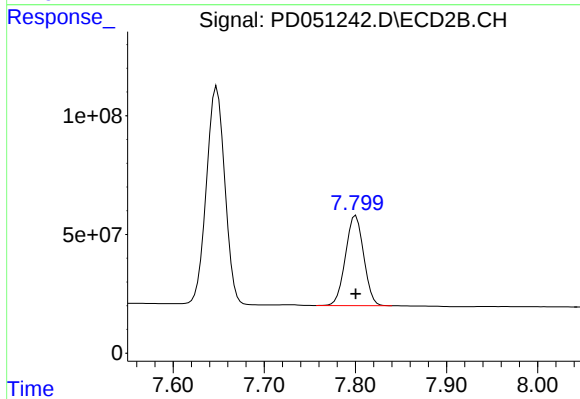

#21 Endrin ketone


R.T.: 7.801 min
Delta R.T.: 0.000 min
Response: 526024908
Conc: 23.05 ng/ml

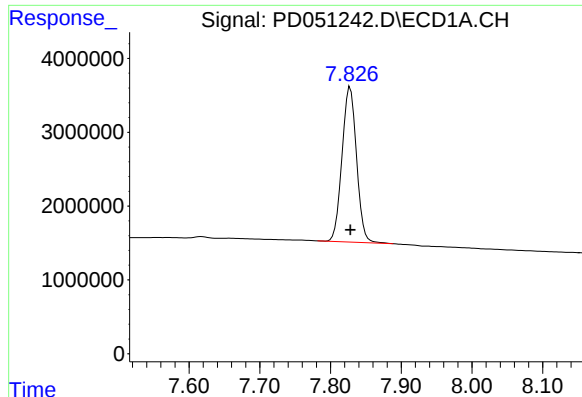

#28 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 29920840
Conc: 26.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

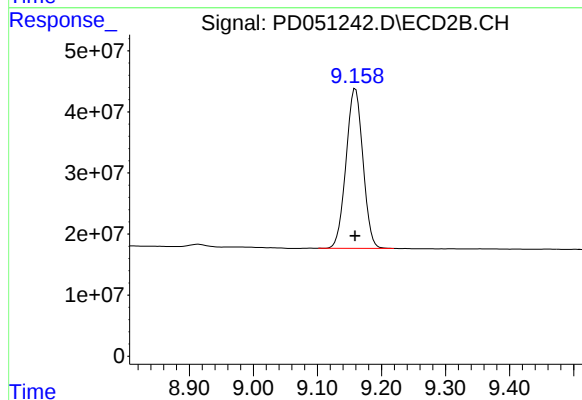

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.000 min
Response: 477333367
Conc: 27.03 ng/ml