

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD020819\  
 Data File : PD051248.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 08 Feb 2019 11:28  
 Operator : AJ\SJ  
 Sample : PCHLORICC500  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 PCHLORICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 08 23:39:15 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD020819.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Feb 08 23:38:27 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 3.225 | 4.045 | 72631762 | 1400.2E6 | 50.000  | 50.000  |
| 28)                         | SA Decachlor... | 7.828 | 9.159 | 55498928 | 864.0E6  | 50.000  | 50.000  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 23)                         | Chlordane-1     | 4.048 | 5.048 | 33009503 | 749.0E6  | 500.000 | 500.000 |
| 24)                         | Chlordane-2     | 4.528 | 5.519 | 38875321 | 675.4E6  | 500.000 | 500.000 |
| 25)                         | Chlordane-3     | 5.069 | 6.168 | 118.8E6  | 2192.2E6 | 500.000 | 500.000 |
| 26)                         | Chlordane-4     | 5.125 | 6.242 | 115.1E6  | 2508.7E6 | 500.000 | 500.000 |
| 27)                         | Chlordane-5     | 5.930 | 7.051 | 37757529 | 525.5E6  | 500.000 | 500.000 |
| -----                       |                 |       |       |          |          |         |         |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD020819\  
Data File : PD051248.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 08 Feb 2019 11:28  
Operator : AJ\SJ  
Sample : PCHLORICC500  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
PCHLORICC500

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 08 23:39:15 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD020819.M  
Quant Title : GC Extractables  
QLast Update : Fri Feb 08 23:38:27 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

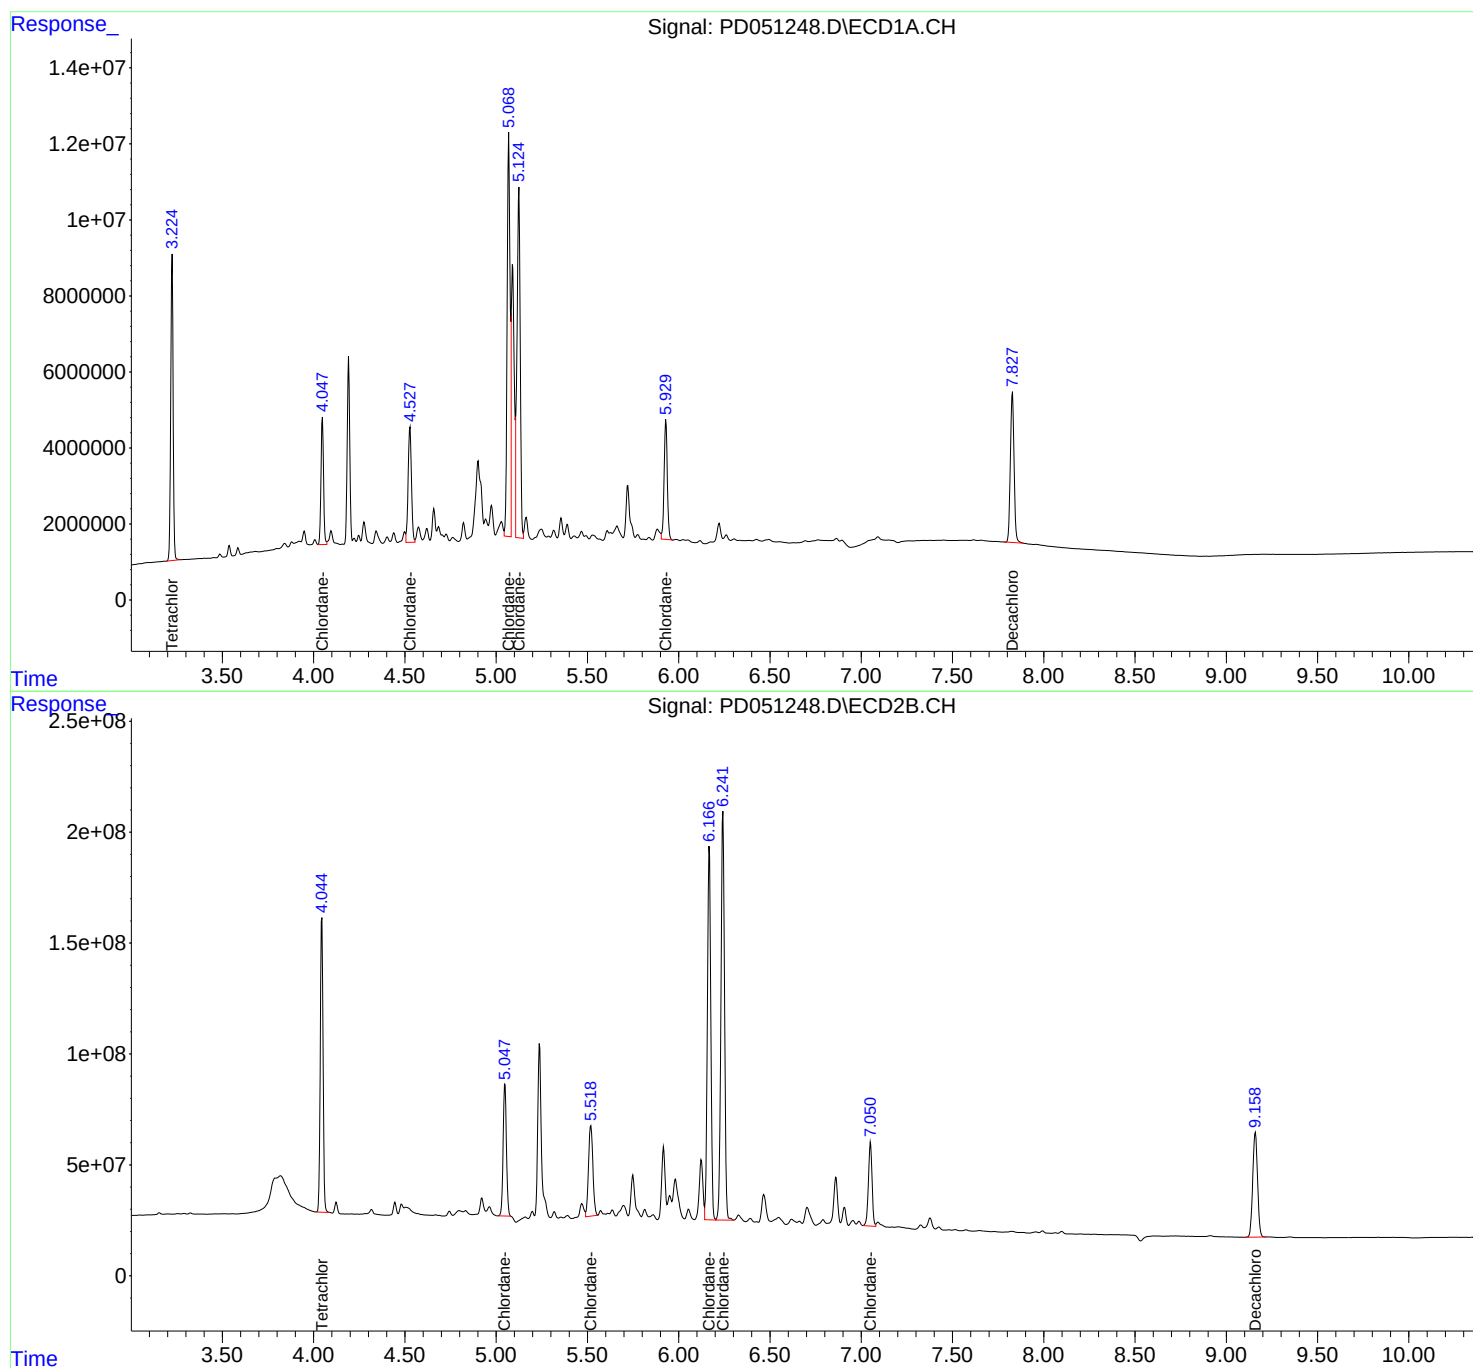


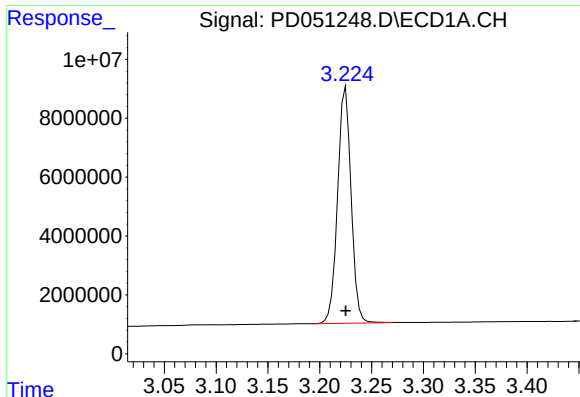

#1 Tetrachloro-m-xylene


R.T.: 3.225 min  
Delta R.T.: 0.000 min  
Response: 72631762  
Conc: 50.00 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PCHLORICC500

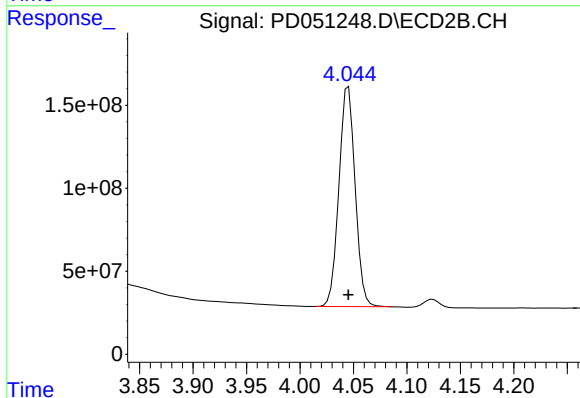


#1 Tetrachloro-m-xylene

R.T.: 4.045 min  
Delta R.T.: 0.000 min  
Response: 1400226532  
Conc: 50.00 ng/ml

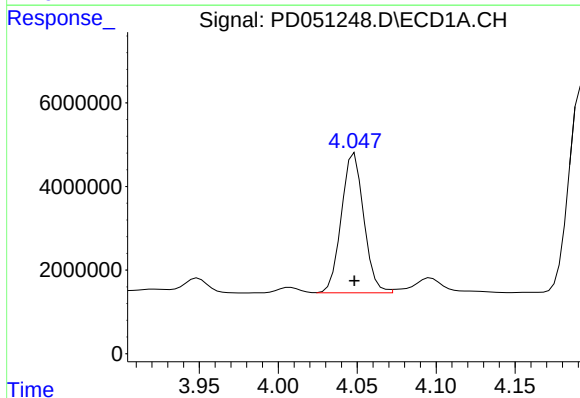


#23 Chlordane-1

R.T.: 4.048 min  
Delta R.T.: 0.000 min  
Response: 33009503  
Conc: 500.00 ng/ml

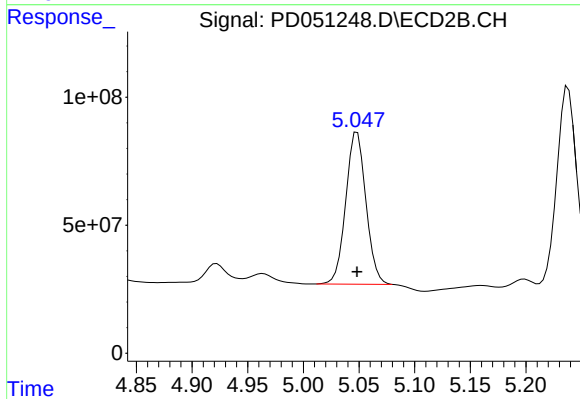

#23 Chlordane-1


R.T.: 5.048 min  
Delta R.T.: 0.000 min  
Response: 748950303  
Conc: 500.00 ng/ml

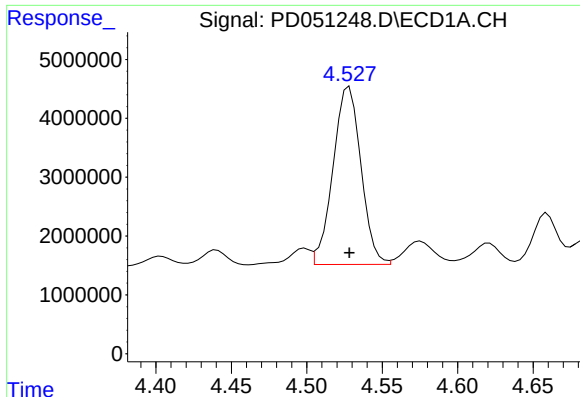

#24 Chlordane-2


R.T.: 4.528 min  
Delta R.T.: 0.000 min  
Response: 38875321  
Conc: 500.00 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PCHLORICC500

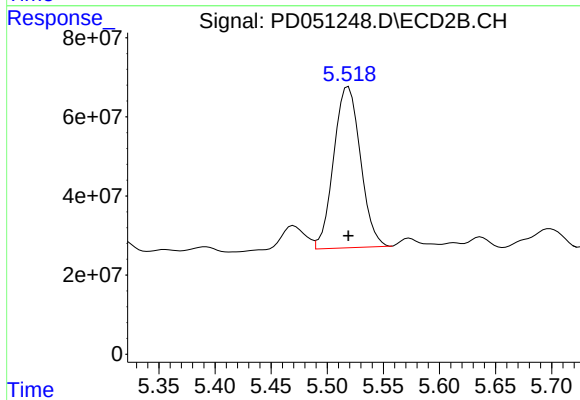


#24 Chlordane-2

R.T.: 5.519 min  
Delta R.T.: 0.000 min  
Response: 675422114  
Conc: 500.00 ng/ml

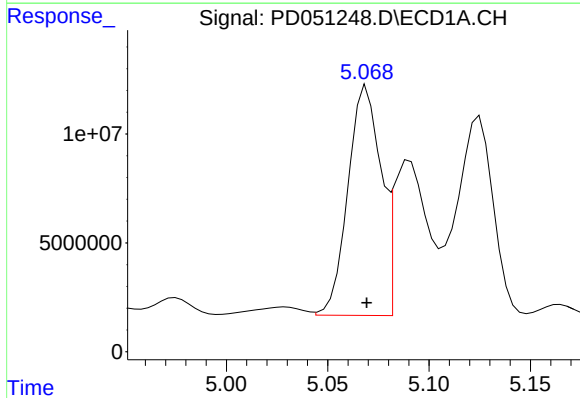


#25 Chlordane-3

R.T.: 5.069 min  
Delta R.T.: 0.000 min  
Response: 118846832  
Conc: 500.00 ng/ml

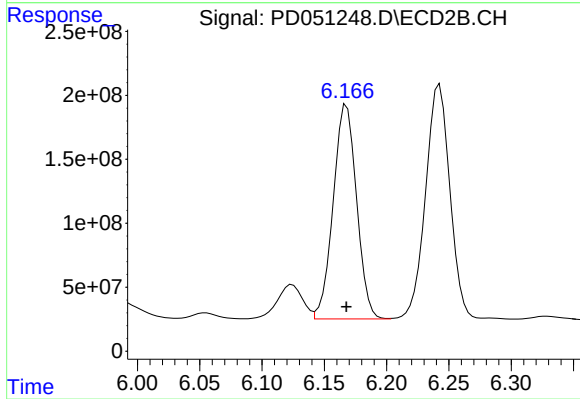

#25 Chlordane-3


R.T.: 6.168 min  
Delta R.T.: 0.000 min  
Response: 2192156216  
Conc: 500.00 ng/ml

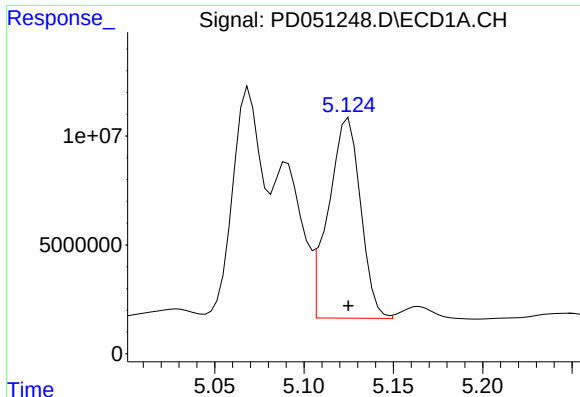

#26 Chlordane-4


R.T.: 5.125 min  
Delta R.T.: 0.000 min  
Response: 115063557  
Conc: 500.00 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PCHLORICC500

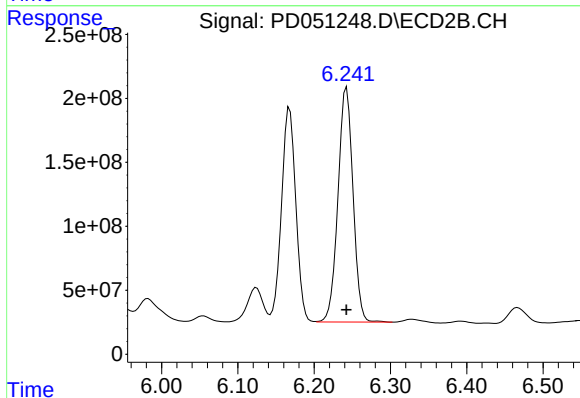


#26 Chlordane-4

R.T.: 6.242 min  
Delta R.T.: 0.000 min  
Response: 2508712480  
Conc: 500.00 ng/ml

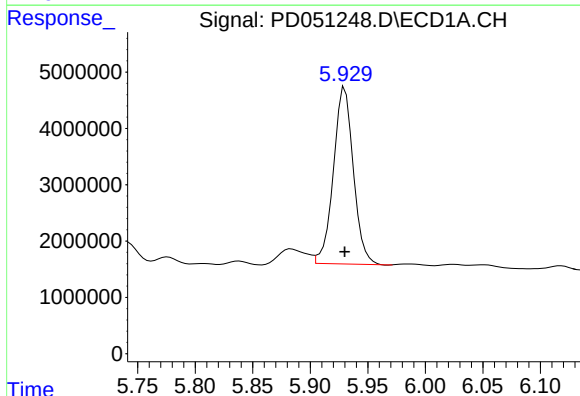


#27 Chlordane-5

R.T.: 5.930 min  
Delta R.T.: 0.000 min  
Response: 37757529  
Conc: 500.00 ng/ml

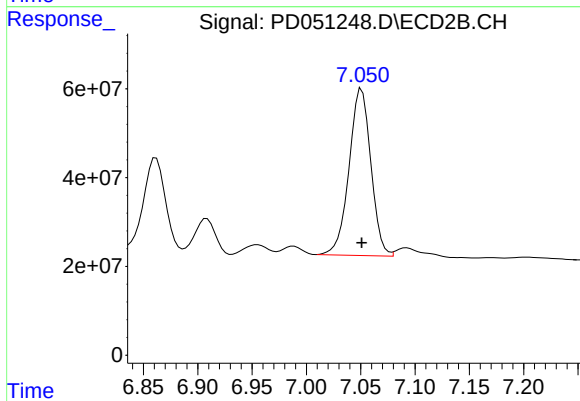

#27 Chlordane-5


R.T.: 7.051 min  
Delta R.T.: 0.000 min  
Response: 525548874  
Conc: 500.00 ng/ml

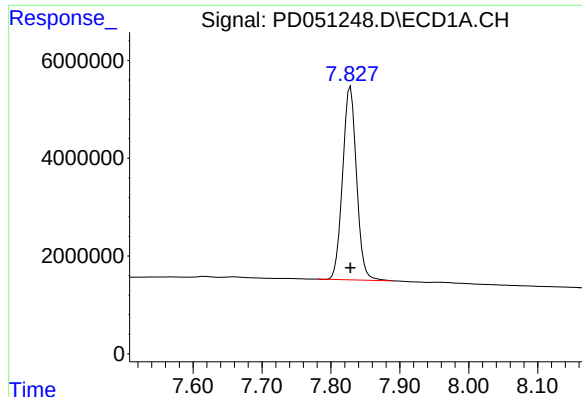

#28 Decachlorobiphenyl

R.T.: 7.828 min  
Delta R.T.: 0.000 min  
Response: 55498928  
Conc: 50.00 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PCHLORICC500

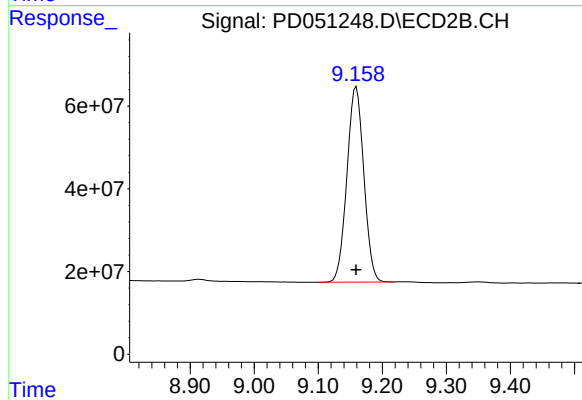

#28 Decachlorobiphenyl

R.T.: 9.159 min  
Delta R.T.: 0.000 min  
Response: 863965227  
Conc: 50.00 ng/ml