

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
 Data File : PD051273.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2019 17:53
 Operator : AJ\SJ
 Sample : K1422-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TEST-PIT-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:54:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
 Quant Title : GC Extractables
 QLast Update : Sat Feb 09 00:01:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	29023074	572.2E6	20.987	19.661
28)	SA Decachlor...	7.827	9.157	21122781	322.8E6	18.398	18.278

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020819\
Data File : PD051273.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2019 17:53
Operator : AJ\SJ
Sample : K1422-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TEST-PIT-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:54:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020819.M
Quant Title : GC Extractables
QLast Update : Sat Feb 09 00:01:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

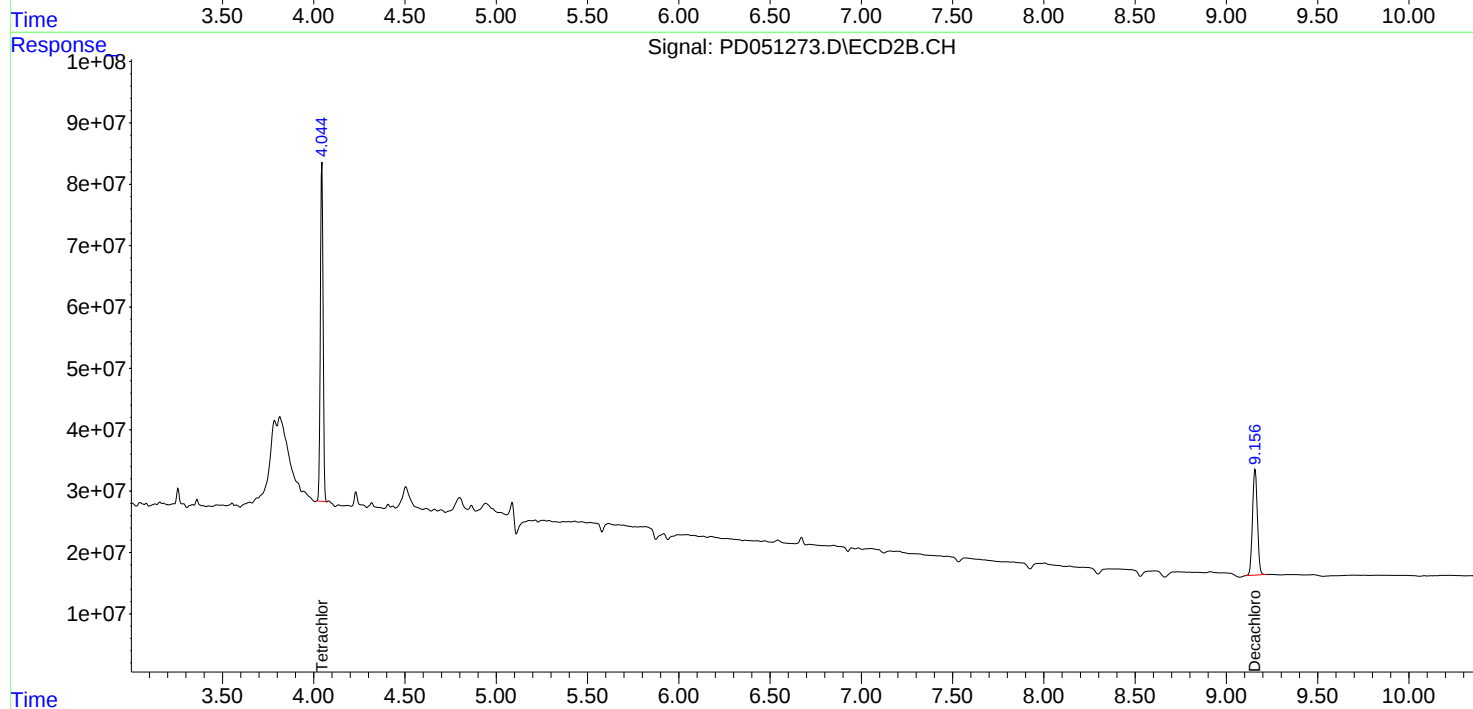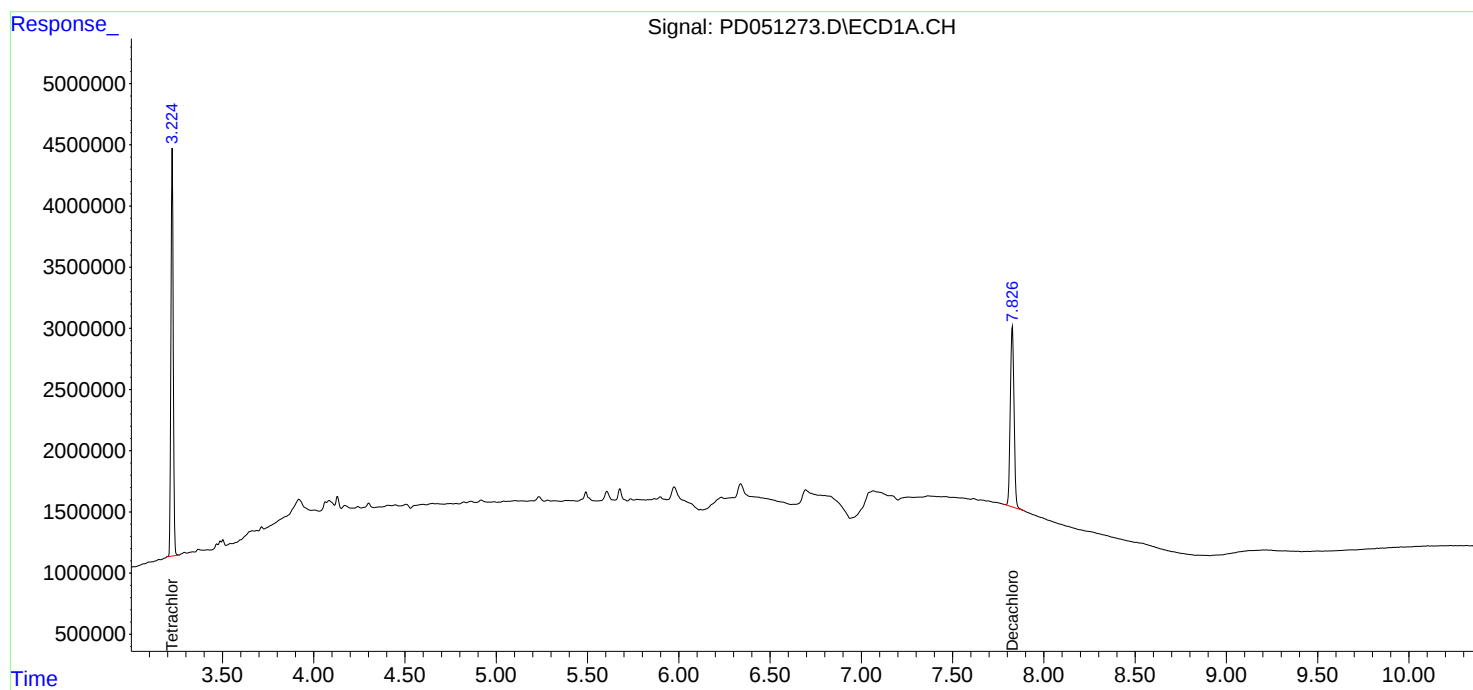


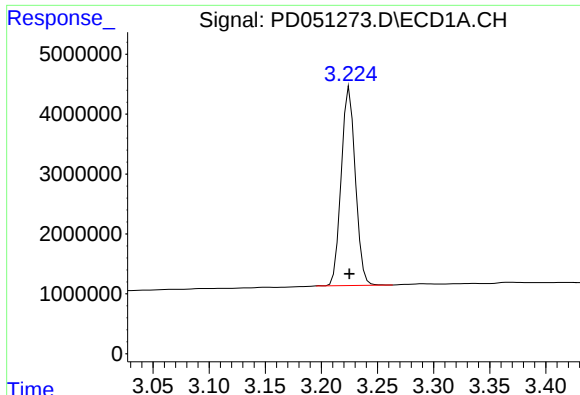

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 29023074
Conc: 20.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
TEST-PIT-1

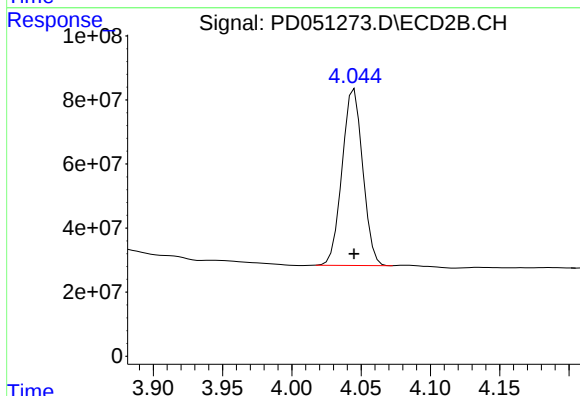


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 572154483
Conc: 19.66 ng/ml

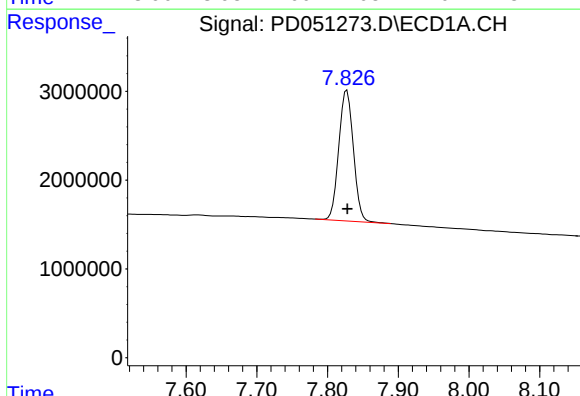

#28 Decachlorobiphenyl

R.T.: 7.827 min
Delta R.T.: 0.000 min
Response: 21122781
Conc: 18.40 ng/ml

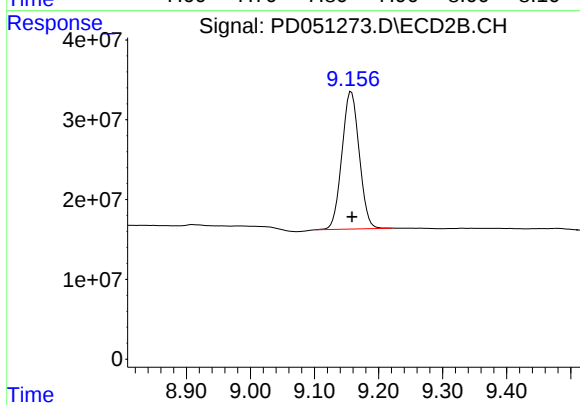

#28 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: -0.001 min
Response: 322827876
Conc: 18.28 ng/ml