

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020821\
 Data File : PD061137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2021 14:11
 Operator : DD\AJ
 Sample : M1274-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AD2

Manual Integrations
 APPROVED

Ankita
 2/9/2021 10:53:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 06:13:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.506	3.990f	4493.8E6	28142.2E6	4427.431m	3932.788m
27) SA Decachlor...	8.273	9.101	36358531	206.3E6	28.855	30.383
Target Compounds						
8) B Heptachlo...	5.214	5.892	6201379	7368188	4.557	0.850m#
13) MA Dieldrin	5.805	6.514	13611849	81658729	9.270m	8.784
14) MA Endrin	6.080	6.743	3491474	15296961	2.809	2.071 #
17) MA 4,4'-DDT	6.431	7.135	4625467	18450618	3.778	2.541 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020821\
Data File : PD061137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2021 14:11
Operator : DD\AJ
Sample : M1274-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 06:13:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

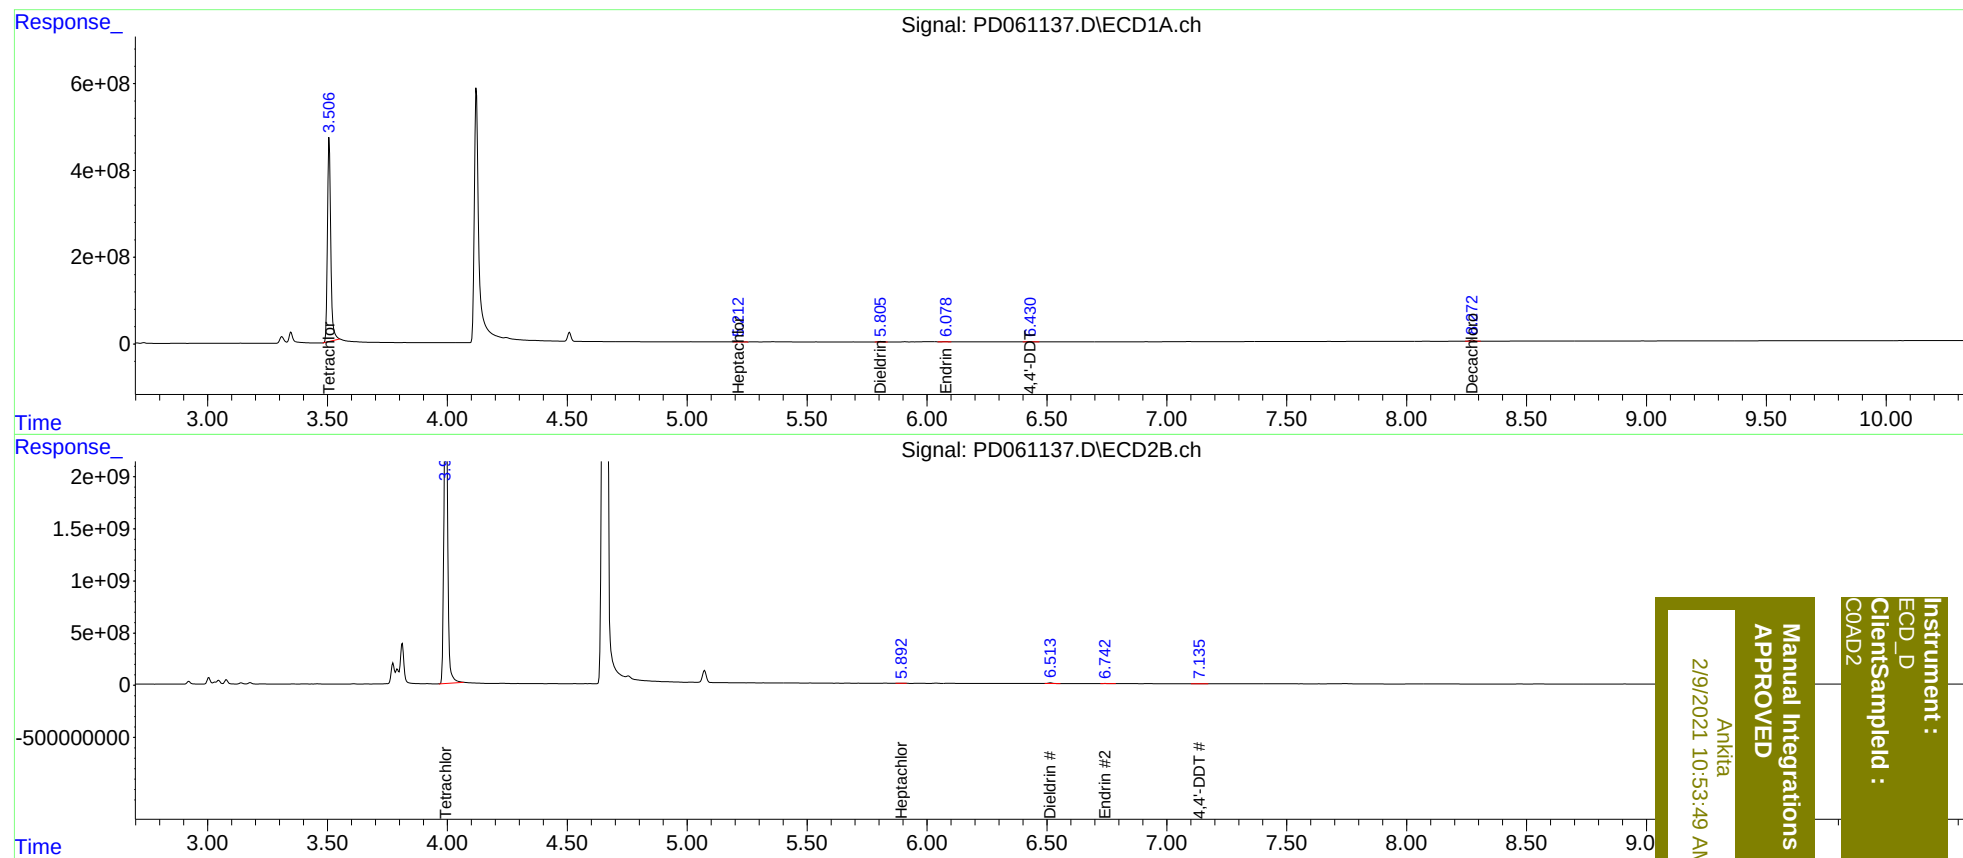

Manual Integrations
APPROVED

Ankita
2/9/2021 10:53:49 AM

Instrument :
ECD_D
ClientSampleId :
C0AD2