

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020823\
 Data File : PD073855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2023 18:37
 Operator : AR\AJ
 Sample : 01462-15 (Sig #1); 01462-015 (Sig #2)
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 01:53:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.775	23602209	12803931	10.097	10.058
28)	SA Decachlor...	9.099	7.931	36511026	15390733	12.956	13.228

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020823\
Data File : PD073855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2023 18:37
Operator : AR\AJ
Sample : 01462-15 (Sig #1); 01462-015 (Sig #2)
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 01:53:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

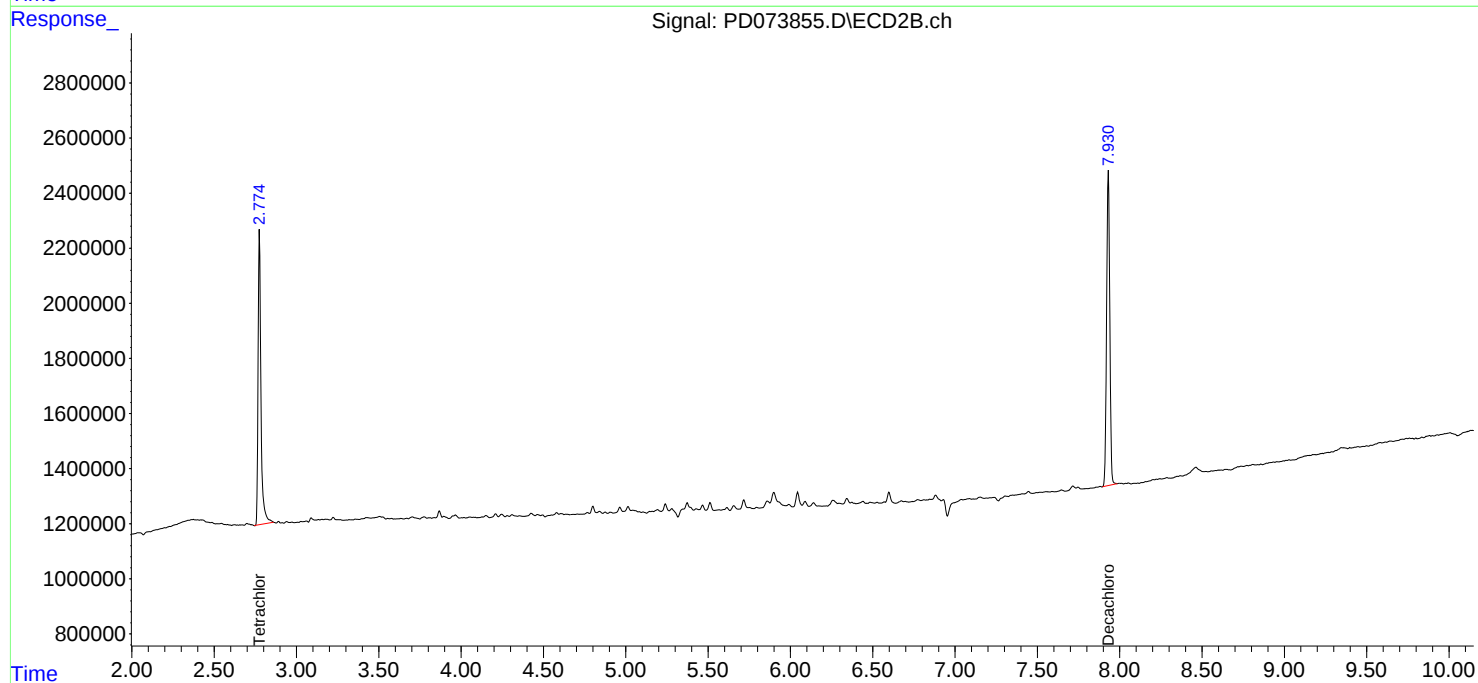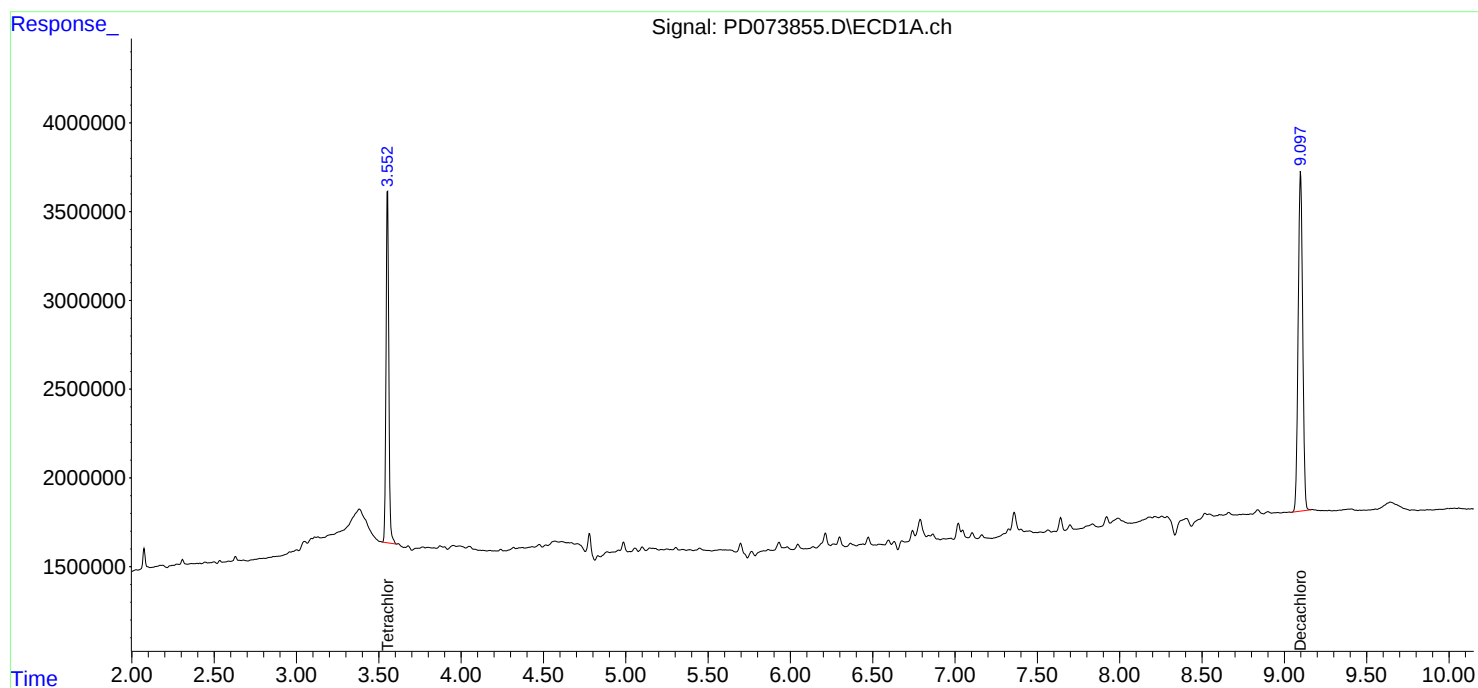


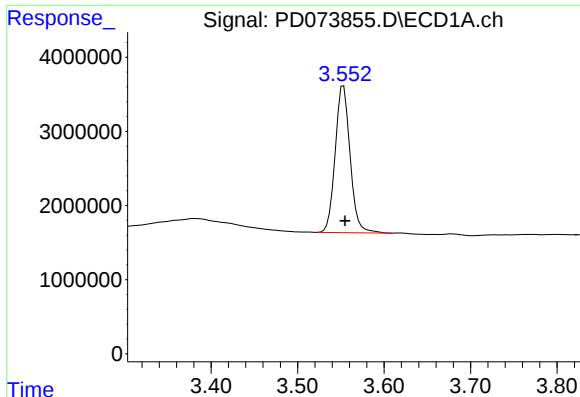

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: -0.002 min
Response: 23602209
Conc: 10.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-3

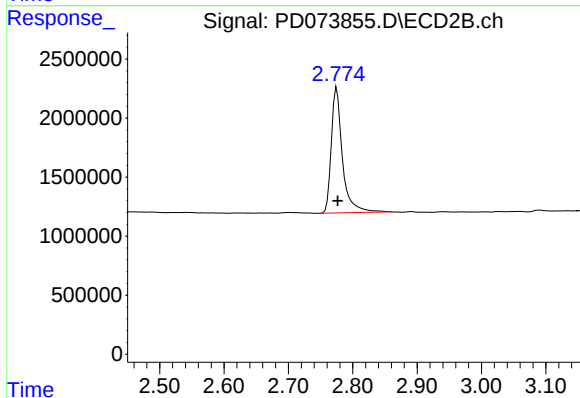


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: -0.002 min
Response: 12803931
Conc: 10.06 ng/ml

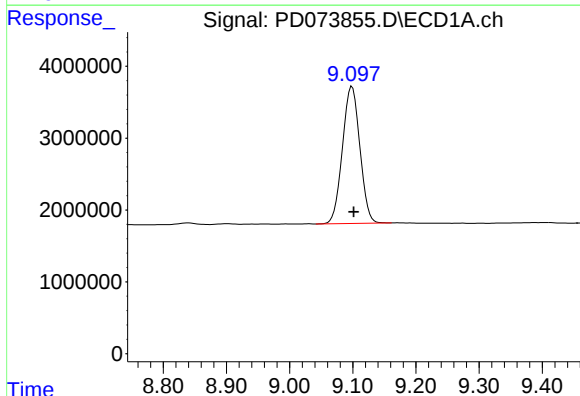

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.003 min
Response: 36511026
Conc: 12.96 ng/ml

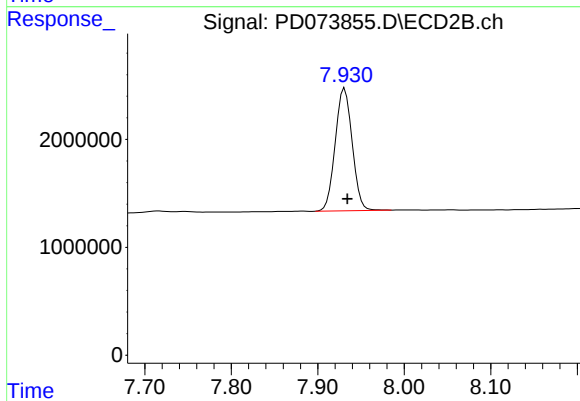

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: -0.003 min
Response: 15390733
Conc: 13.23 ng/ml