

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020823\
 Data File : PD073862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2023 20:12
 Operator : AR\AJ
 Sample : 01466-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 01:58:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.775	32208464	18107692	13.779	14.224
28)	SA Decachlor...	9.098	7.931	25991302	10541154	9.223	9.060
Target Compounds							
13)	MA Dieldrin	6.368	5.372	3893058	1950797	1.221	1.488



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020823\
Data File : PD073862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2023 20:12
Operator : AR\AJ
Sample : 01466-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
A-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 01:58:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

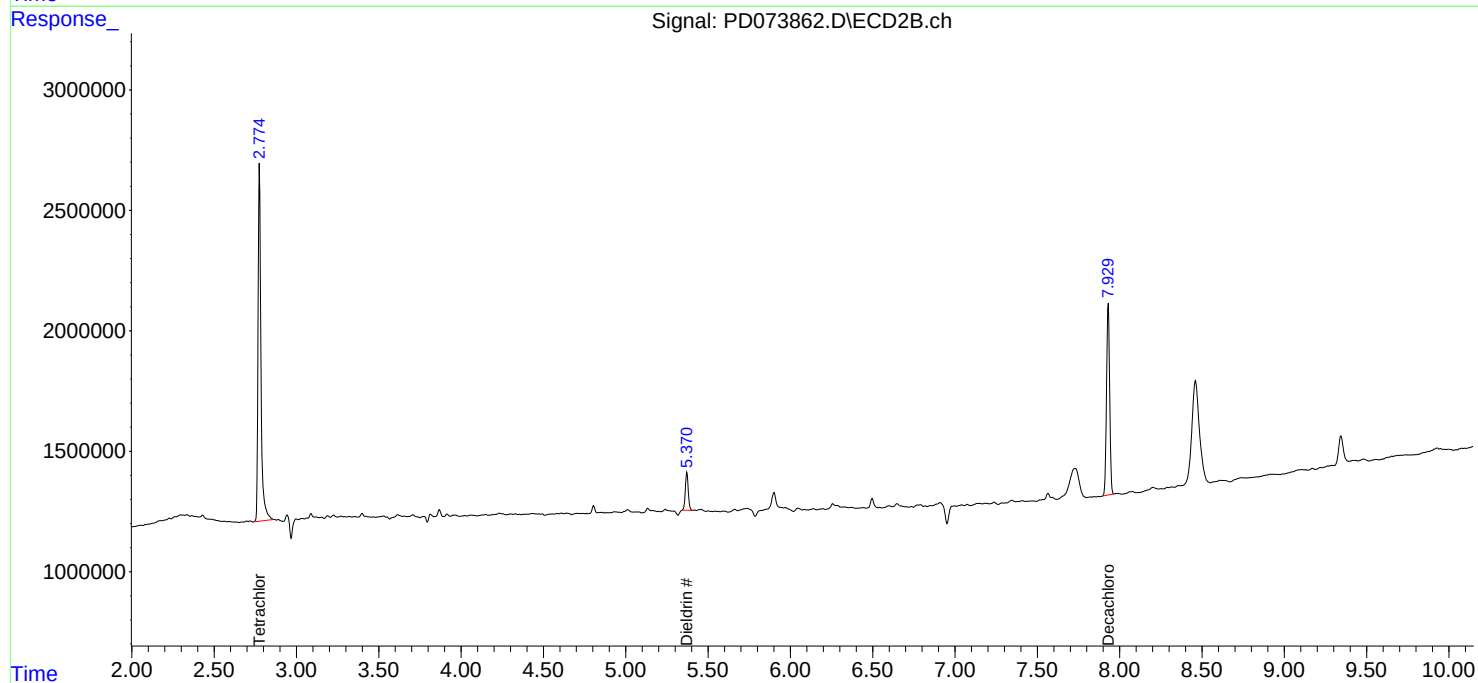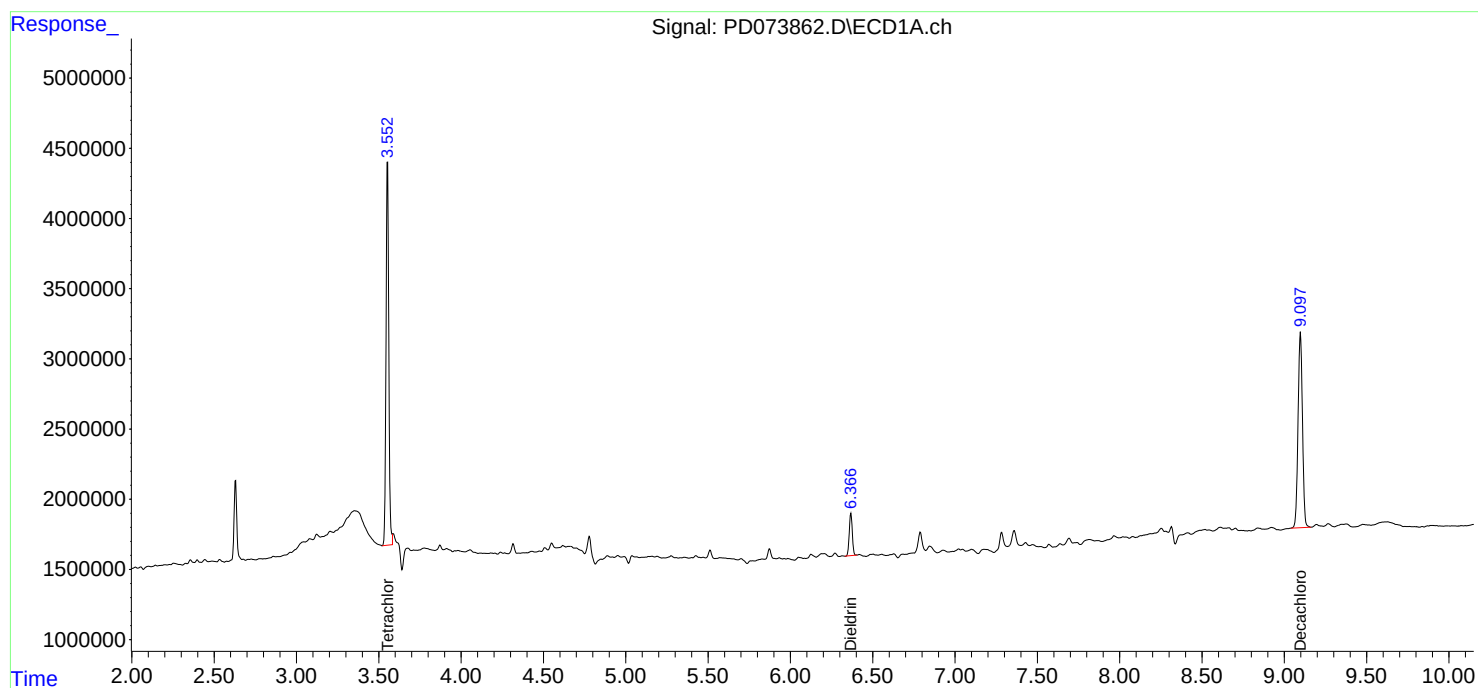


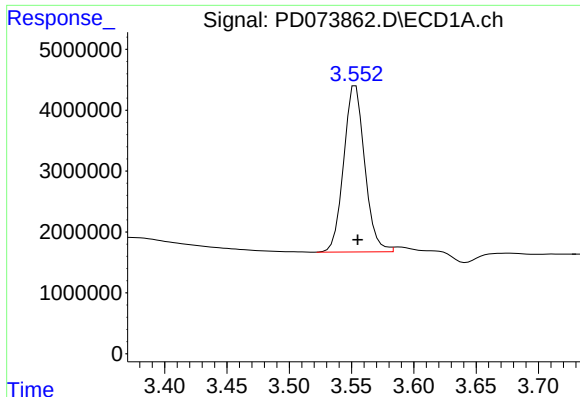

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: -0.002 min
Response: 32208464
Conc: 13.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

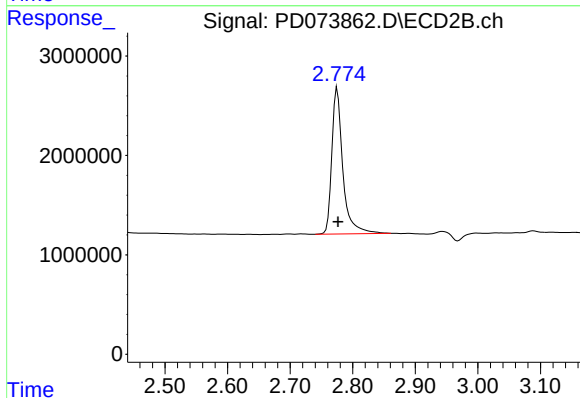


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: -0.002 min
Response: 18107692
Conc: 14.22 ng/ml

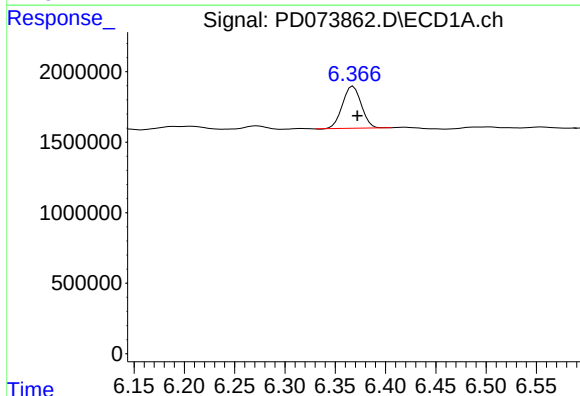


#13 Dieldrin

R.T.: 6.368 min
Delta R.T.: -0.004 min
Response: 3893058
Conc: 1.22 ng/ml

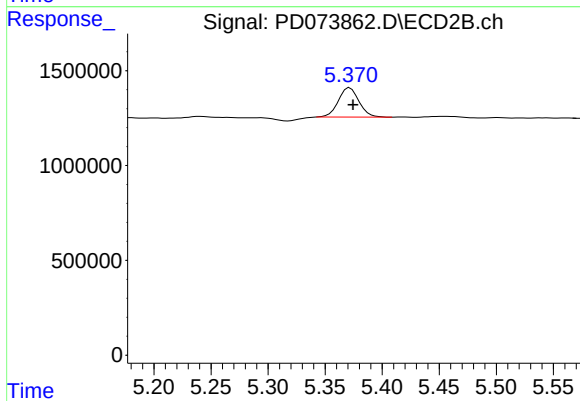

#13 Dieldrin


R.T.: 5.372 min
Delta R.T.: -0.003 min
Response: 1950797
Conc: 1.49 ng/ml

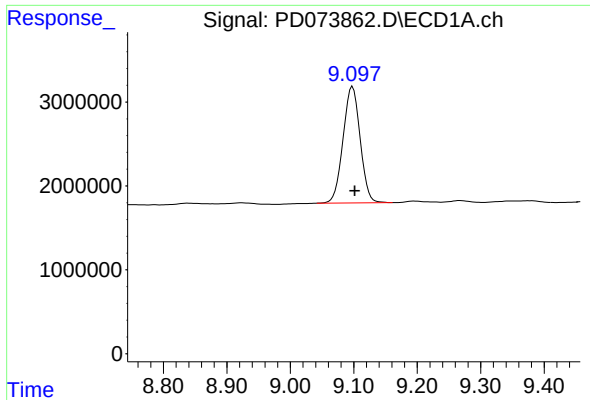

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.004 min
Response: 25991302
Conc: 9.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

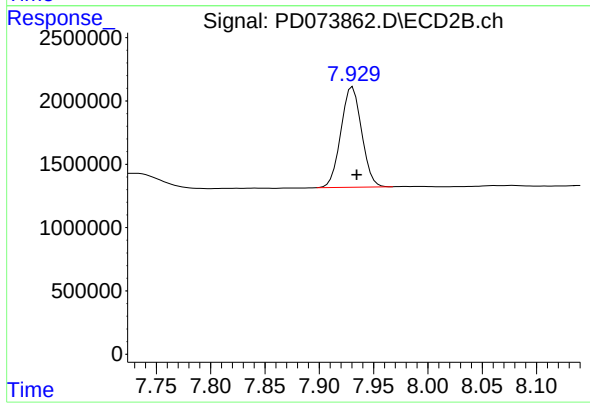

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: -0.004 min
Response: 10541154
Conc: 9.06 ng/ml