

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020823\
 Data File : PD073868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2023 22:13
 Operator : AR\AJ
 Sample : 01445-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JPP-26-020323

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/08/2023
 Supervised By :Ankita Jodhani 02/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 03:48:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.554	2.774	37225418	18692520	15.925	14.683m
28) SA Decachlor...	9.086f	7.929	77072032	24680149	27.349	21.213

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020823\
Data File : PD073868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2023 22:13
Operator : AR\AJ
Sample : 01445-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
JPP-26-020323


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/08/2023
Supervised By : Ankita Jodhani 02/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 03:48:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

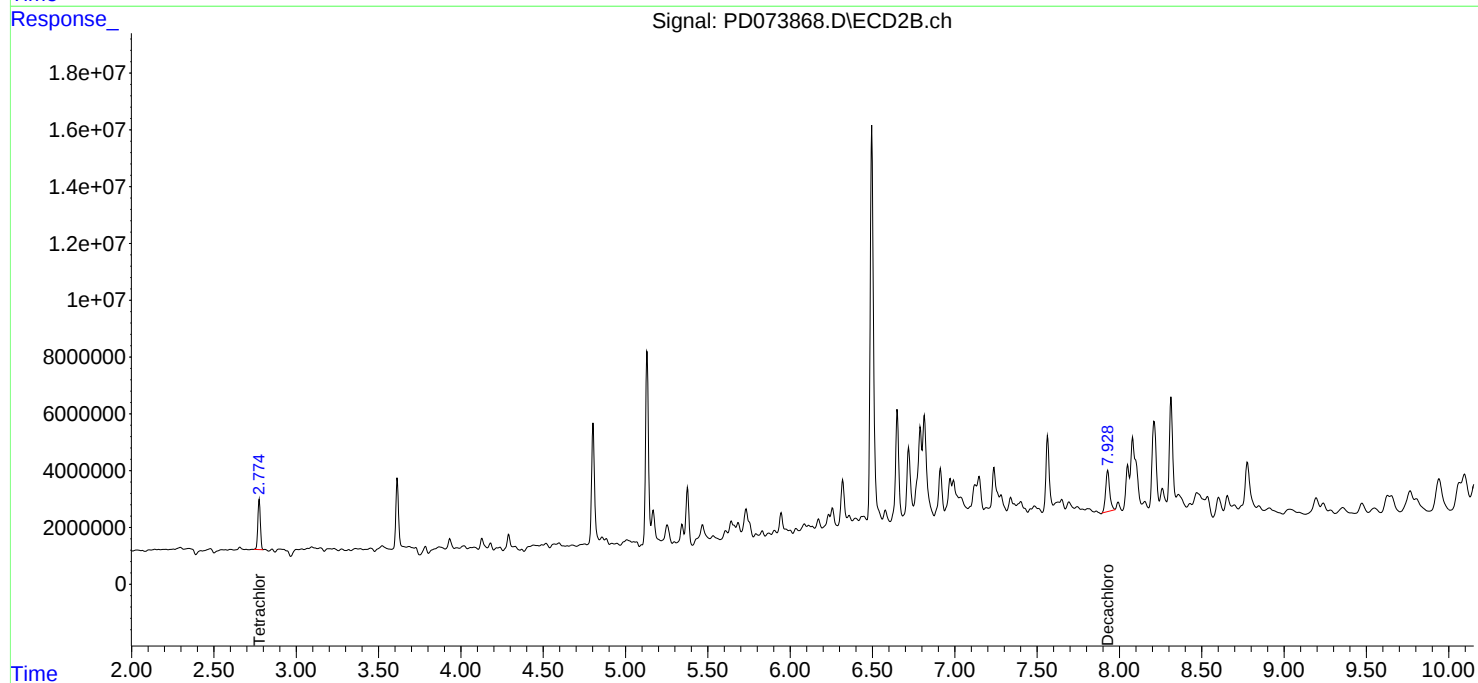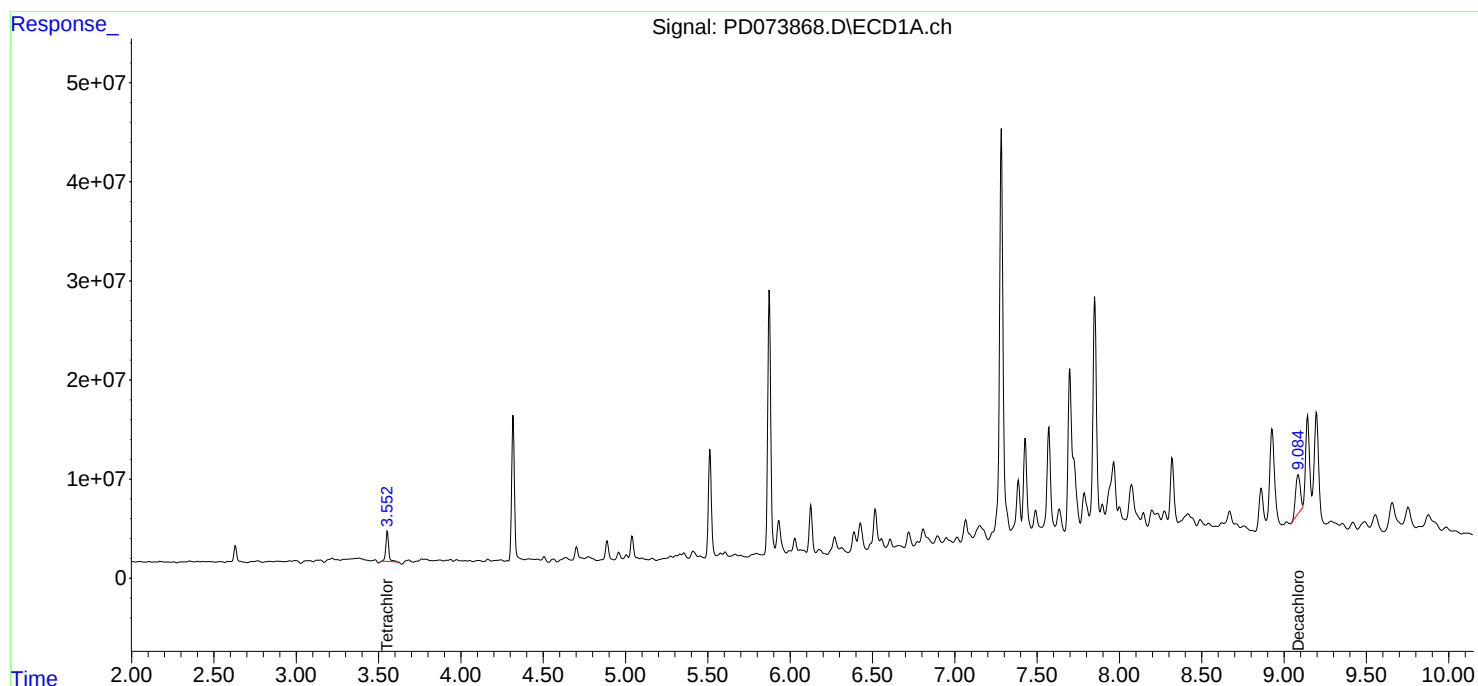

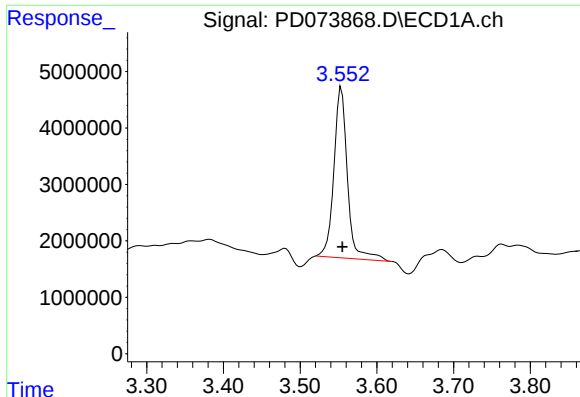

#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: -0.001 min
Response: 37225418
Conc: 15.93 ng/ml

Instrument :


ECD_D

ClientSampleId :

JPP-26-020323


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/08/2023
Supervised By :Ankita Jodhani 02/08/2023

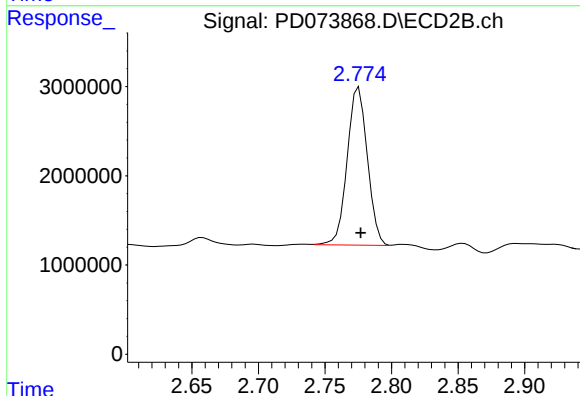


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: -0.003 min
Response: 18692520
Conc: 14.68 ng/ml m

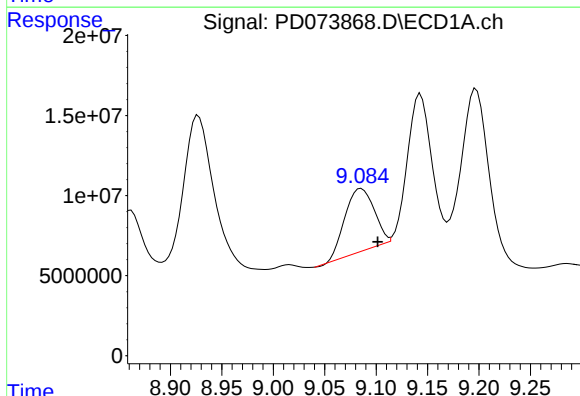

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: -0.016 min
Response: 77072032
Conc: 27.35 ng/ml

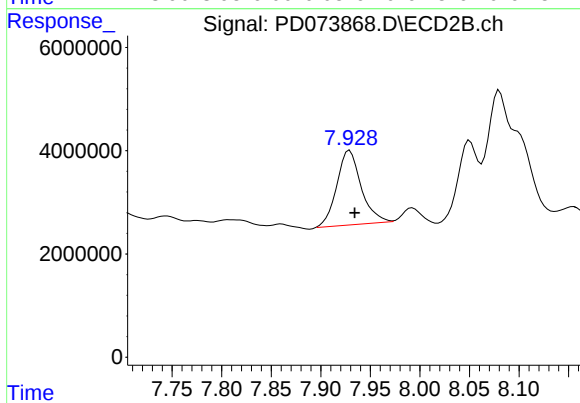

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: -0.005 min
Response: 24680149
Conc: 21.21 ng/ml