

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020824\
 Data File : PD081198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 11:45
 Operator : AR\AJ
 Sample : P1367-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-6-7-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 19:59:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.795	28394073	49267279	20.002	20.595
28)	SA Decachlor...	9.109	7.931	39663447	51467111	19.709	19.322
Target Compounds							
3)	MA gamma-BHC...	0.000	3.634	0	394640	N.D.	0.106 #
4)	MA Heptachlor	4.960	0.000	146327	0	0.059	N.D. #
7)	B delta-BHC	4.792	0.000	9213776	0	3.673	N.D. #
9)	A Endosulfan I	6.130f	0.000	242114	0	0.117	N.D. #
10)	B gamma-Chl...	5.944f	0.000	1165402	0	0.532	N.D. #
13)	MA Dieldrin	6.389	0.000	92462	0	0.042	N.D. #
14)	MA Endrin	0.000	5.672	0	557785	N.D.	0.188 #
15)	B Endosulfa...	6.852f	5.978f	386619	441378	0.200	0.153
21)	B Endrin ke...	7.707f	0.000	246007	0	0.118	N.D. #
27)	Chlordane-5	0.000	5.978f	0	441378	N.D.	3.640 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020824\
Data File : PD081198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 11:45
Operator : AR\AJ
Sample : P1367-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 19:59:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

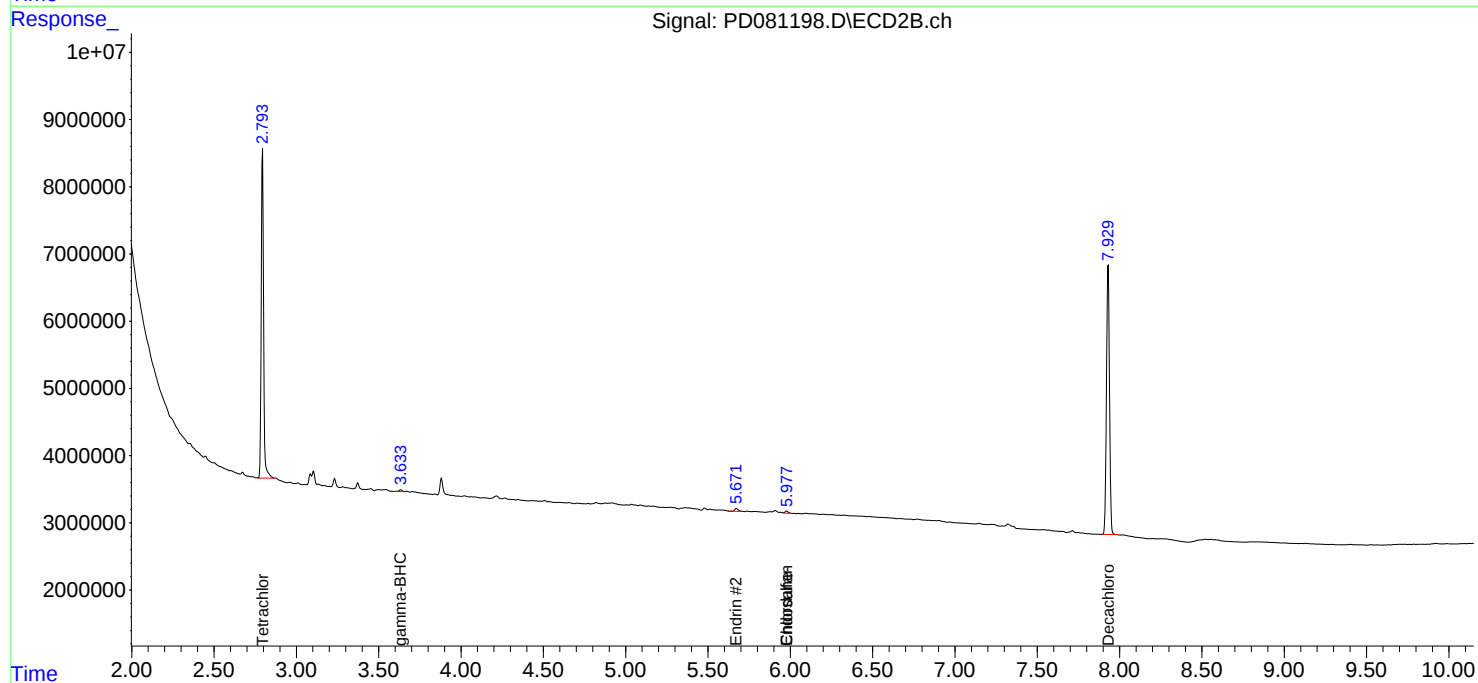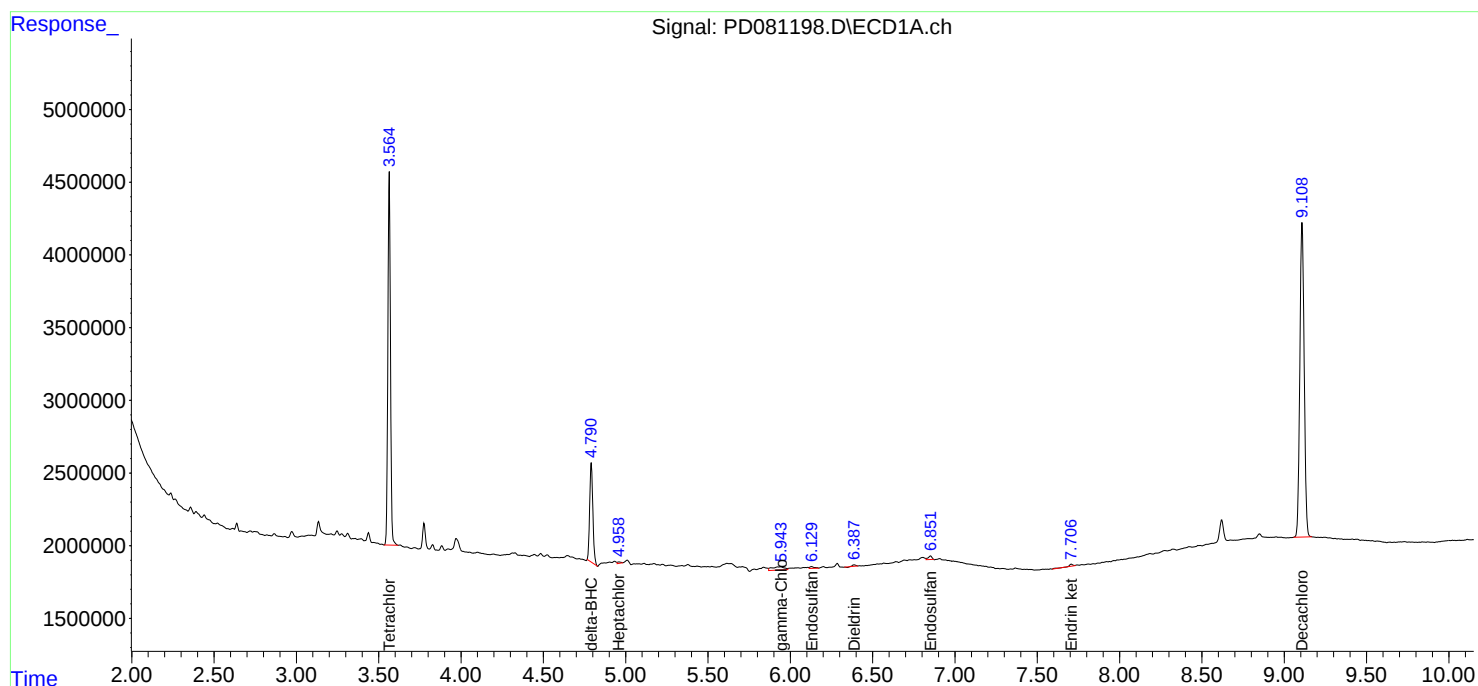


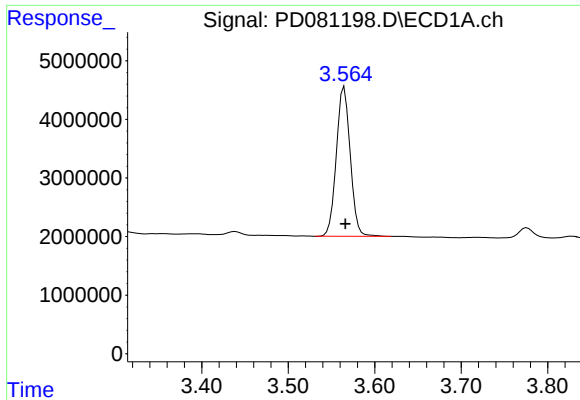

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: -0.001 min
Response: 28394073
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

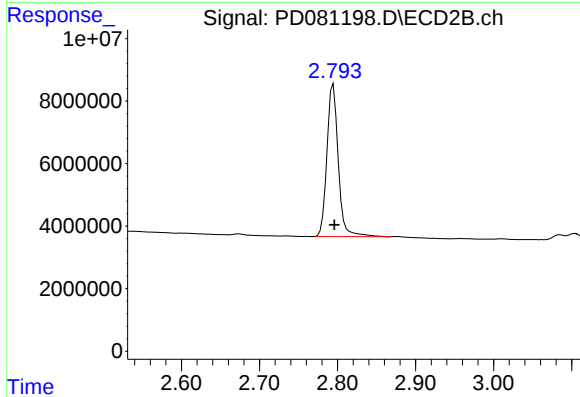


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.001 min
Response: 49267279
Conc: 20.60 ng/ml

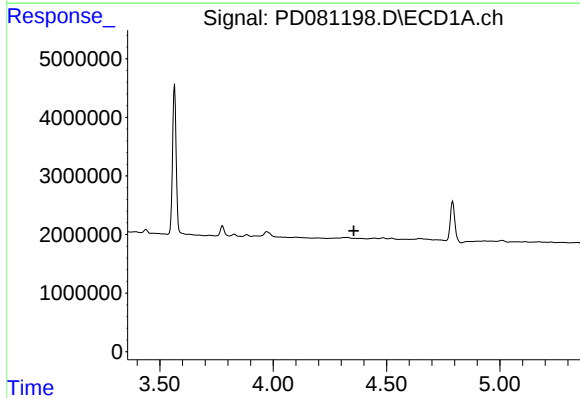


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.355 min
Response: 0
Conc: N.D.

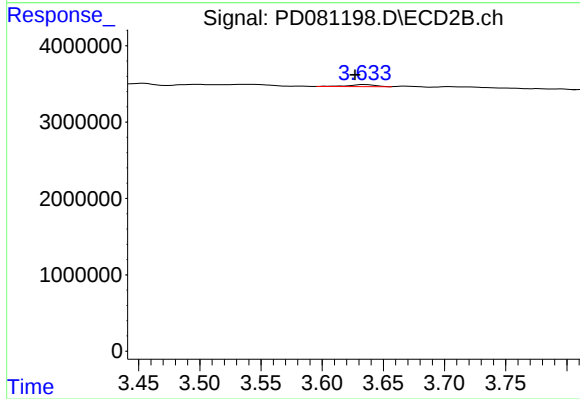

#3 gamma-BHC (Lindane)


R.T.: 3.634 min
Delta R.T.: 0.007 min
Response: 394640
Conc: 0.11 ng/ml

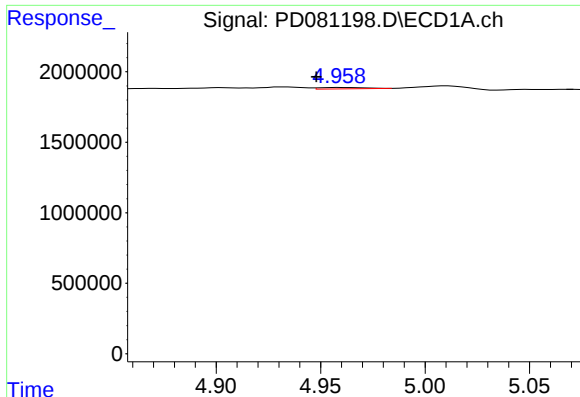

#4 Heptachlor


R.T.: 4.960 min
Delta R.T.: 0.012 min
Response: 146327
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

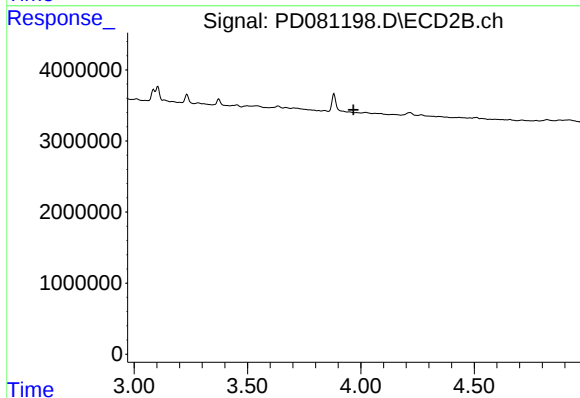


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.968 min
Response: 0
Conc: N.D.

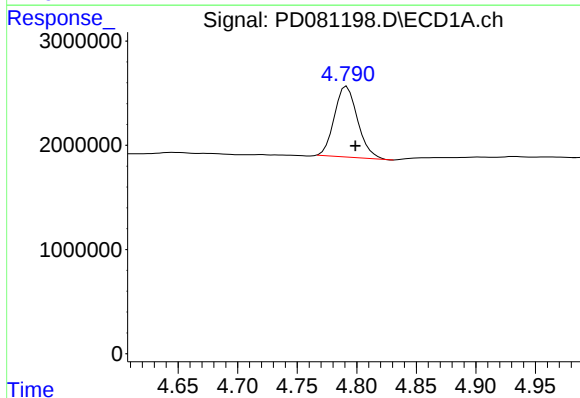


#7 delta-BHC

R.T.: 4.792 min
Delta R.T.: -0.007 min
Response: 9213776
Conc: 3.67 ng/ml

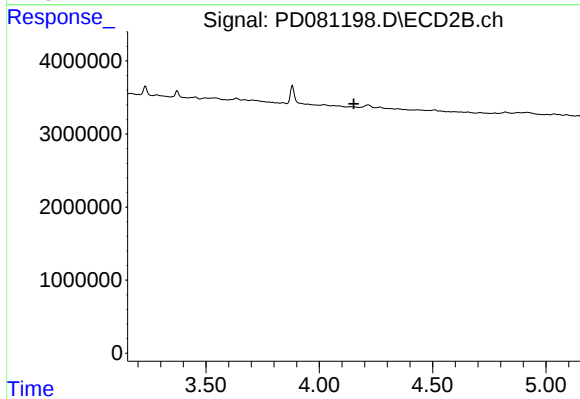

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

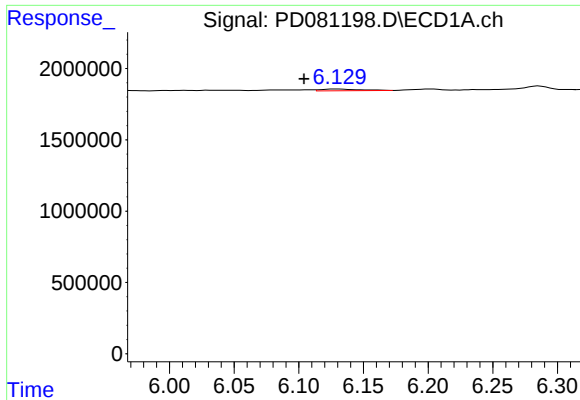

#9 Endosulfan I


R.T.: 6.130 min
Delta R.T.: 0.026 min
Response: 242114
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

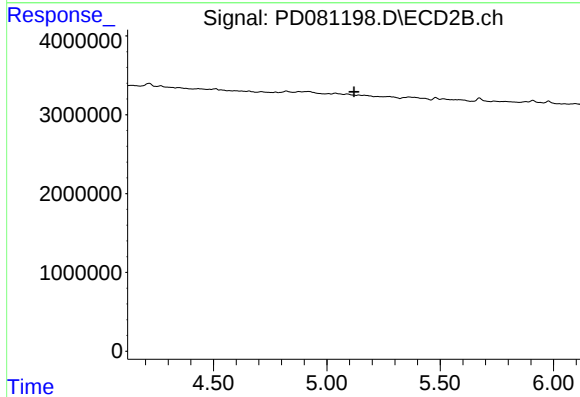


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.120 min
Response: 0
Conc: N.D.

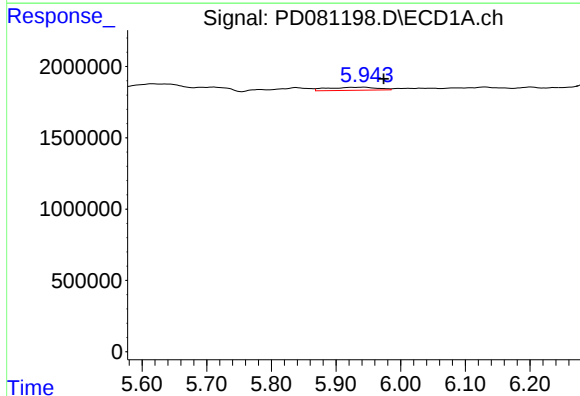


#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.030 min
Response: 1165402
Conc: 0.53 ng/ml

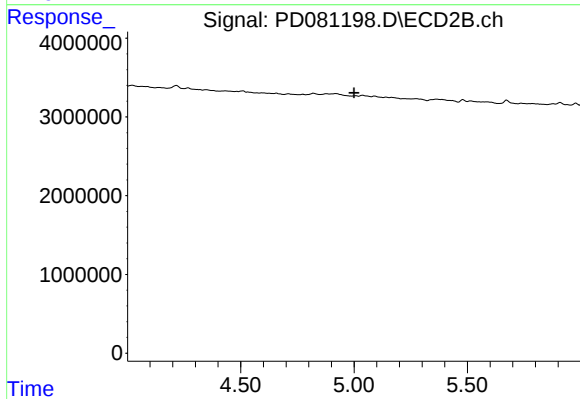

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

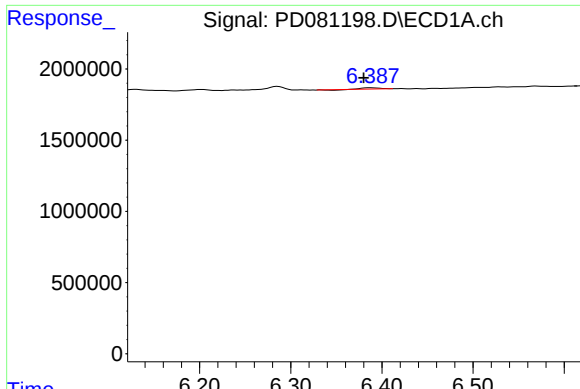

#13 Dieldrin


R.T.: 6.389 min
Delta R.T.: 0.009 min
Response: 92462
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

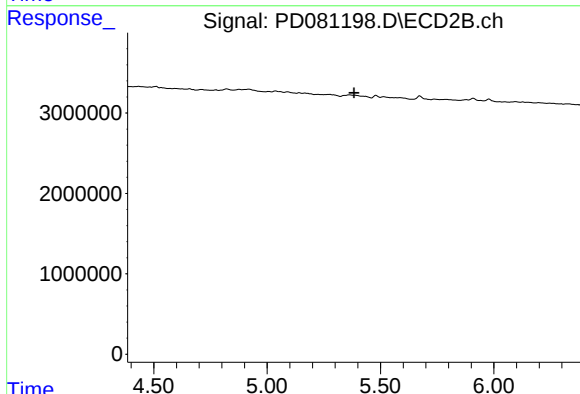


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

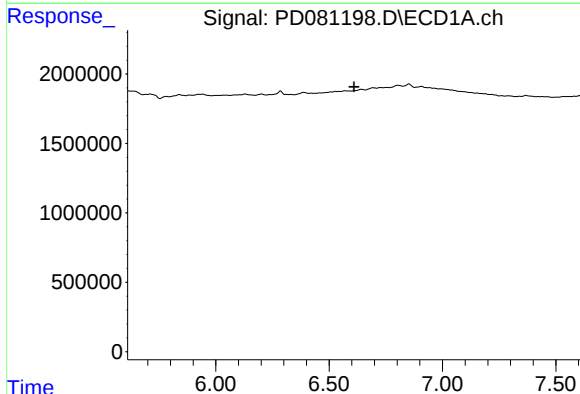


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.610 min
Response: 0
Conc: N.D.

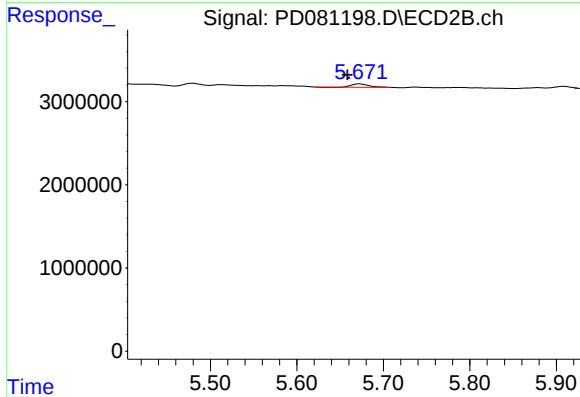

#14 Endrin


R.T.: 5.672 min
Delta R.T.: 0.014 min
Response: 557785
Conc: 0.19 ng/ml

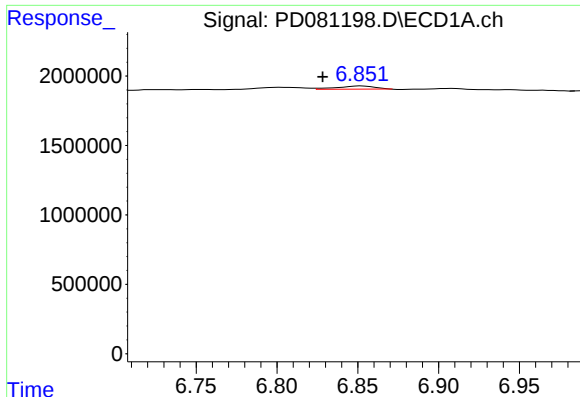

#15 Endosulfan II


R.T.: 6.852 min
Delta R.T.: 0.024 min
Response: 386619
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

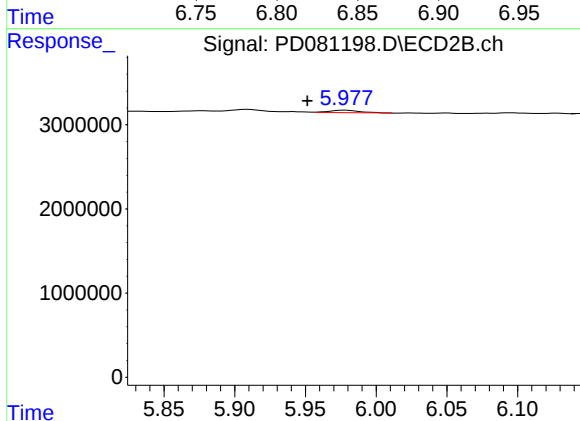


#15 Endosulfan II

R.T.: 5.978 min
Delta R.T.: 0.027 min
Response: 441378
Conc: 0.15 ng/ml

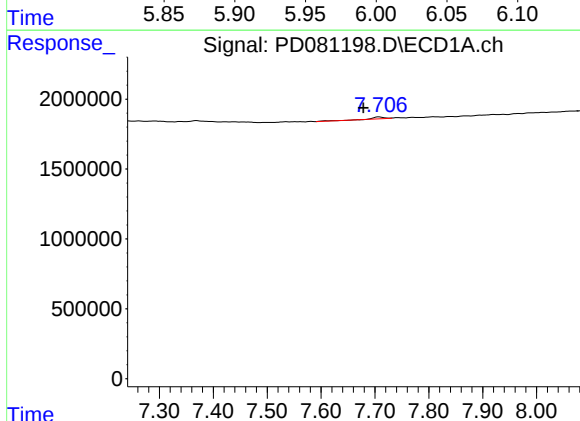


#21 Endrin ketone

R.T.: 7.707 min
Delta R.T.: 0.029 min
Response: 246007
Conc: 0.12 ng/ml

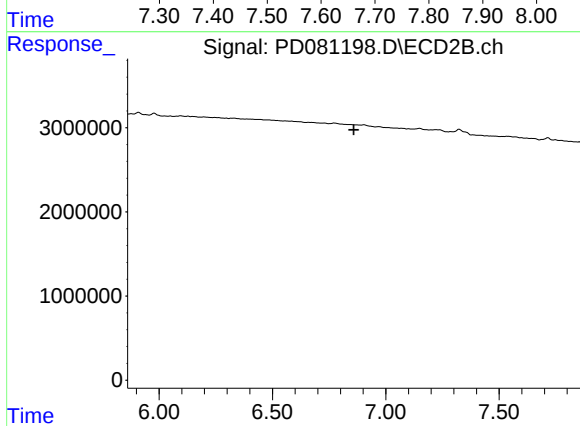

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.859 min
Response: 0
Conc: N.D.

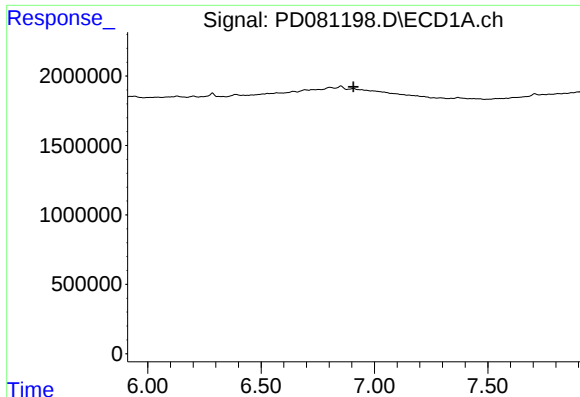

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-6-7-9

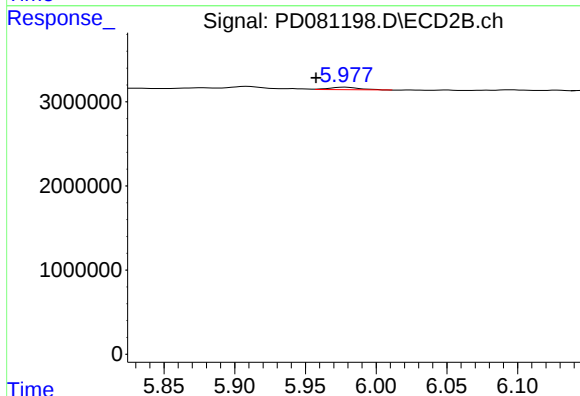


#27 Chlordane-5

R.T.: 5.978 min
Delta R.T.: 0.021 min
Response: 441378
Conc: 3.64 ng/ml

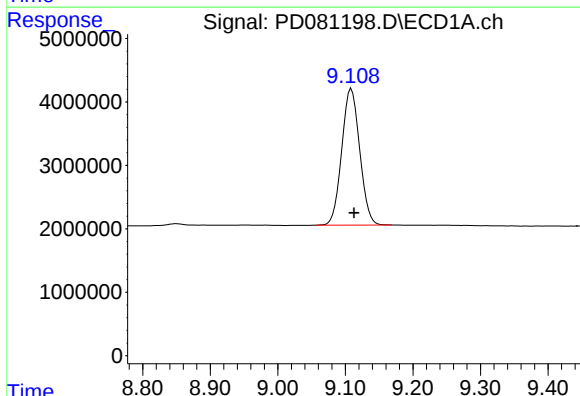

#28 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.004 min
Response: 39663447
Conc: 19.71 ng/ml

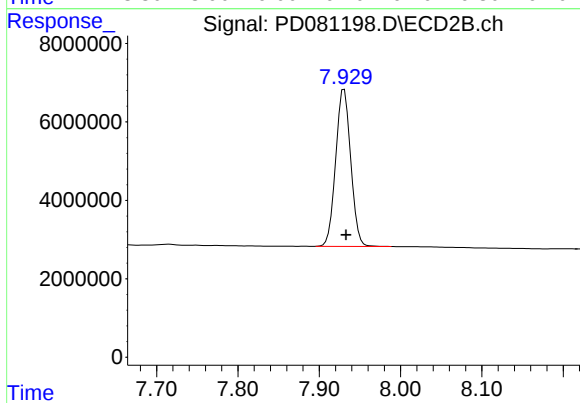

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: -0.002 min
Response: 51467111
Conc: 19.32 ng/ml