

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020824\
 Data File : PD081194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 10:47
 Operator : AR\AJ
 Sample : P1364-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 19:53:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.794	34857850	68683023	24.555	28.712
28)	SA Decachlor...	9.118	7.932	40633865	58417643	20.191	21.932
Target Compounds							
10)	B gamma-Chl...	5.981	4.998	29196261	47108490	13.337	14.402
11)	B alpha-Chl...	6.061	5.061	50910704	40267148	23.381	12.316 #
12)	B 4,4'-DDE	6.231	5.250	935.9E6	1434.8E6	459.934	468.375
16)	A 4,4'-DDD	6.748	5.804	33325739	56460410	20.282	21.507
17)	MA 4,4'-DDT	7.064	6.055	1468.0E6	2258.7E6	824.336	851.373



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020824\
Data File : PD081194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 10:47
Operator : AR\AJ
Sample : P1364-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 19:53:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

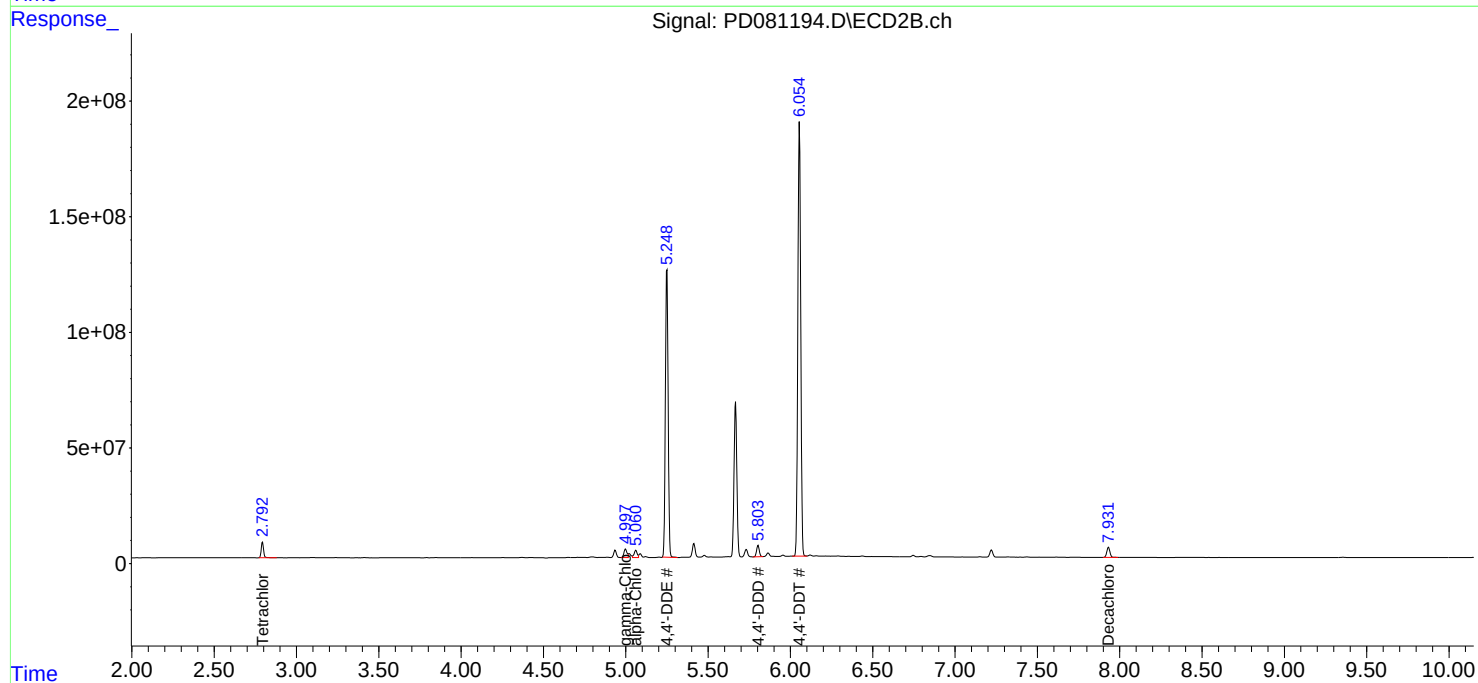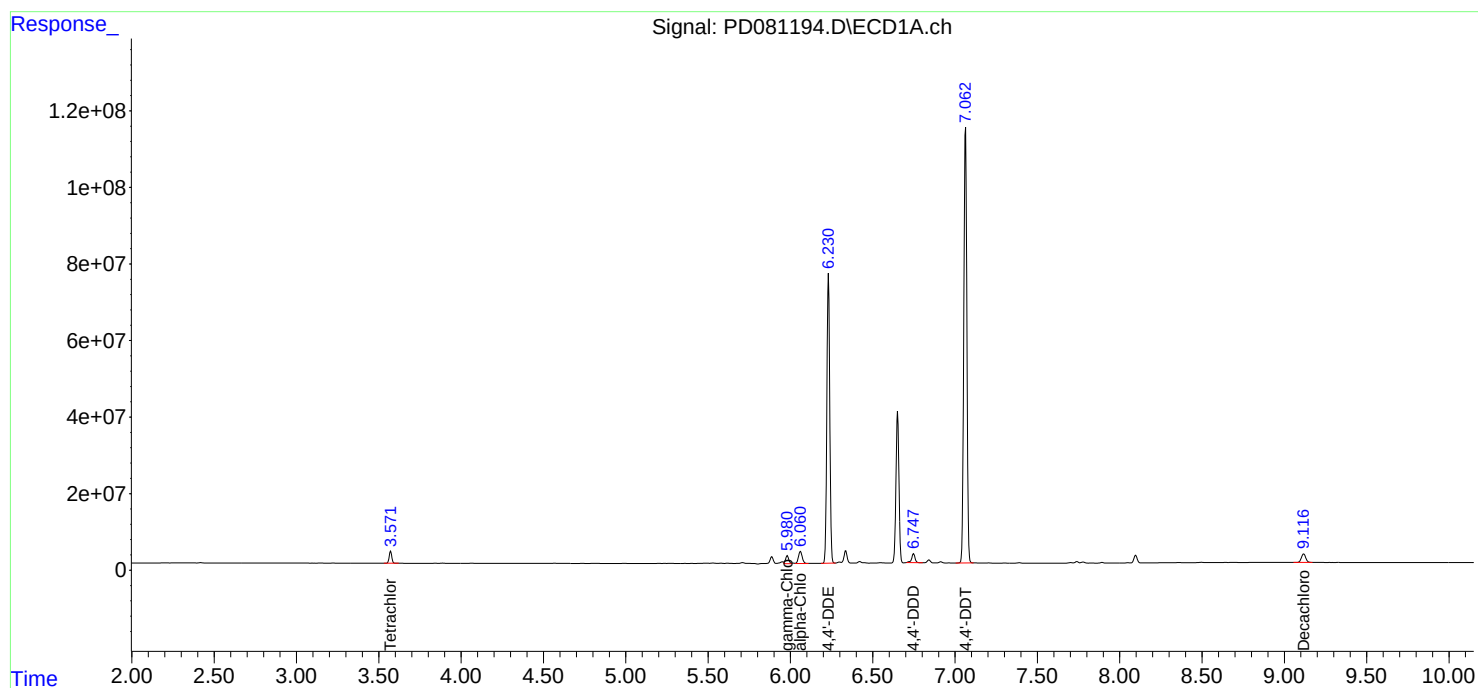


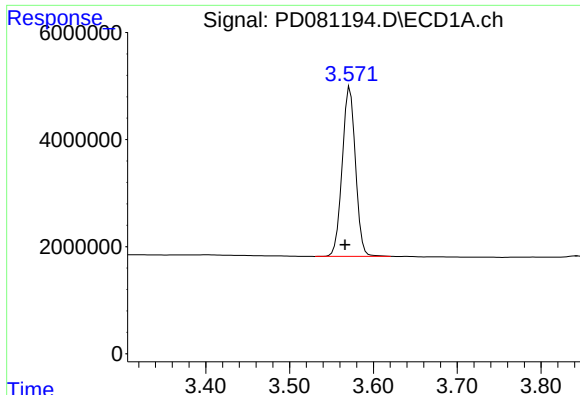

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: 0.006 min
Response: 34857850
Conc: 24.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

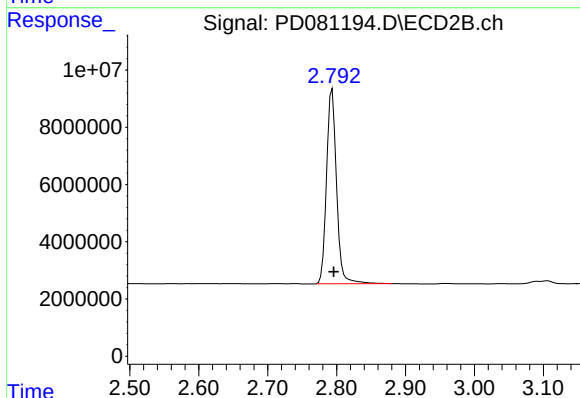


#1 Tetrachloro-m-xylene

R.T.: 2.794 min
Delta R.T.: -0.002 min
Response: 68683023
Conc: 28.71 ng/ml

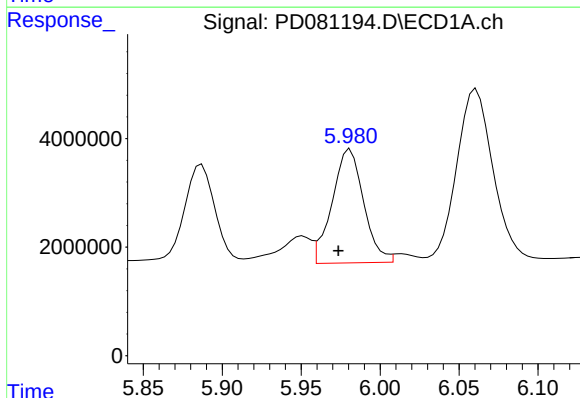


#10 gamma-Chlordane

R.T.: 5.981 min
Delta R.T.: 0.007 min
Response: 29196261
Conc: 13.34 ng/ml

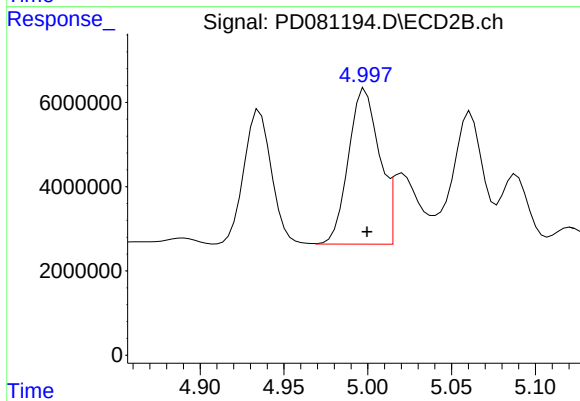

#10 gamma-Chlordane


R.T.: 4.998 min
Delta R.T.: -0.001 min
Response: 47108490
Conc: 14.40 ng/ml

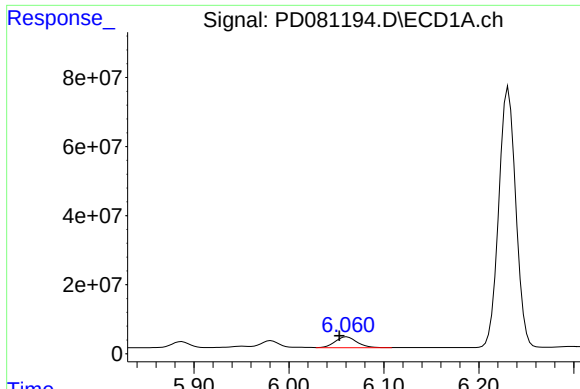

#11 alpha-Chlordane


R.T.: 6.061 min
Delta R.T.: 0.008 min
Response: 50910704
Conc: 23.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

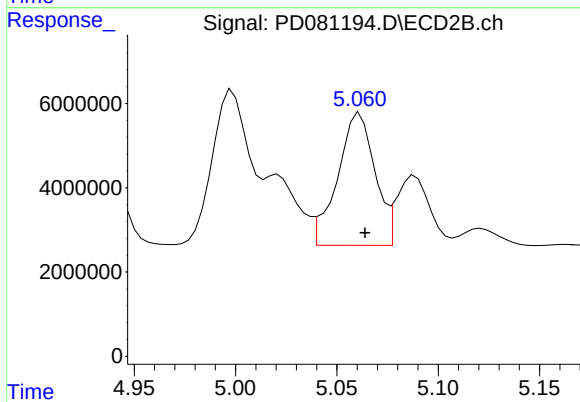


#11 alpha-Chlordane

R.T.: 5.061 min
Delta R.T.: -0.003 min
Response: 40267148
Conc: 12.32 ng/ml

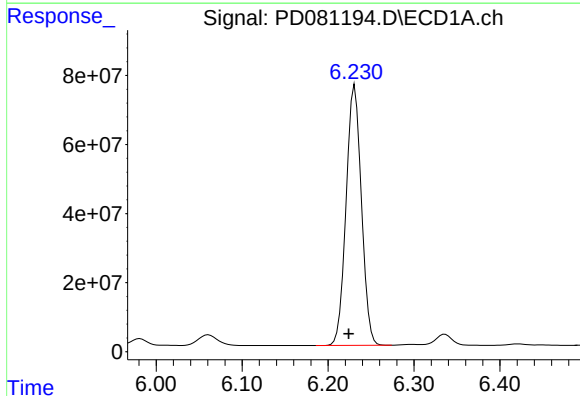


#12 4,4'-DDE

R.T.: 6.231 min
Delta R.T.: 0.007 min
Response: 935912263
Conc: 459.93 ng/ml

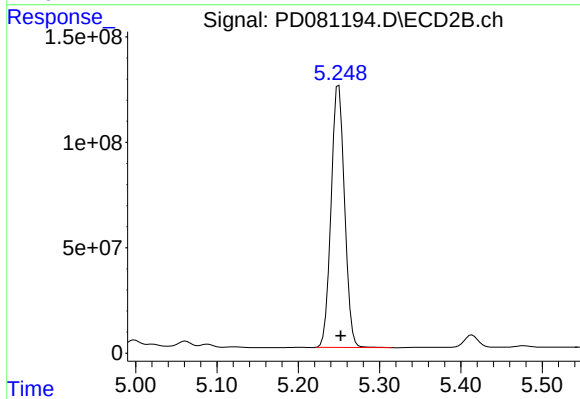

#12 4,4'-DDE


R.T.: 5.250 min
Delta R.T.: -0.002 min
Response: 1434752924
Conc: 468.38 ng/ml

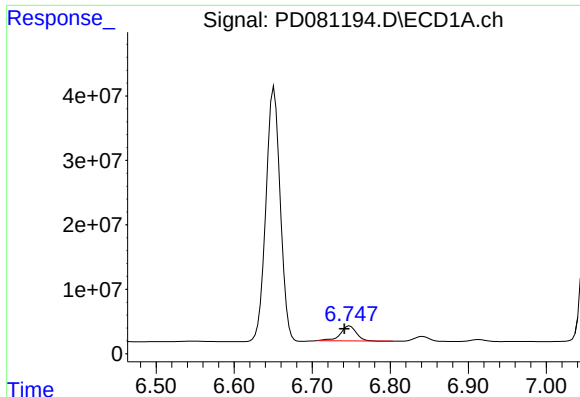

#16 4,4'-DDD


R.T.: 6.748 min
Delta R.T.: 0.007 min
Response: 33325739
Conc: 20.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

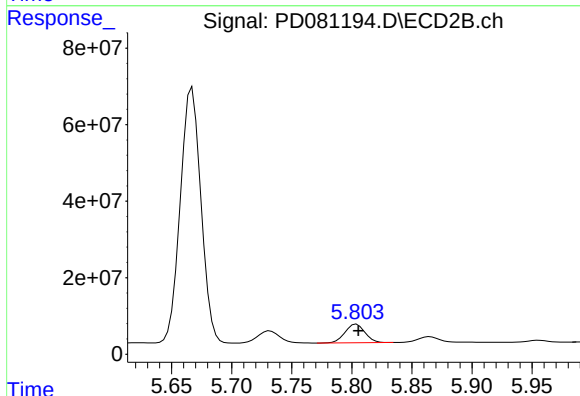


#16 4,4'-DDD

R.T.: 5.804 min
Delta R.T.: -0.001 min
Response: 56460410
Conc: 21.51 ng/ml

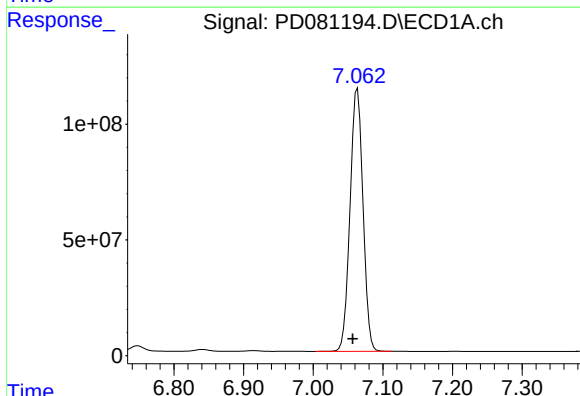


#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: 0.007 min
Response: 1468047918
Conc: 824.34 ng/ml

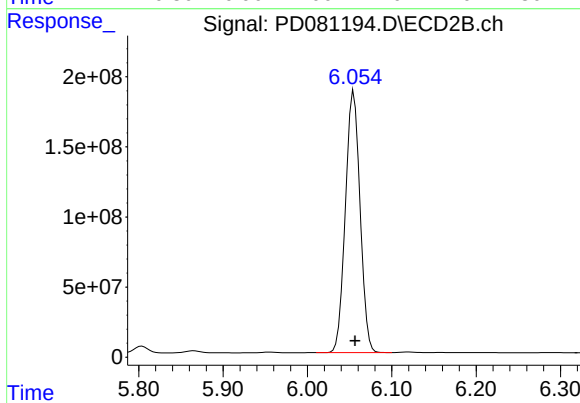

#17 4,4'-DDT


R.T.: 6.055 min
Delta R.T.: -0.002 min
Response: 2258744066
Conc: 851.37 ng/ml

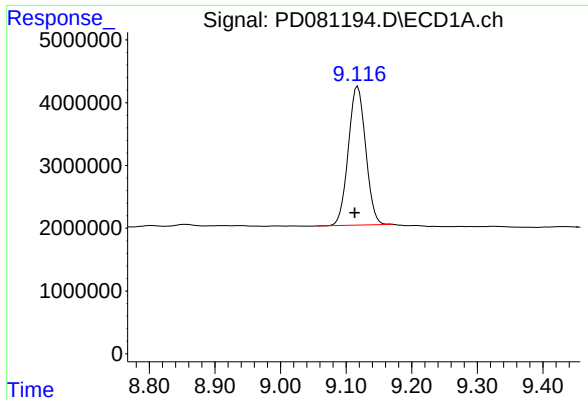

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.005 min
Response: 40633865
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

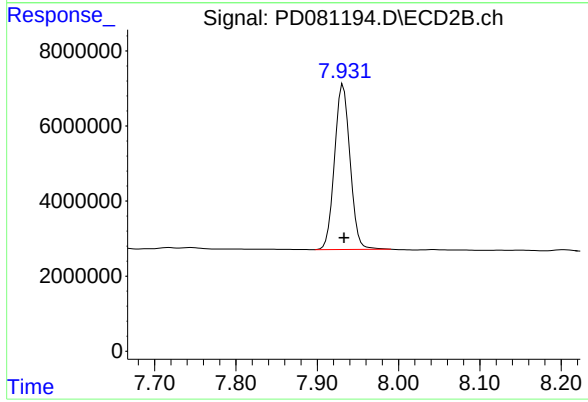

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.001 min
Response: 58417643
Conc: 21.93 ng/ml