

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020824\
 Data File : PD081206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 13:32
 Operator : AR\AJ
 Sample : P1321-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/09/2024
 Supervised By :Ankita Jodhani 02/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 20:10:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.793	22656602	29880709	15.960	12.491m
2)	SA Decachlor...	9.110	7.929	49366802	25883568	24.531m	9.717m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020824\
Data File : PD081206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 13:32
Operator : AR\AJ
Sample : P1321-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/09/2024
Supervised By : Ankita Jodhani 02/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 20:10:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

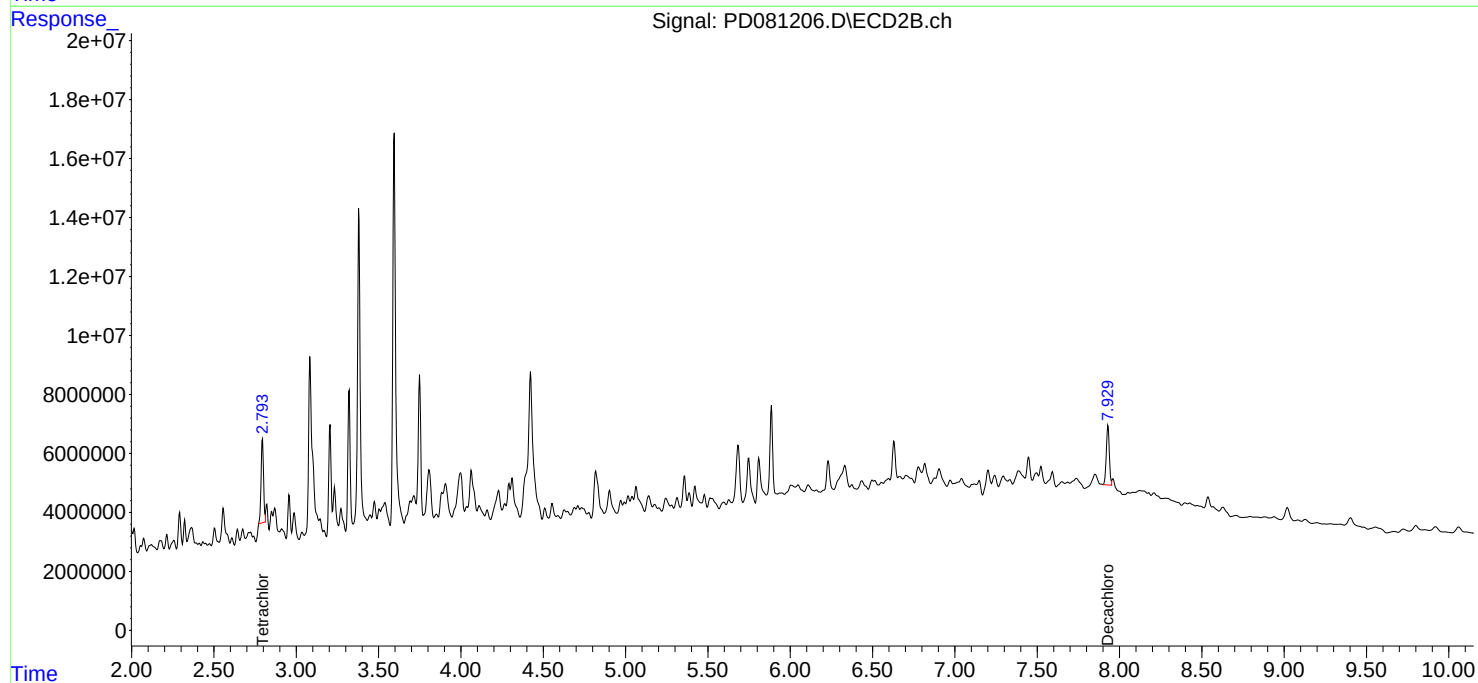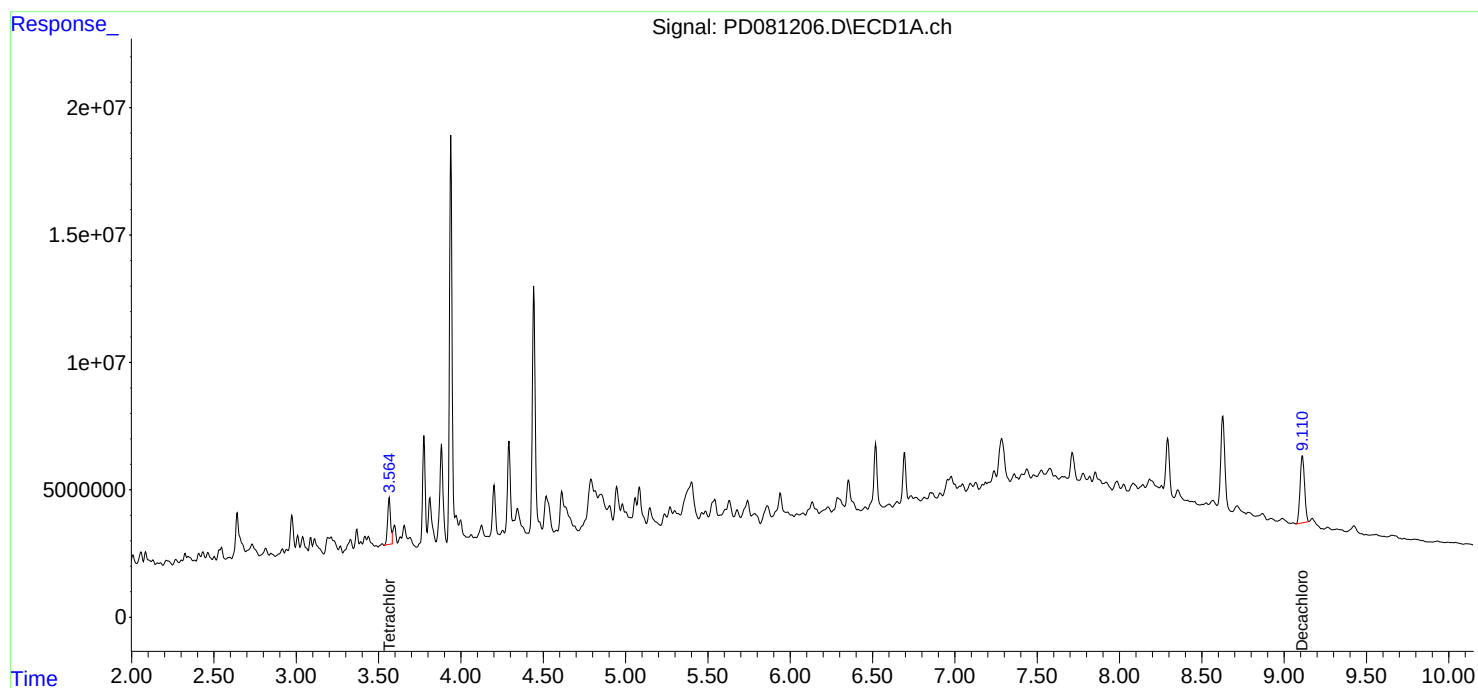

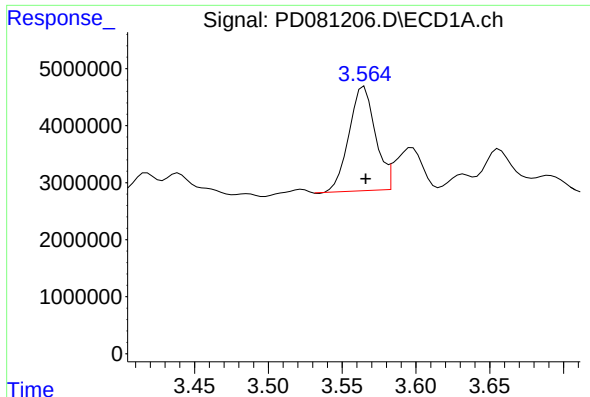


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.001 min
Response: 22656602
Conc: 15.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/09/2024
Supervised By :Ankita Jodhani 02/09/2024

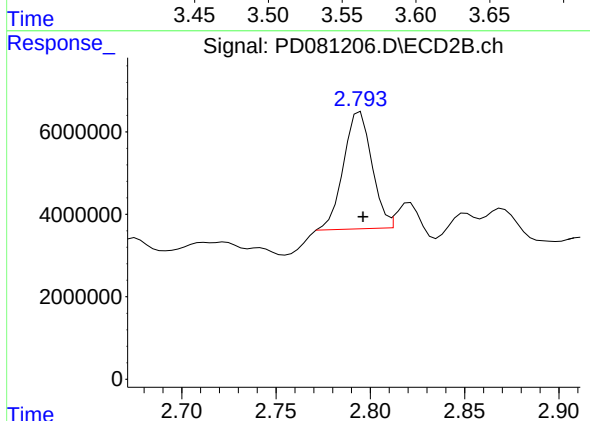


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.003 min
Response: 29880709
Conc: 12.49 ng/ml m

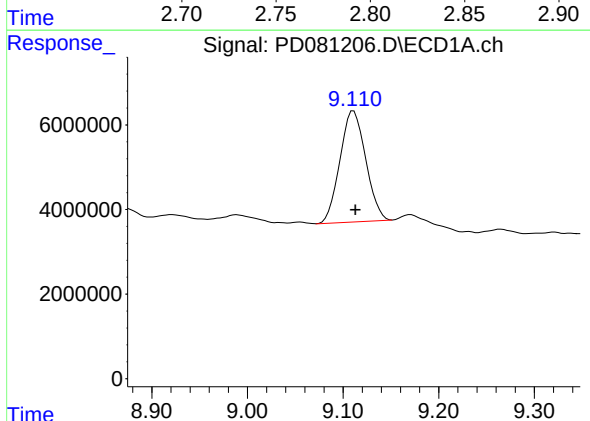

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.003 min
Response: 49366802
Conc: 24.53 ng/ml m

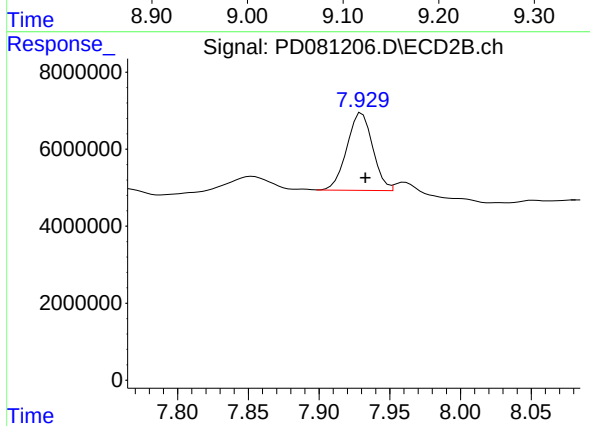

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: -0.004 min
Response: 25883568
Conc: 9.72 ng/ml m