

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
 Data File : PD061148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 15:36
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 03:40:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 10 03:32:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.020	27041851	170.6E6	21.704	21.673
28)	SA Decachlor...	8.275	9.105	30266715	168.4E6	21.511	22.090
Target Compounds							
9)	A Endosulfan I	5.562	6.259	16946190	105.8E6	10.222	10.750
10)	B gamma-Chl...	5.449	6.136	18057766	111.4E6	10.251	10.483
12)	B 4,4'-DDE	5.671	6.364	37855695	214.8E6	21.293	20.979
13)	MA Dieldrin	5.807	6.516	38507049	224.0E6	20.587	21.321
19)	B Endosulfa...	6.721	7.290	28743018	179.2E6	19.806	20.758
20)	A Methoxychlor	6.978	7.611	78220493	413.0E6	102.032	98.402
21)	B Endrin ke...	7.216	7.763	37083809	182.3E6	20.054	20.633



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
Data File : PD061148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 15:36
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 03:40:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
Quant Title : GC Extractables
QLast Update : Wed Feb 10 03:32:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

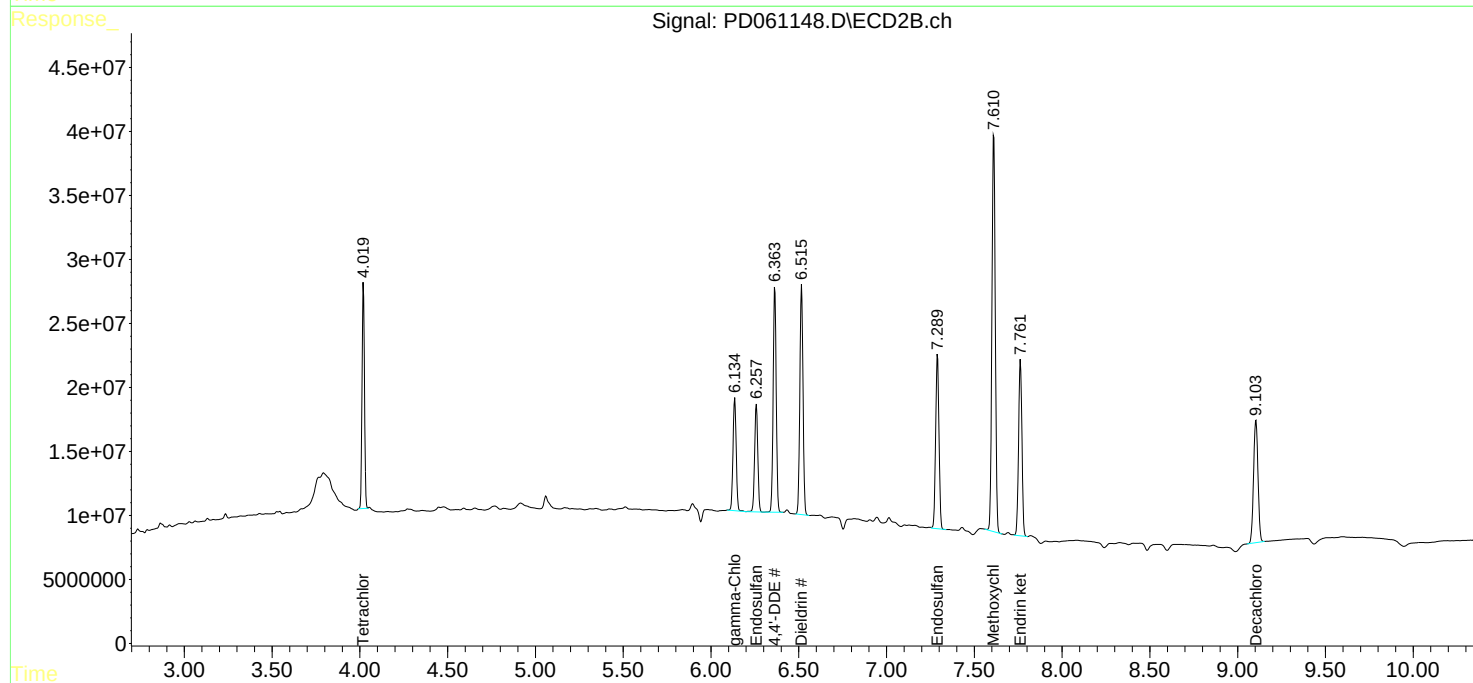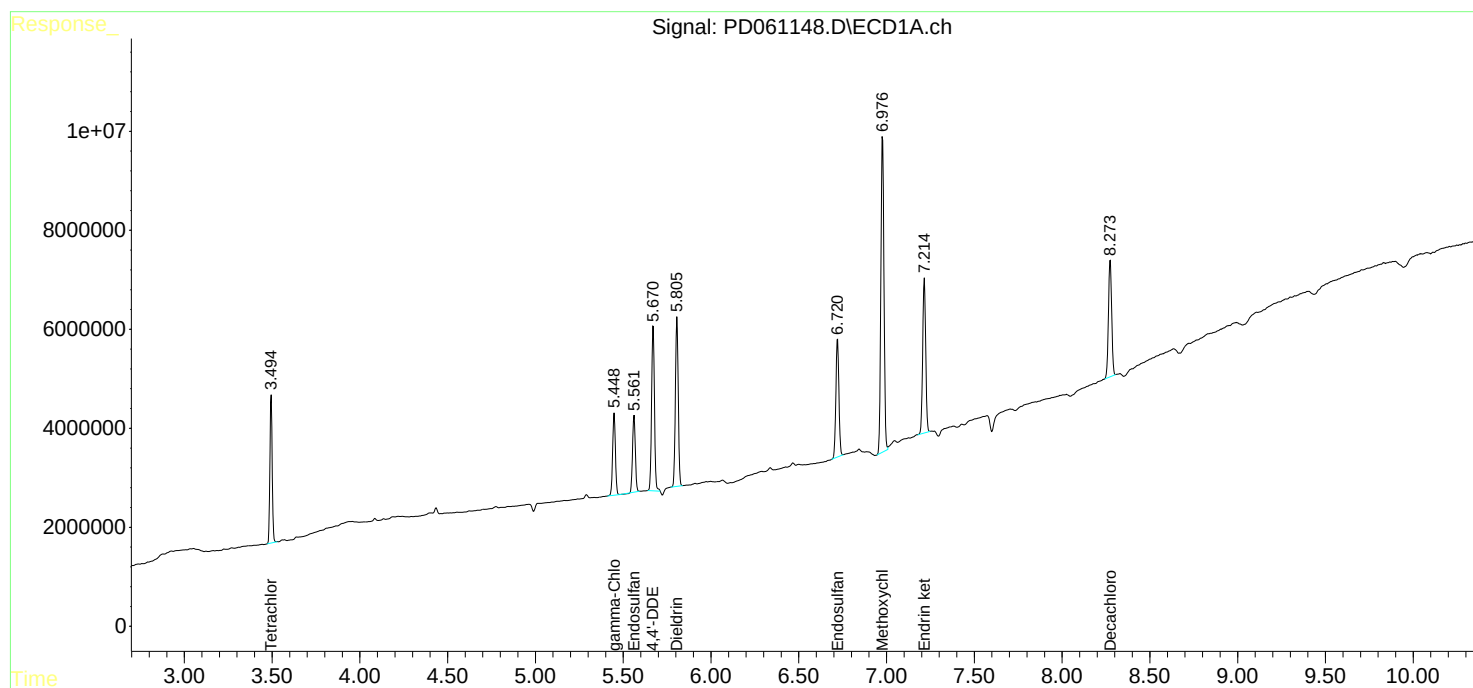


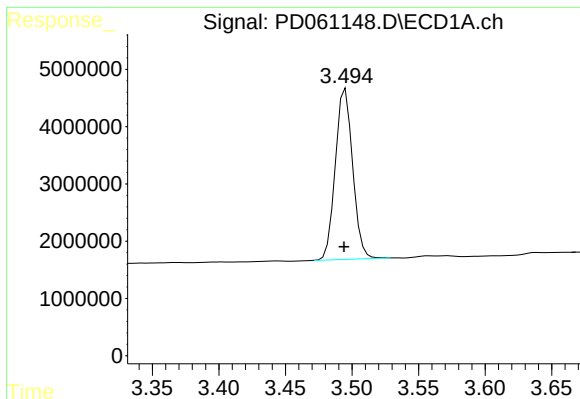

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.001 min
Response: 27041851
Conc: 21.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

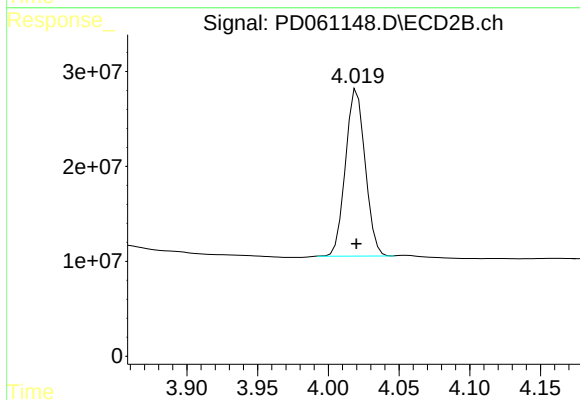


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 170611689
Conc: 21.67 ng/ml

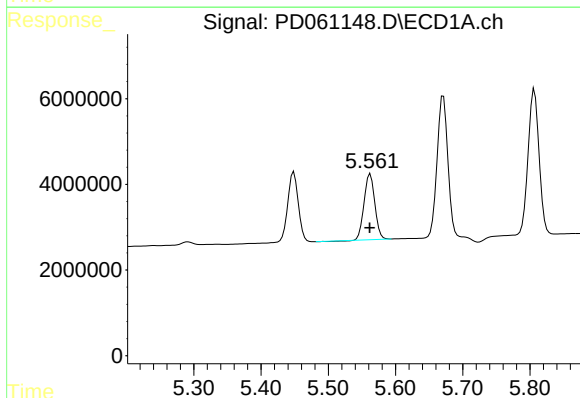


#9 Endosulfan I

R.T.: 5.562 min
Delta R.T.: 0.000 min
Response: 16946190
Conc: 10.22 ng/ml

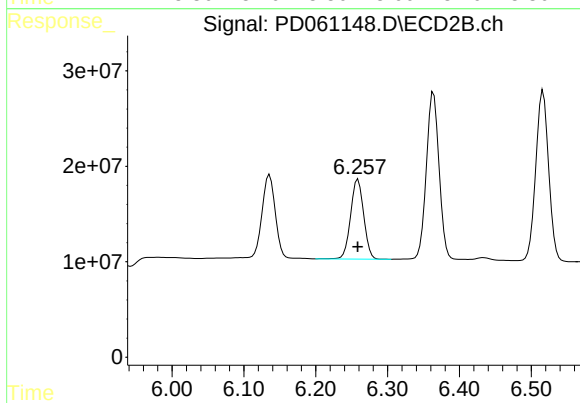

#9 Endosulfan I


R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 105807781
Conc: 10.75 ng/ml

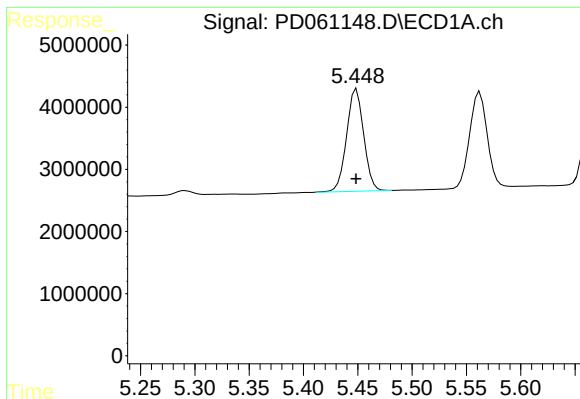

#10 gamma-Chlordane


R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 18057766
Conc: 10.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

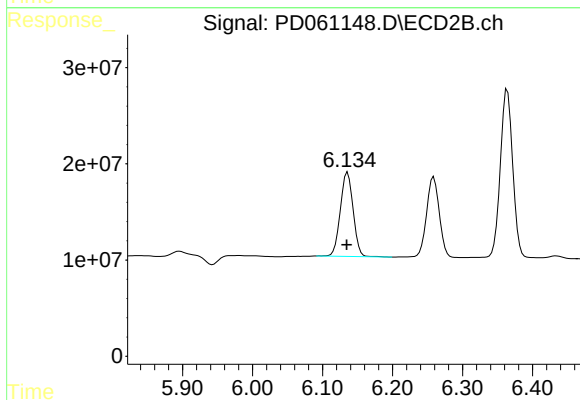


#10 gamma-Chlordane

R.T.: 6.136 min
Delta R.T.: 0.001 min
Response: 111352159
Conc: 10.48 ng/ml

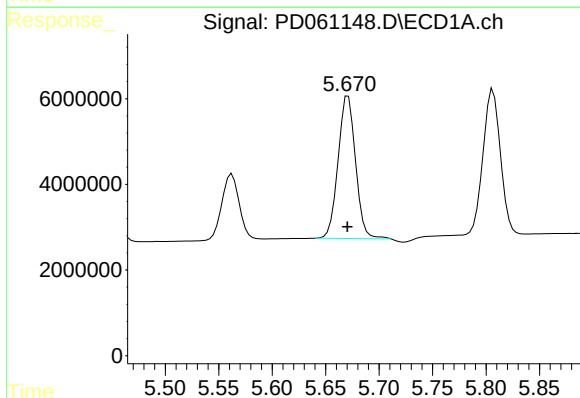


#12 4,4'-DDE

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 37855695
Conc: 21.29 ng/ml

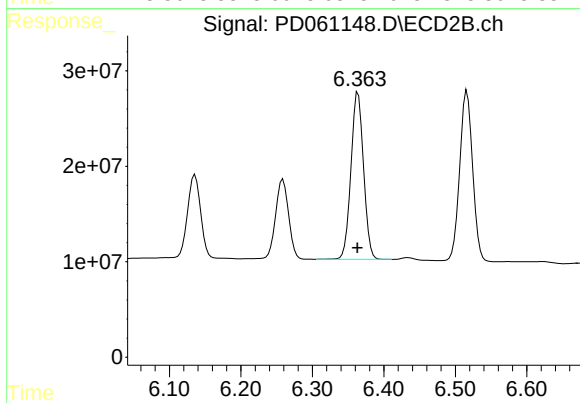

#12 4,4'-DDE


R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 214804223
Conc: 20.98 ng/ml

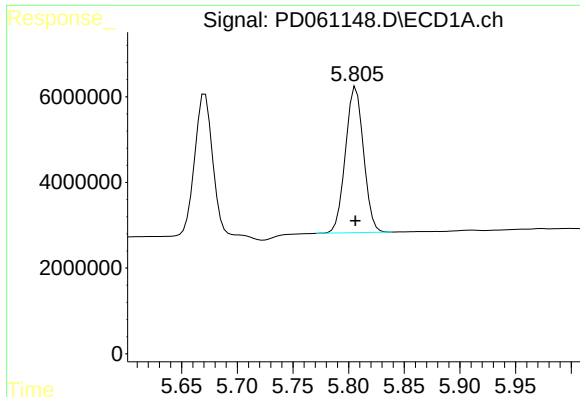

#13 Dieldrin


R.T.: 5.807 min
Delta R.T.: 0.000 min
Response: 38507049
Conc: 20.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

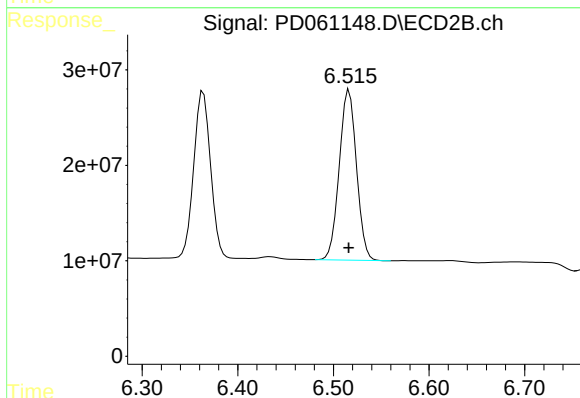


#13 Dieldrin

R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 224039386
Conc: 21.32 ng/ml

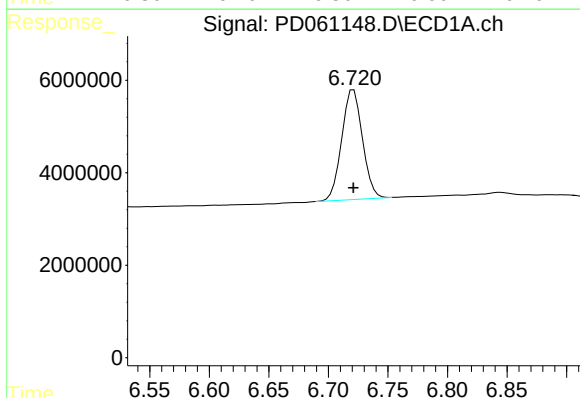


#19 Endosulfan Sulfate

R.T.: 6.721 min
Delta R.T.: 0.000 min
Response: 28743018
Conc: 19.81 ng/ml

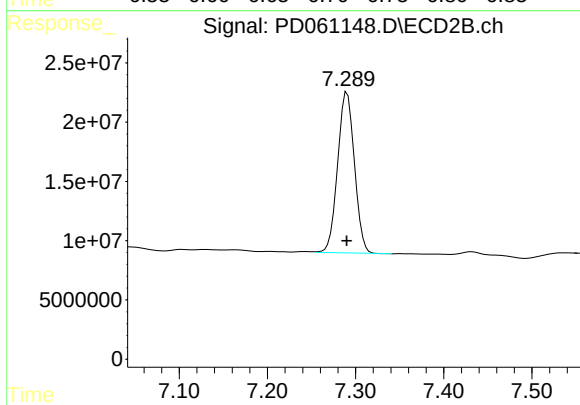

#19 Endosulfan Sulfate


R.T.: 7.290 min
Delta R.T.: 0.000 min
Response: 179210692
Conc: 20.76 ng/ml

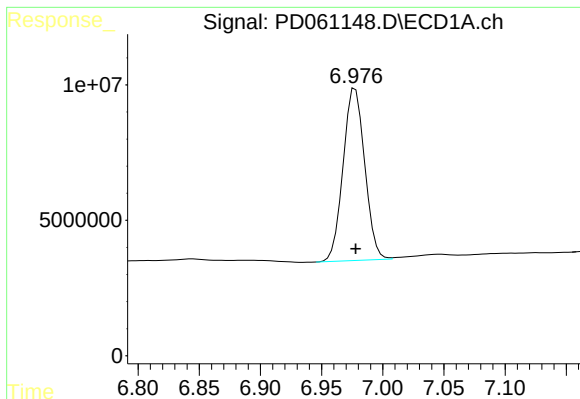

#20 Methoxychlor


R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 78220493
Conc: 102.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

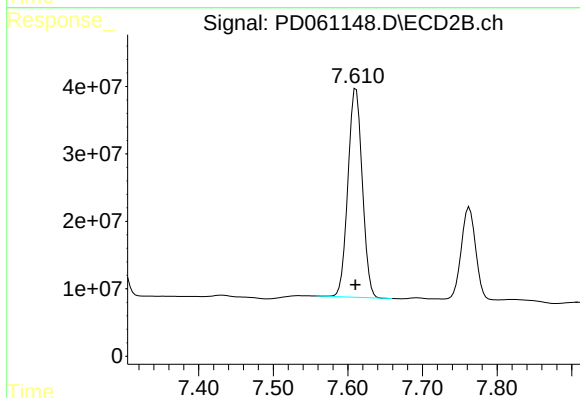


#20 Methoxychlor

R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 413017853
Conc: 98.40 ng/ml

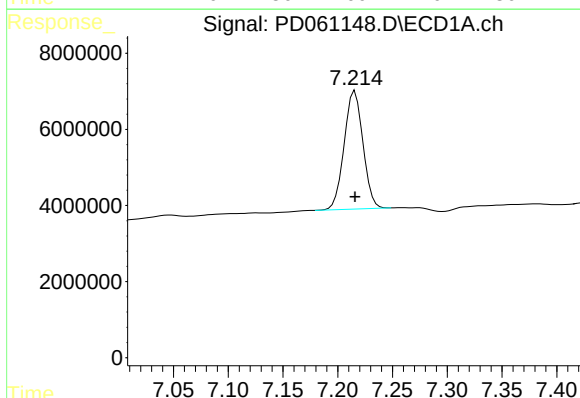


#21 Endrin ketone

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 37083809
Conc: 20.05 ng/ml

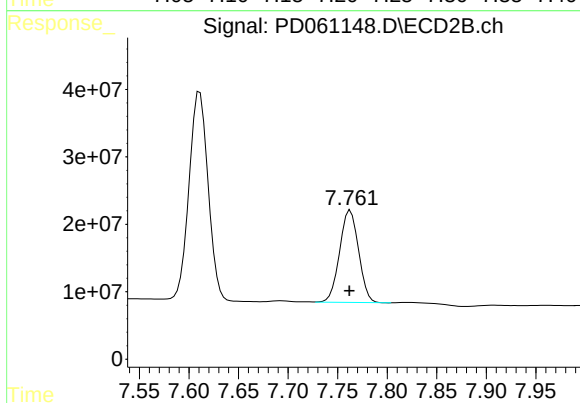

#21 Endrin ketone


R.T.: 7.763 min
Delta R.T.: 0.000 min
Response: 182349794
Conc: 20.63 ng/ml

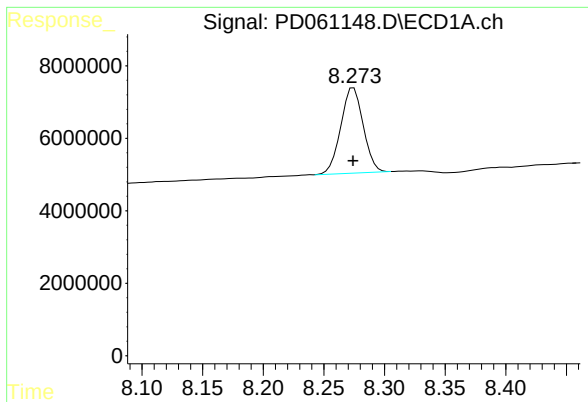

#28 Decachlorobiphenyl

R.T.: 8.275 min
Delta R.T.: 0.000 min
Response: 30266715
Conc: 21.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

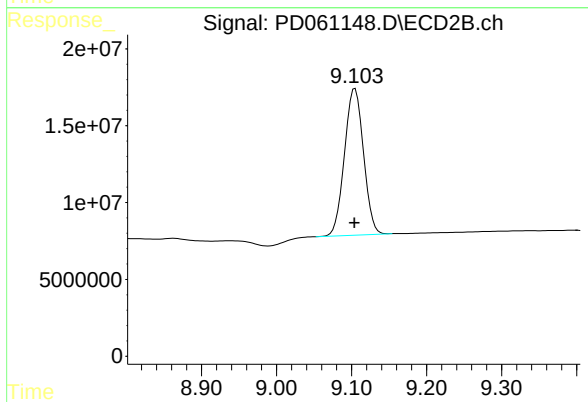

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 168379271
Conc: 22.09 ng/ml