

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
 Data File : PD061154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 17:00
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:55:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 10 02:53:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.020	132.2E6	705.5E6	97.682	96.827
28)	SA Decachlor...	8.274	9.103	127.5E6	640.6E6	98.159	95.637
Target Compounds							
23)	Chlordane-1	4.371	5.018	41055068	294.2E6	966.192	972.416
24)	Chlordane-2	4.876	5.487	43398479	276.3E6	962.593	962.111
25)	Chlordane-3	5.449	6.135	141.0E6	1173.8E6	976.568	975.756
26)	Chlordane-4	5.507	6.210	113.6E6	1363.1E6	971.075	968.878
27)	Chlordane-5	6.348	7.016	52203637	250.5E6	973.918	975.484



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
Data File : PD061154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 17:00
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:55:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
Quant Title : GC Extractables
QLast Update : Wed Feb 10 02:53:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

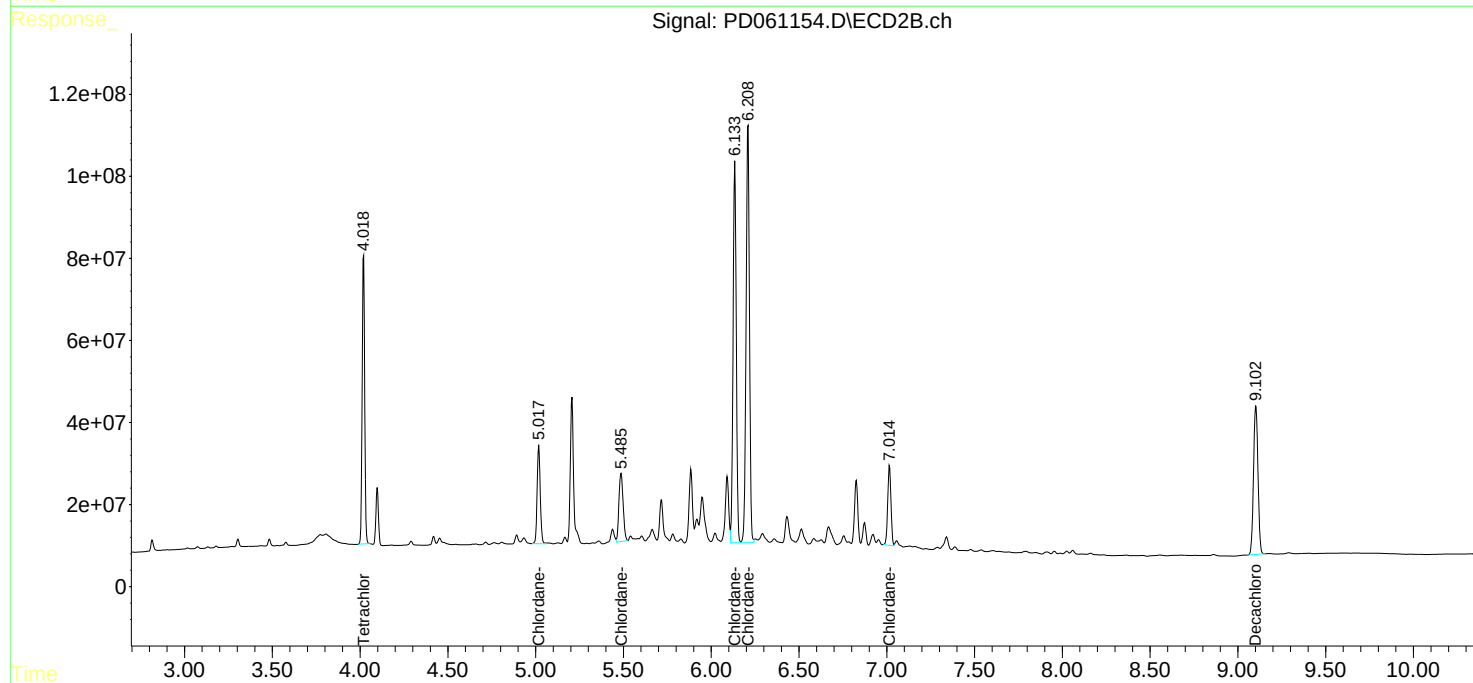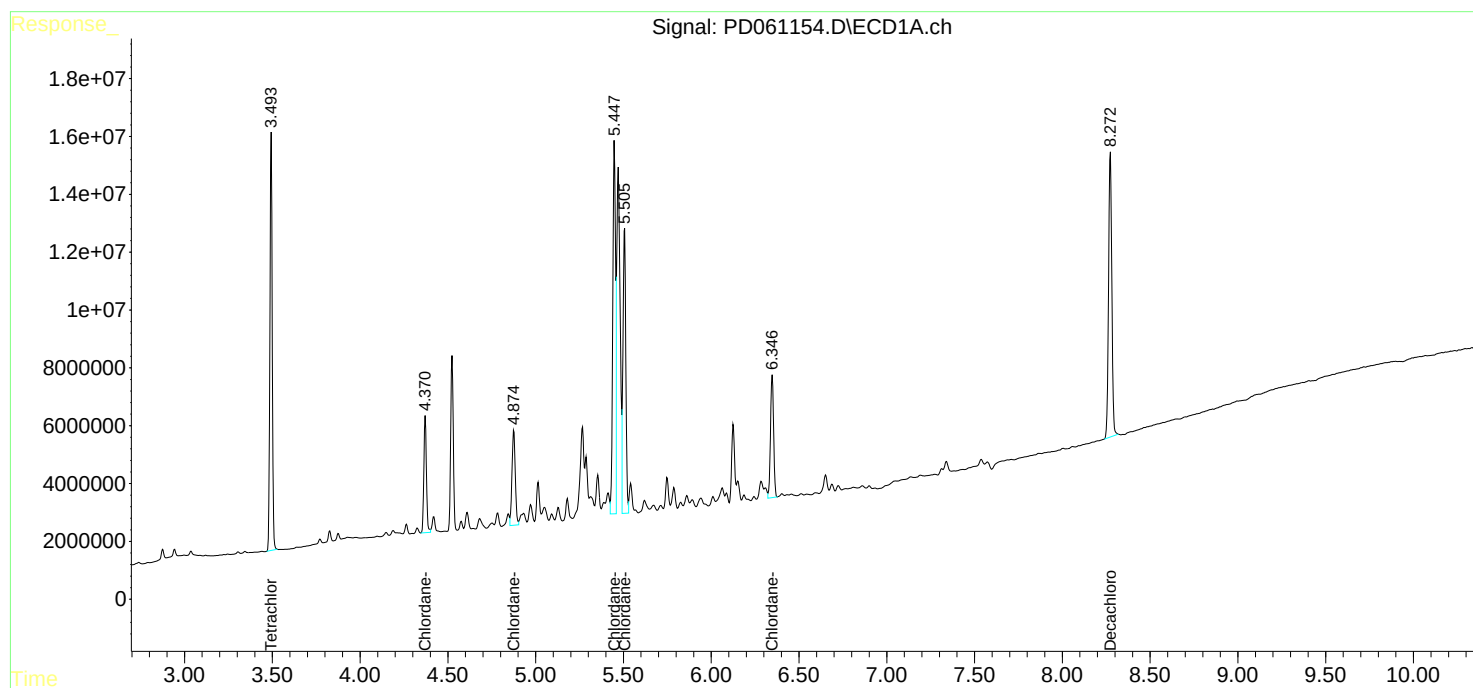


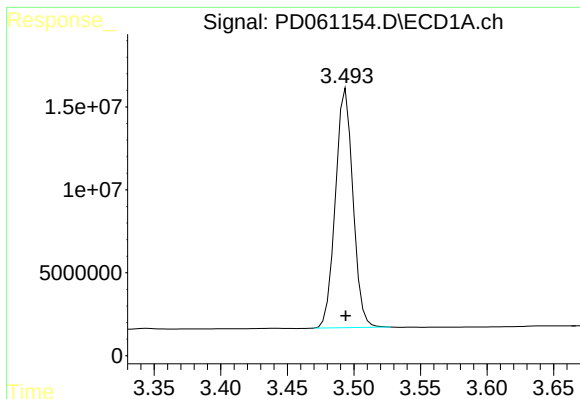

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 132201376
Conc: 97.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

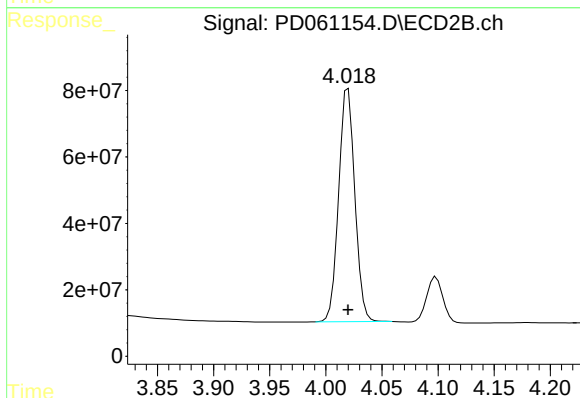


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 705492393
Conc: 96.83 ng/ml

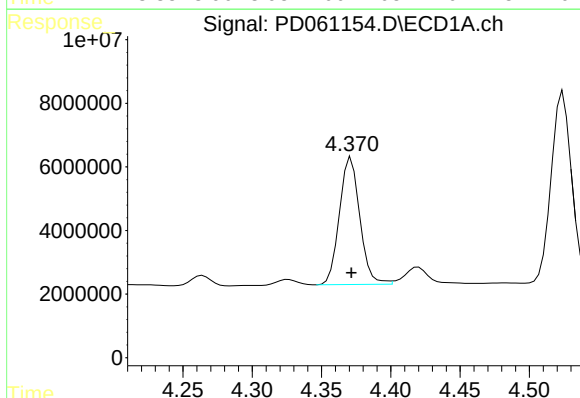


#23 Chlordane-1

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 41055068
Conc: 966.19 ng/ml

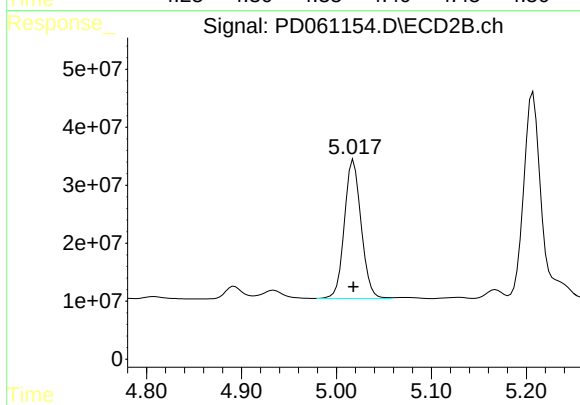

#23 Chlordane-1


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 294151870
Conc: 972.42 ng/ml

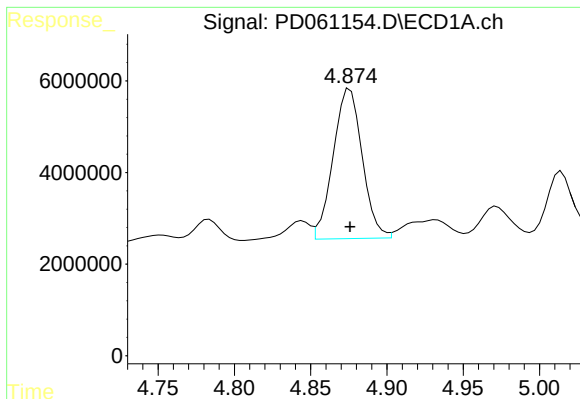

#24 Chlordane-2


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 43398479
Conc: 962.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

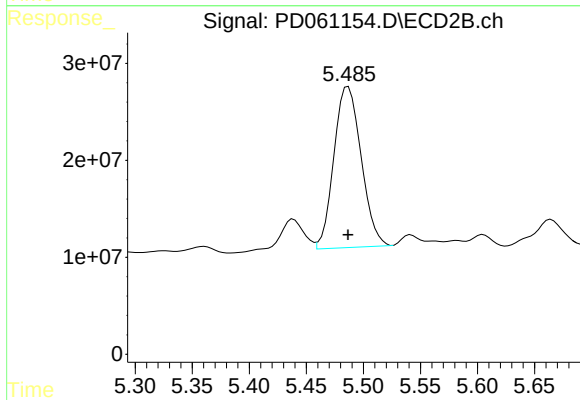


#24 Chlordane-2

R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 276311247
Conc: 962.11 ng/ml

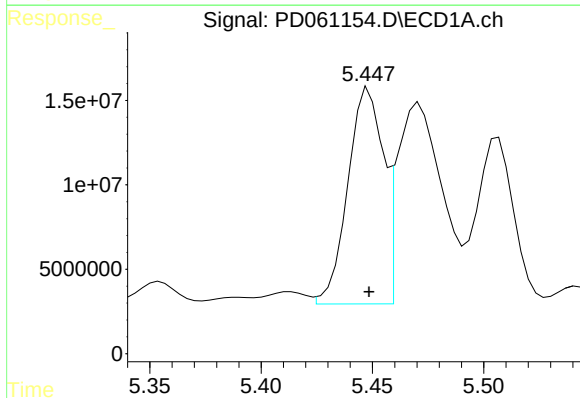


#25 Chlordane-3

R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 141025343
Conc: 976.57 ng/ml

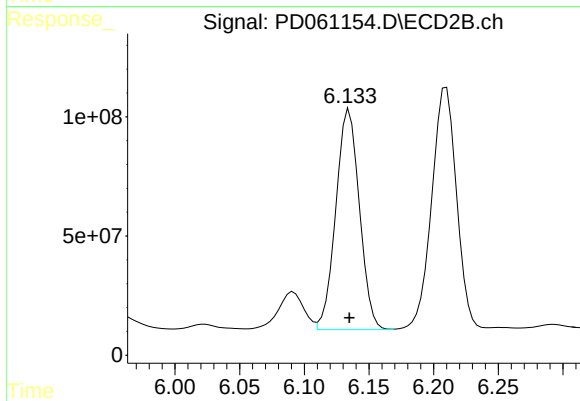

#25 Chlordane-3


R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 1173843652
Conc: 975.76 ng/ml

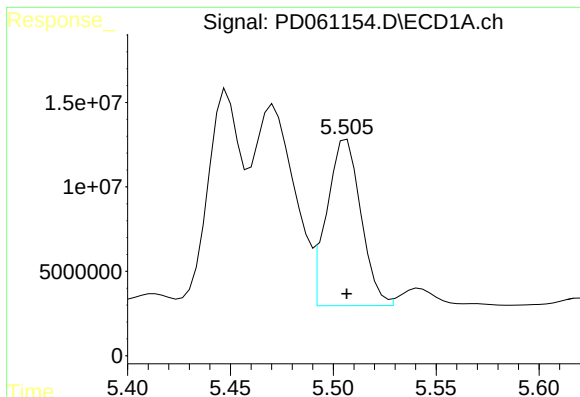

#26 Chlordane-4


R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 113590352
Conc: 971.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

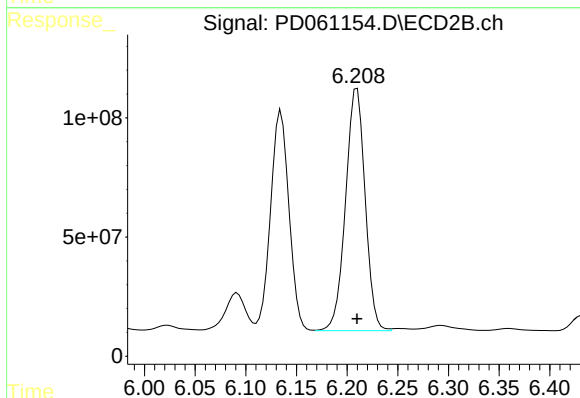


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 1363142513
Conc: 968.88 ng/ml

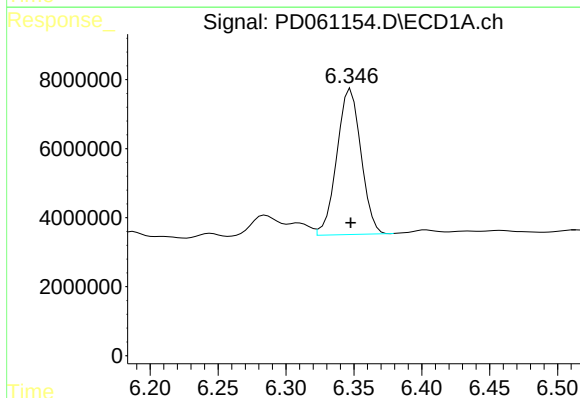


#27 Chlordane-5

R.T.: 6.348 min
Delta R.T.: 0.000 min
Response: 52203637
Conc: 973.92 ng/ml

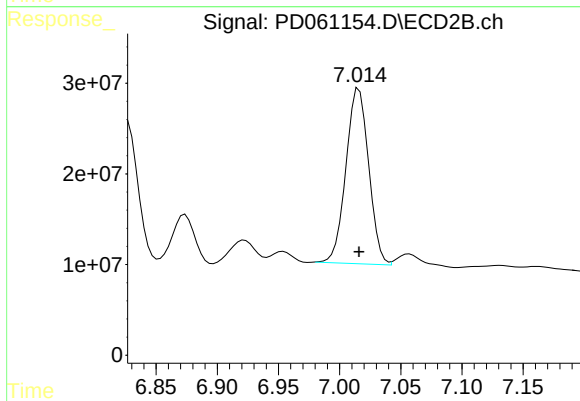

#27 Chlordane-5

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 250485048
Conc: 975.48 ng/ml

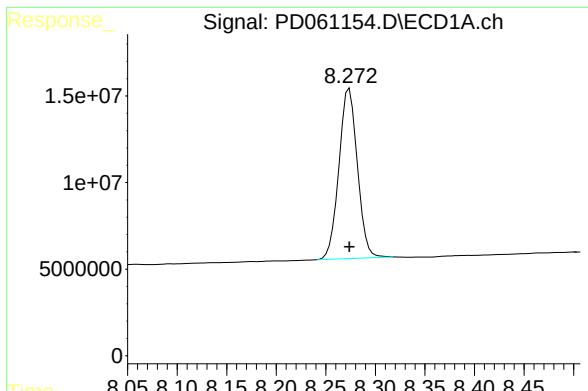

#28 Decachlorobiphenyl


R.T.: 8.274 min

Delta R.T.: 0.000 min

Response: 127488495

Conc: 98.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

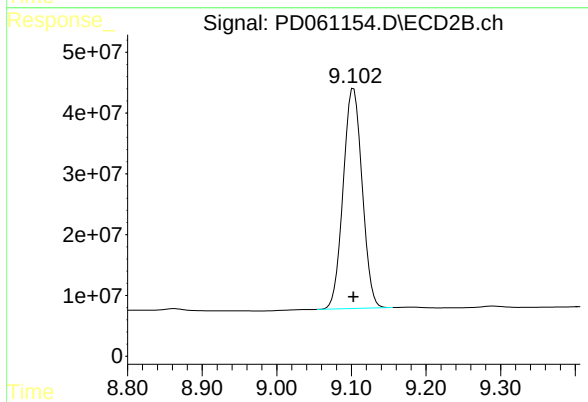

#28 Decachlorobiphenyl

R.T.: 9.103 min

Delta R.T.: 0.000 min

Response: 640553671

Conc: 95.64 ng/ml