

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
 Data File : PD061155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 17:14
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:57:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 10 02:53:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.020	98769730	529.5E6	73.641	73.433
28)	SA Decachlor...	8.274	9.104	96476286	476.6E6	74.519	72.398
Target Compounds							
23)	Chlordane-1	4.372	5.018	30804582	219.0E6	733.116	732.558
24)	Chlordane-2	4.876	5.487	32566577	210.7E6	731.329	738.935
25)	Chlordane-3	5.449	6.135	104.5E6	886.1E6	732.342	740.995
26)	Chlordane-4	5.507	6.210	85179387	1023.6E6	735.319	734.856
27)	Chlordane-5	6.348	7.016	36834886	189.0E6	706.929	740.557



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
Data File : PD061155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 17:14
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:57:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
Quant Title : GC Extractables
QLast Update : Wed Feb 10 02:53:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

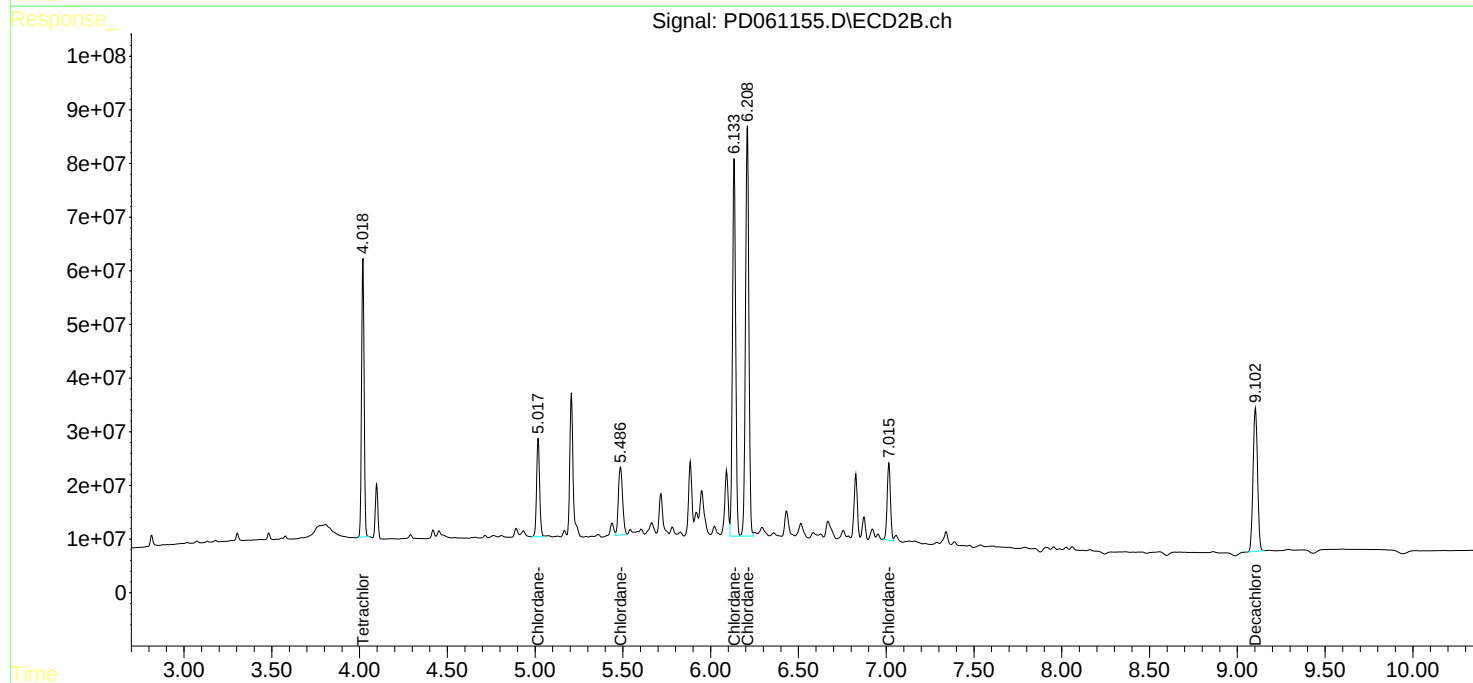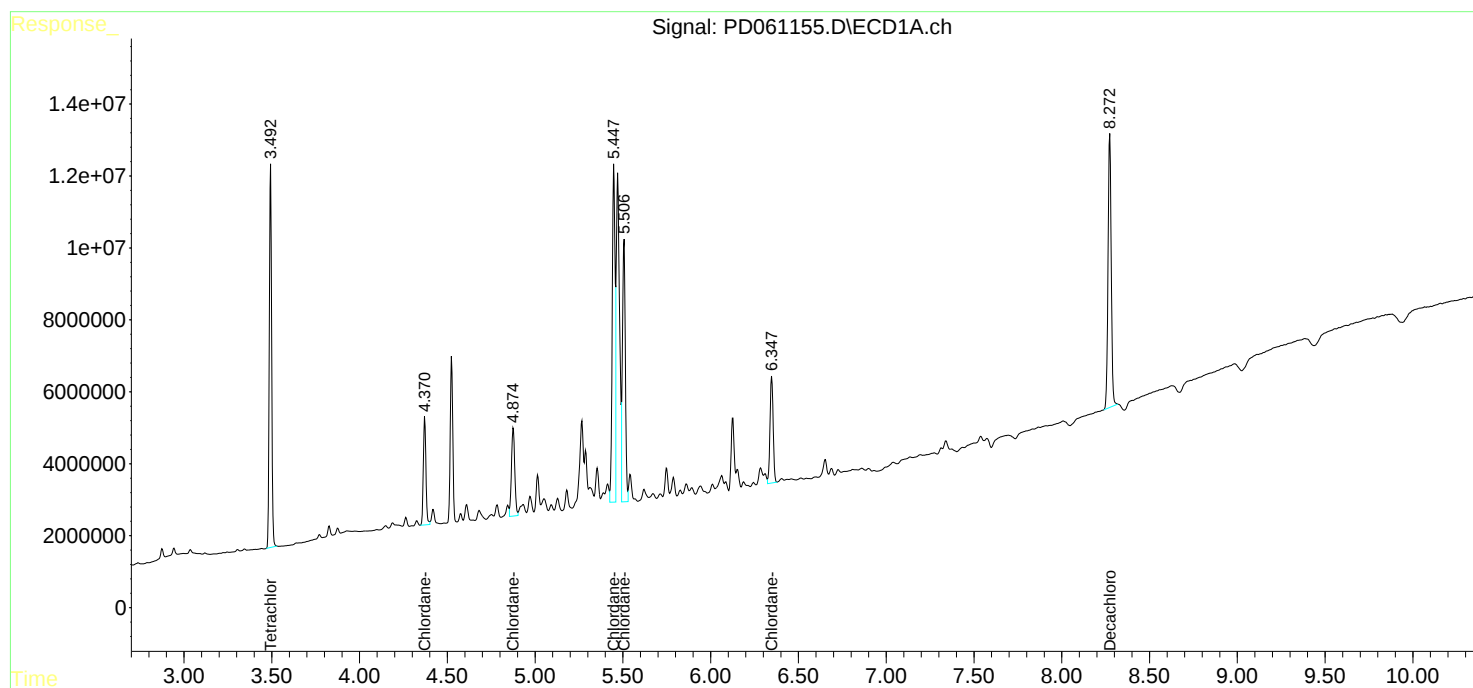


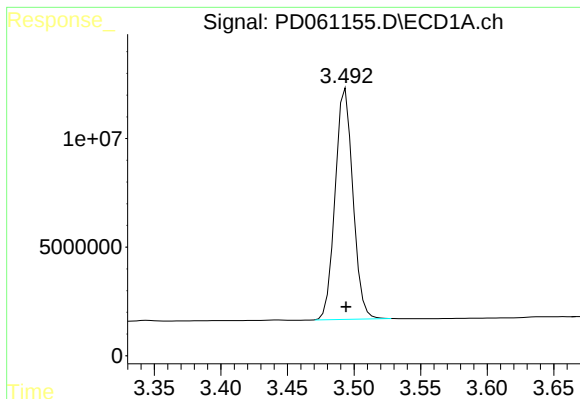

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 98769730
Conc: 73.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

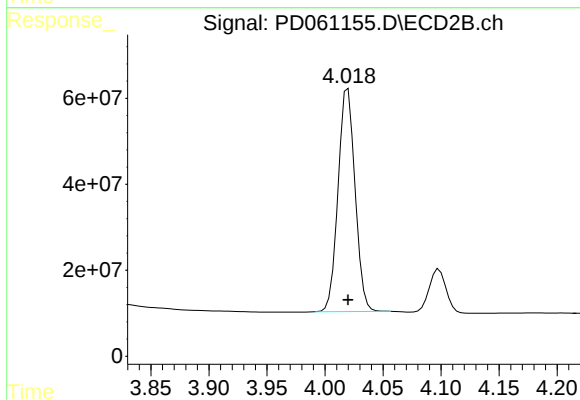


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 529504776
Conc: 73.43 ng/ml

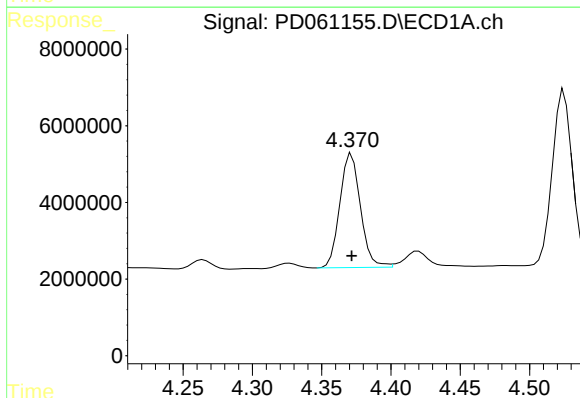


#23 Chlordane-1

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 30804582
Conc: 733.12 ng/ml

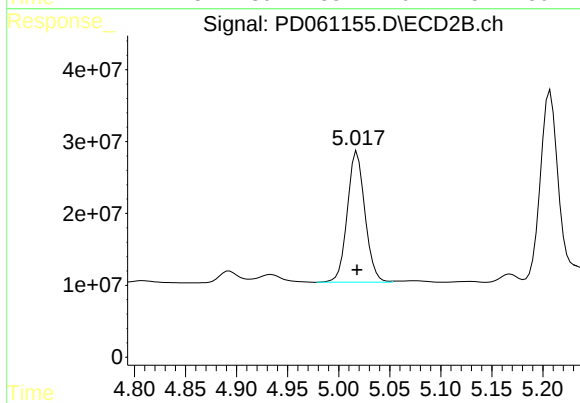

#23 Chlordane-1


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 219048759
Conc: 732.56 ng/ml

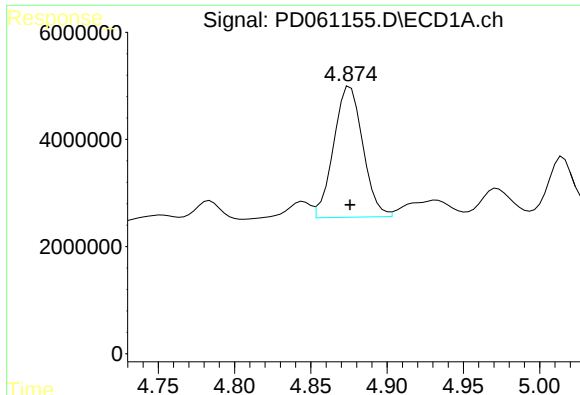

#24 Chlordane-2


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 32566577
Conc: 731.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

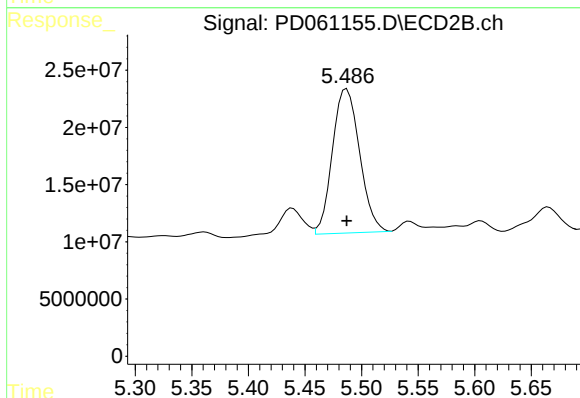


#24 Chlordane-2

R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 210662536
Conc: 738.93 ng/ml

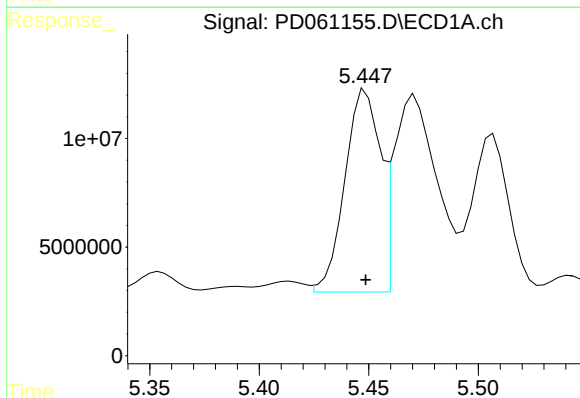


#25 Chlordane-3

R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 104526479
Conc: 732.34 ng/ml

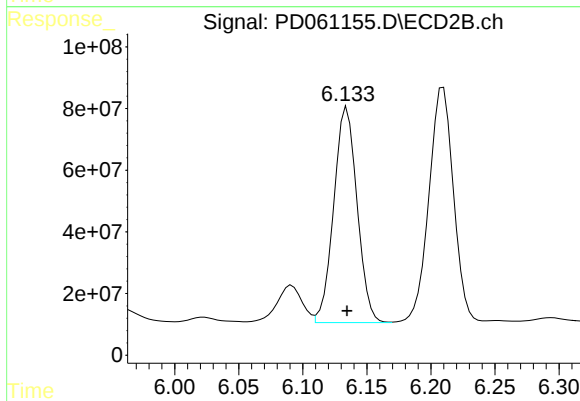

#25 Chlordane-3


R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 886104065
Conc: 740.99 ng/ml

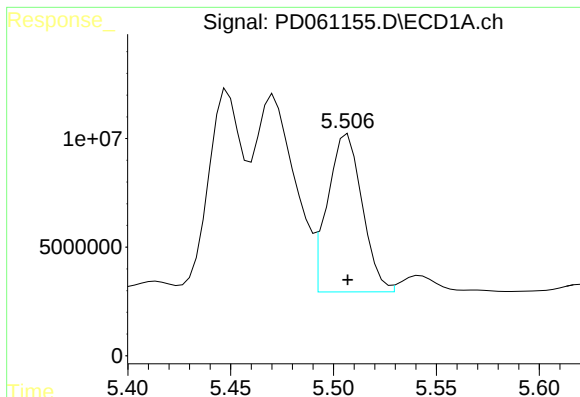

#26 Chlordane-4


R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 85179387
Conc: 735.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

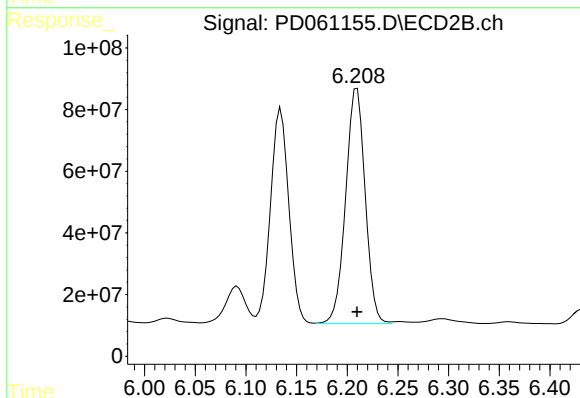


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 1023557522
Conc: 734.86 ng/ml

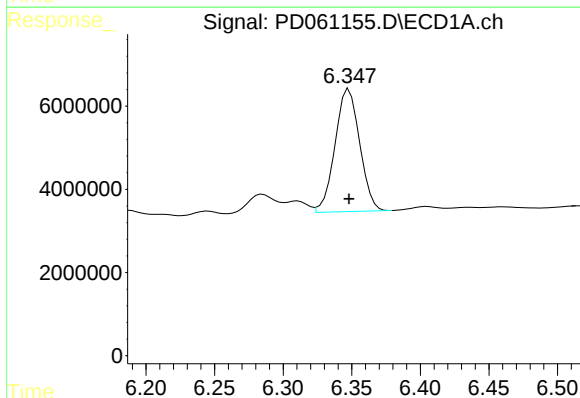


#27 Chlordane-5

R.T.: 6.348 min
Delta R.T.: 0.000 min
Response: 36834886
Conc: 706.93 ng/ml

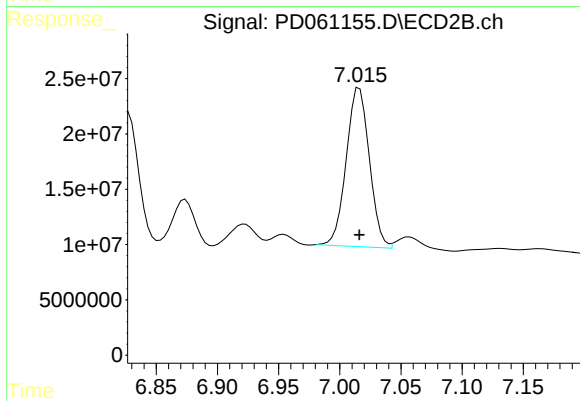

#27 Chlordane-5

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 188970611
Conc: 740.56 ng/ml

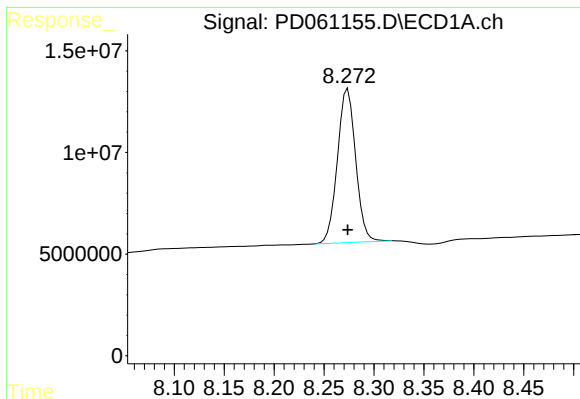

#28 Decachlorobiphenyl


R.T.: 8.274 min

Delta R.T.: 0.000 min

Response: 96476286

Conc: 74.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

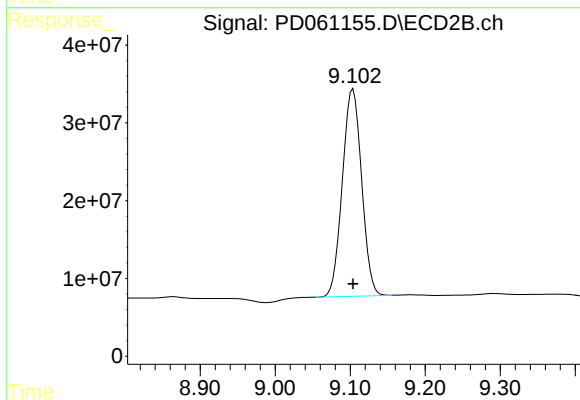

#28 Decachlorobiphenyl

R.T.: 9.104 min

Delta R.T.: 0.000 min

Response: 476636242

Conc: 72.40 ng/ml