

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
 Data File : PD061156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 17:28
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:53:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 10 02:53:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.020	69237311	375.9E6	50.000	50.000
28)	SA Decachlor...	8.275	9.104	66135661	349.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.372	5.019	21964089	155.4E6	500.000	500.000
24)	Chlordane-2	4.876	5.487	23385751	149.0E6	500.000	500.000
25)	Chlordane-3	5.449	6.135	73896466	616.1E6	500.000	500.000
26)	Chlordane-4	5.508	6.210	60178593	725.4E6	500.000	500.000
27)	Chlordane-5	6.349	7.016	27499858	131.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020921\
Data File : PD061156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 17:28
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:53:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020921.M
Quant Title : GC Extractables
QLast Update : Wed Feb 10 02:53:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

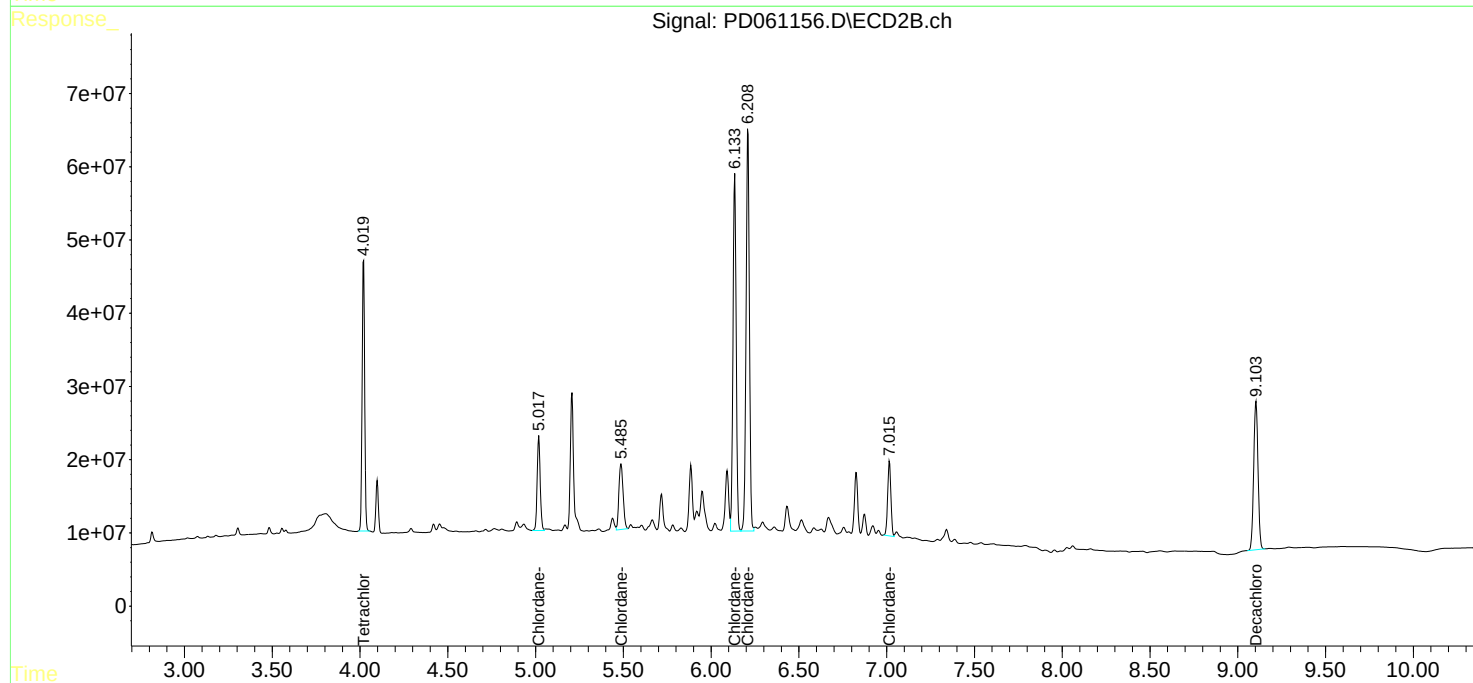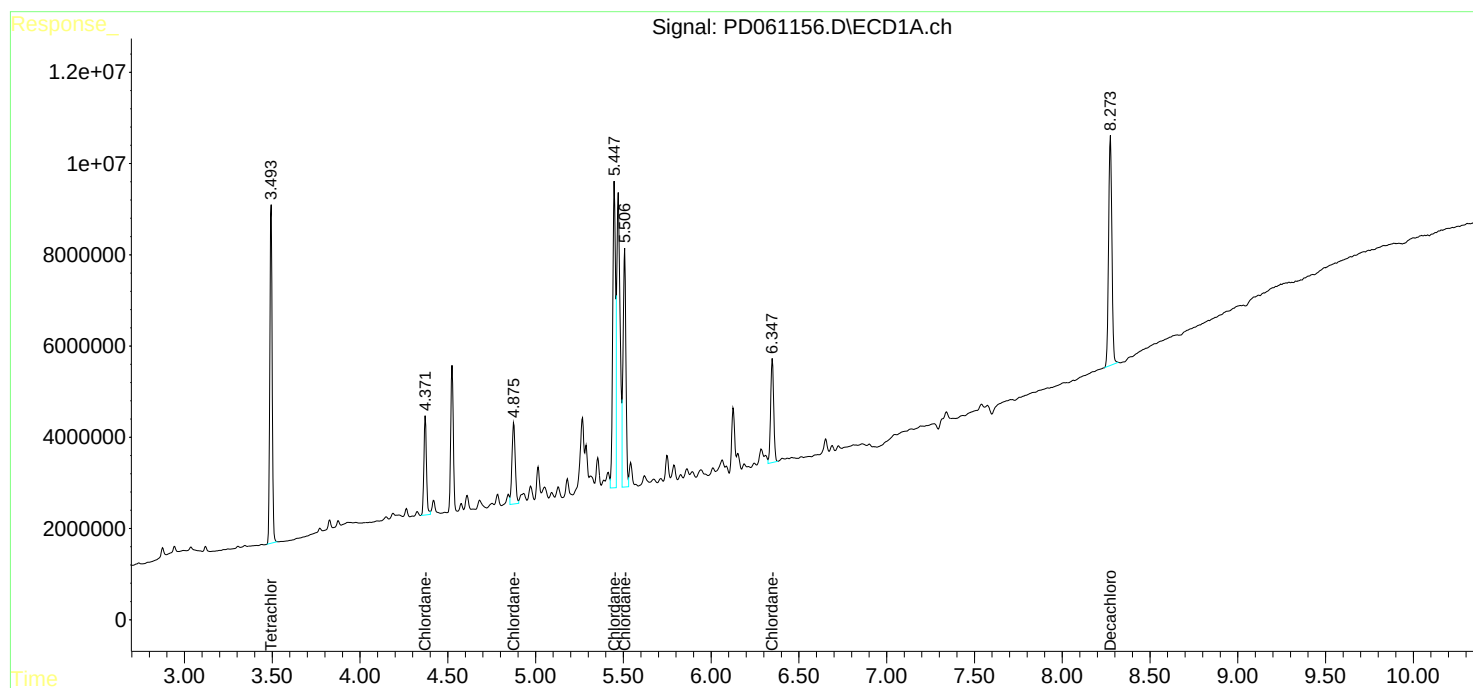


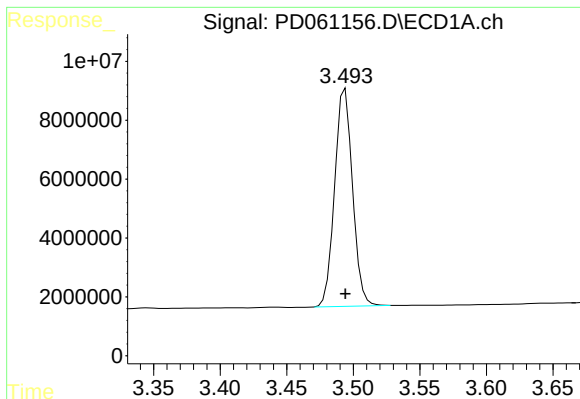

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 69237311
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

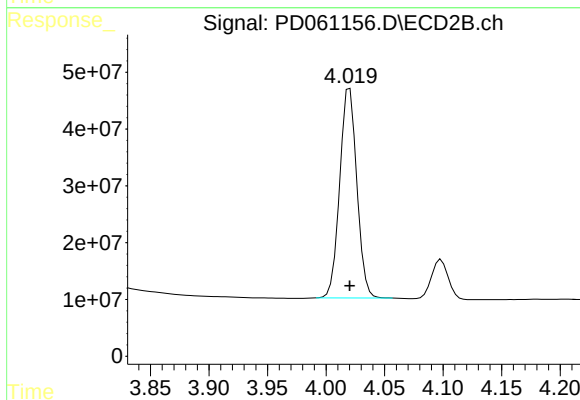


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 375864001
Conc: 50.00 ng/ml

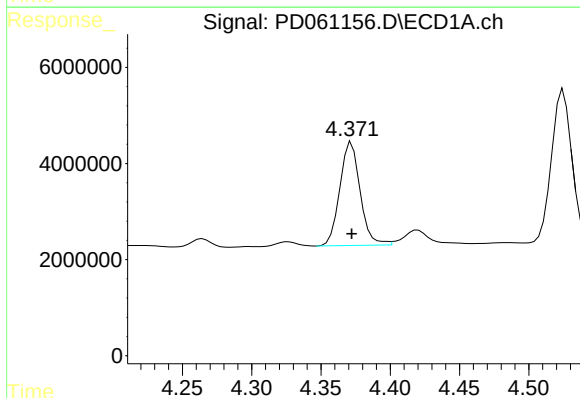


#23 Chlordane-1

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 21964089
Conc: 500.00 ng/ml

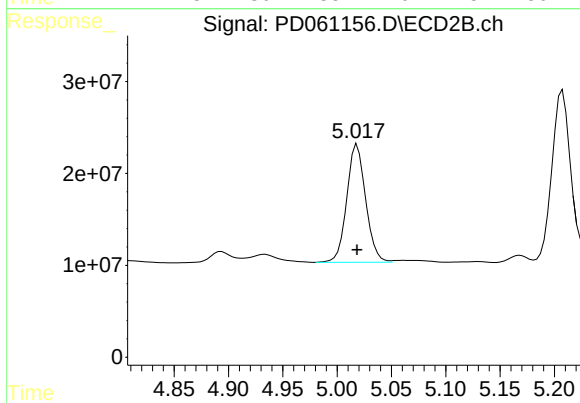

#23 Chlordane-1


R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 155419968
Conc: 500.00 ng/ml

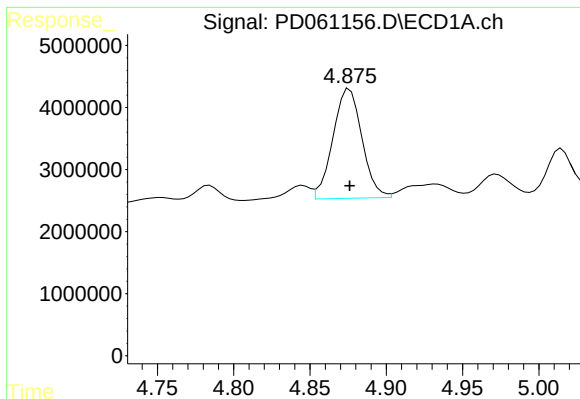

#24 Chlordane-2


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 23385751
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

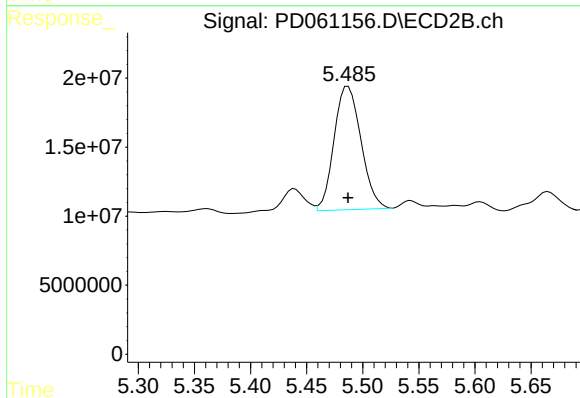


#24 Chlordane-2

R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 149037030
Conc: 500.00 ng/ml

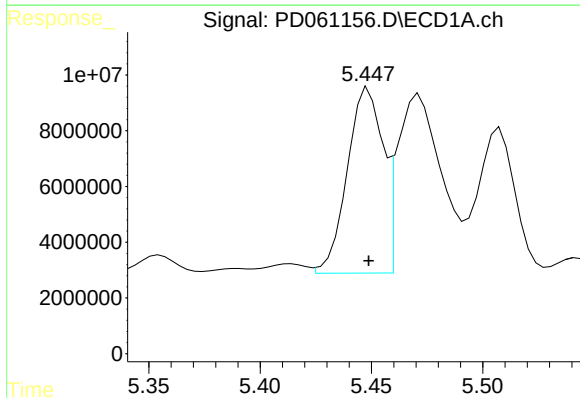


#25 Chlordane-3

R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 73896466
Conc: 500.00 ng/ml

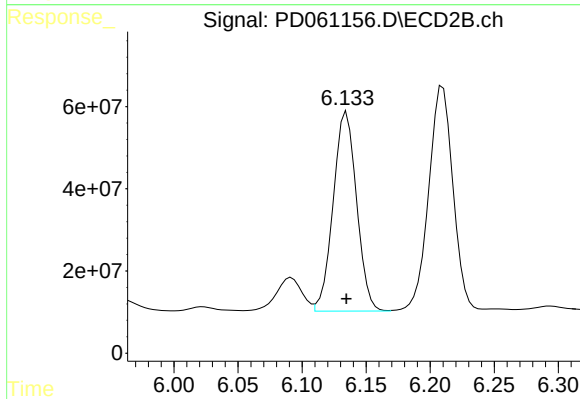

#25 Chlordane-3


R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 616088194
Conc: 500.00 ng/ml

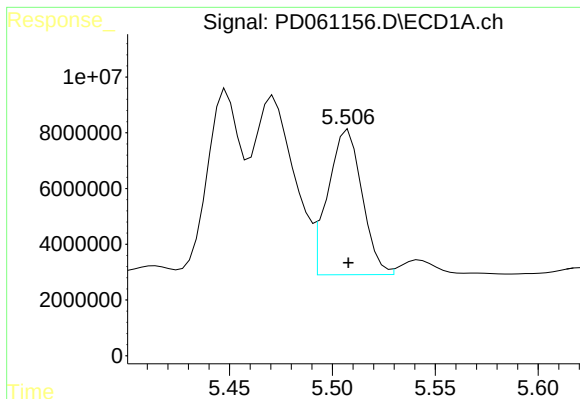

#26 Chlordane-4


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 60178593
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

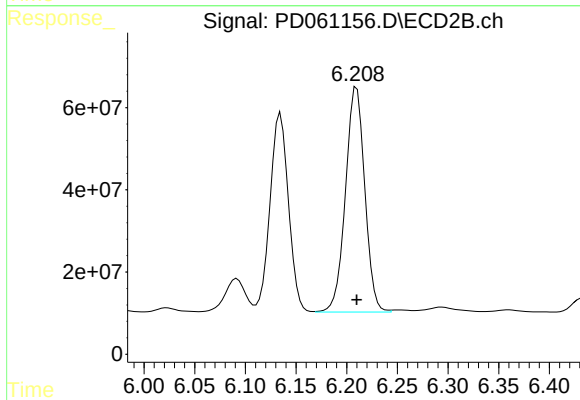


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 725358420
Conc: 500.00 ng/ml

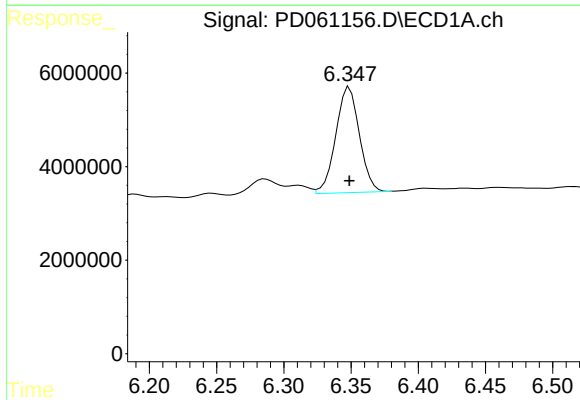


#27 Chlordane-5

R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 27499858
Conc: 500.00 ng/ml

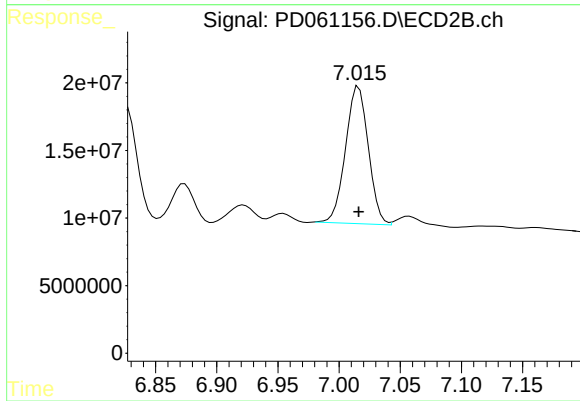

#27 Chlordane-5

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 131537735
Conc: 500.00 ng/ml

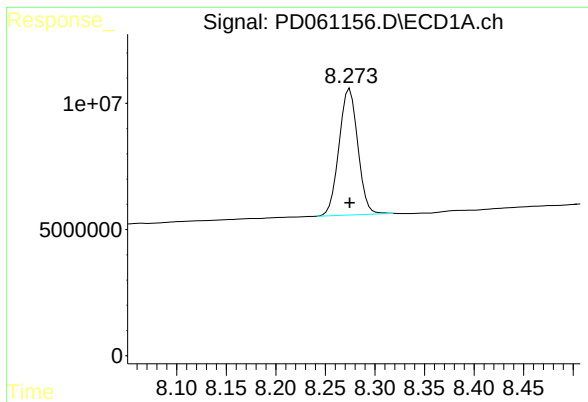

#28 Decachlorobiphenyl


R.T.: 8.275 min

Delta R.T.: 0.000 min

Response: 66135661

Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

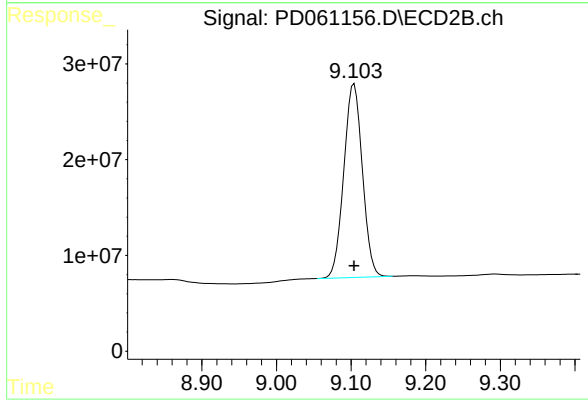

#28 Decachlorobiphenyl

R.T.: 9.104 min

Delta R.T.: 0.000 min

Response: 349499115

Conc: 50.00 ng/ml