

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020922\
 Data File : PD067988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2022 13:45
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5057

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 14:58:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020922CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 09 13:33:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	3.962	150.7E6	734.9E6	74.285	66.416
27)	SA Decachlor...	8.154	9.022	119.7E6	819.1E6	140.507	137.513
Target Compounds							
2)	A alpha-BHC	3.869	4.355	244.0E6	979.5E6	81.348	71.212
3)	MA gamma-BHC...	4.150	4.640	225.8E6	848.6E6	79.077	69.624
4)	MA Heptachlor	4.442	5.139	233.0E6	690.8E6	80.086	68.442
9)	A Endosulfan I	5.463	6.190	186.3E6	489.4E6	78.106	68.525
13)	MA Dieldrin	5.705	6.448	416.7E6	1022.5E6	160.817	141.587
14)	MA Endrin	5.962	6.667	338.1E6	866.8E6	155.702	142.614
16)	A 4,4'-DDD	6.086	6.795	302.5E6	838.3E6	158.374	141.776
17)	MA 4,4'-DDT	6.326	7.091	307.7E6	885.1E6	164.609	145.617
20)	A Methoxychlor	6.873	7.556	632.7E6	2134.7E6	732.869	661.649

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020922\
Data File : PD067988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2022 13:45
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 14:58:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020922CLP.M
Quant Title : GC Extractables
QLast Update : Wed Feb 09 13:33:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

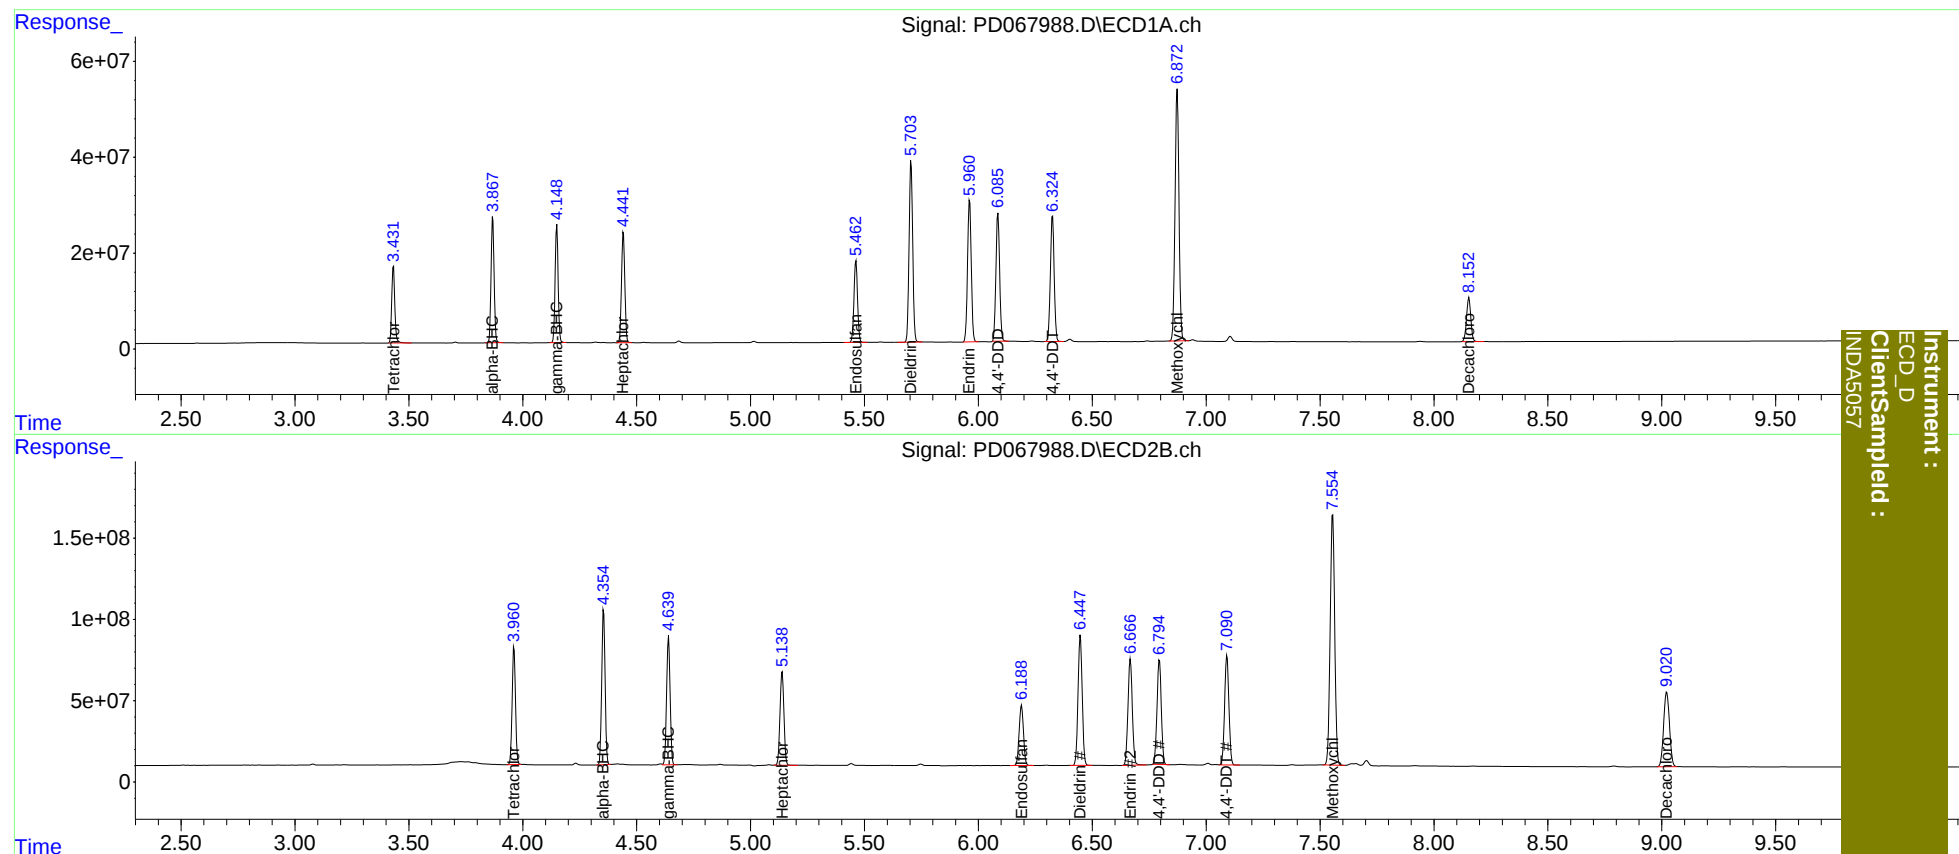

Instrument :
ECD_D
ClientSampled :
INDA5057