

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020923\
 Data File : PD073893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2023 16:23
 Operator : AR\AJ
 Sample : PB150739BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 21:48:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.774	48108932	23750478	20.581	18.656
28)	SA Decachlor...	9.109	7.934	55187552	21976686	19.584	18.889
Target Compounds							
7)	B delta-BHC	4.790	0.000	3445606	0	1.024	N.D. #
8)	B Heptachlo...	5.711	0.000	848470	0	0.266	N.D. #
9)	A Endosulfan I	6.103	0.000	201857	0	0.066	N.D. #
10)	B gamma-Chl...	5.983f	0.000	477487	0	0.145	N.D. #
11)	B alpha-Chl...	6.040	0.000	107247	0	0.033	N.D. #
18)	B Endrin al...	6.978f	6.140f	134293	155662	0.062	0.176 #
19)	B Endosulfa...	7.190	0.000	136440	0	0.051	N.D. #
25)	Chlordane-3	5.983f	0.000	477487	0	1.020	N.D. #
26)	Chlordane-4	6.040	0.000	107247	0	0.187	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020923\
Data File : PD073893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2023 16:23
Operator : AR\AJ
Sample : PB150739BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 21:48:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

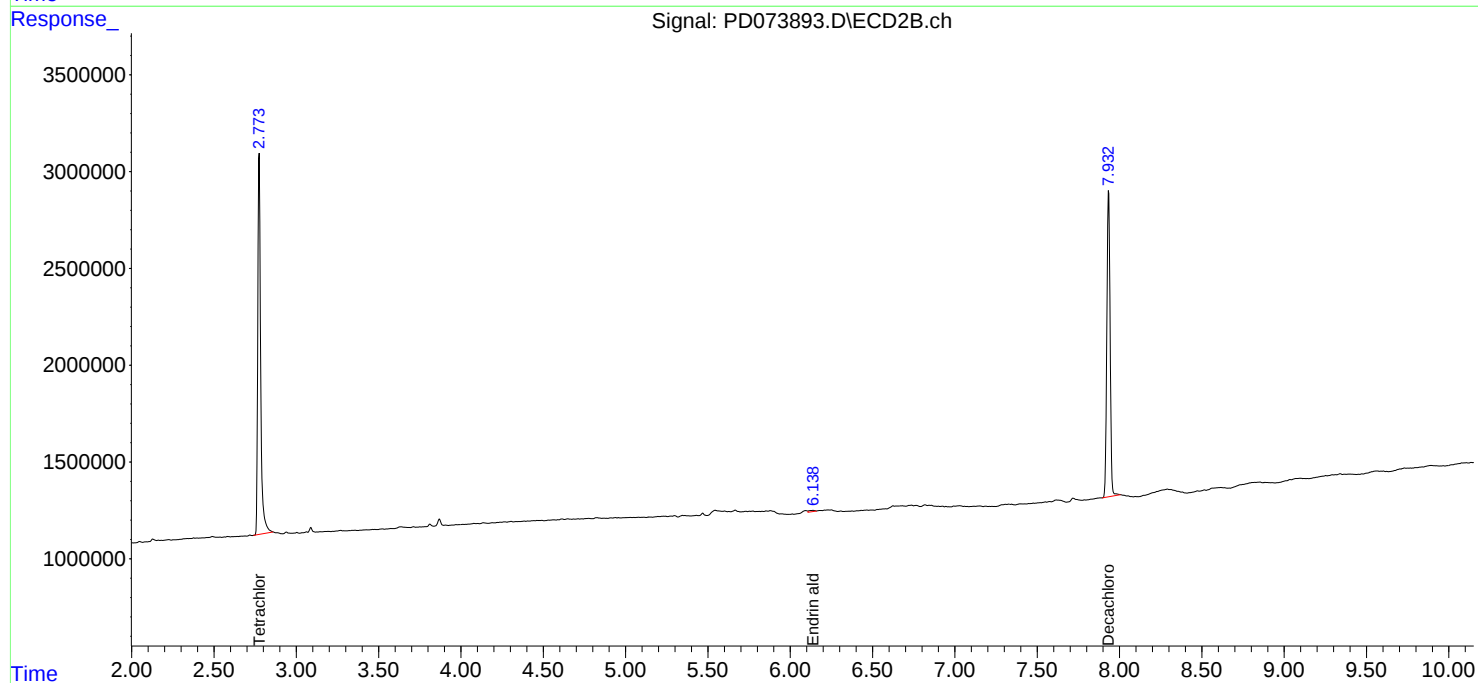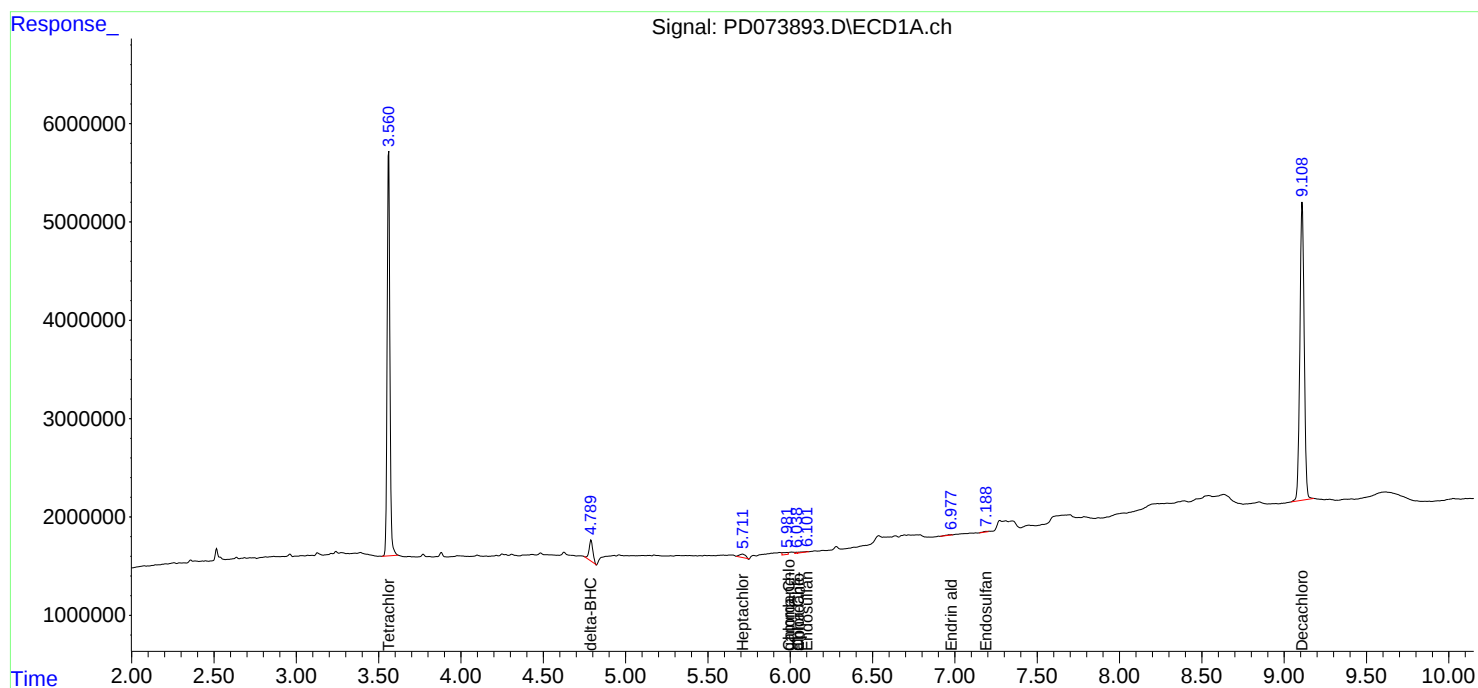


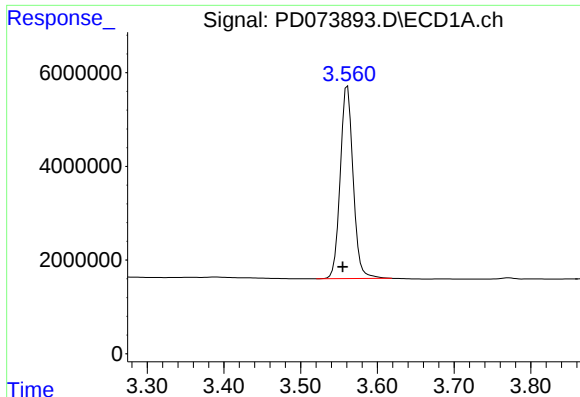

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.006 min
Response: 48108932
Conc: 20.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

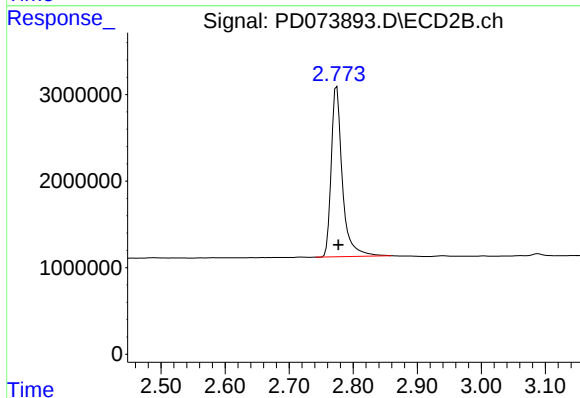


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: -0.002 min
Response: 23750478
Conc: 18.66 ng/ml

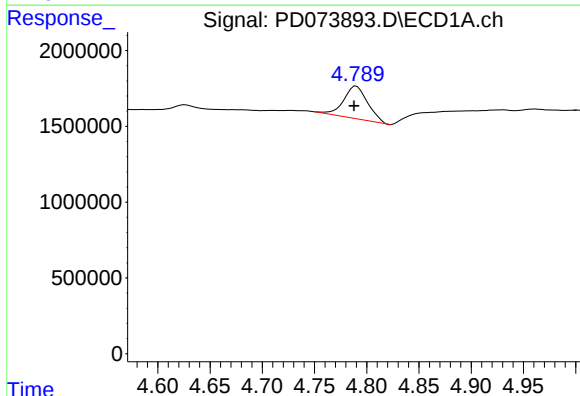


#7 delta-BHC

R.T.: 4.790 min
Delta R.T.: 0.002 min
Response: 3445606
Conc: 1.02 ng/ml

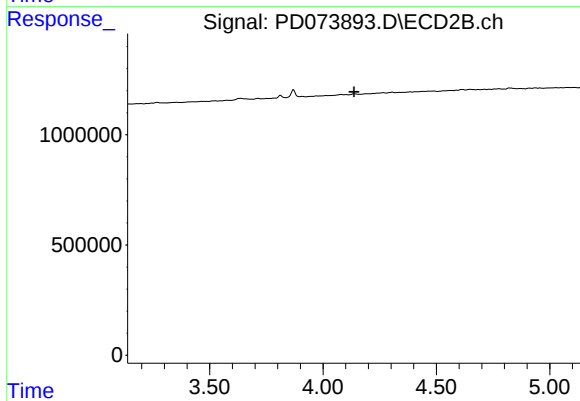

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

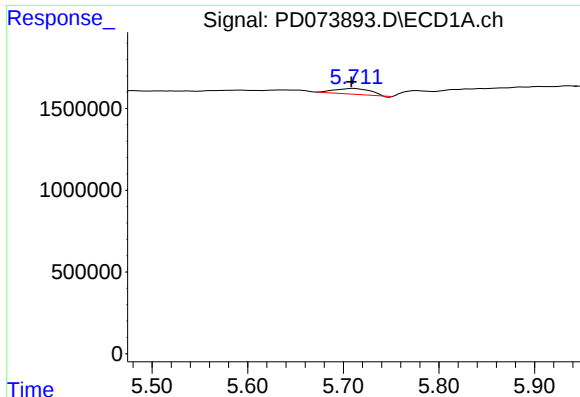

#8 Heptachlor epoxide


R.T.: 5.711 min
Delta R.T.: 0.003 min
Response: 848470
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

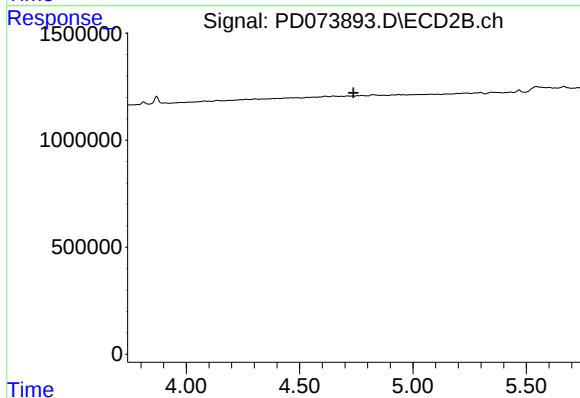


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

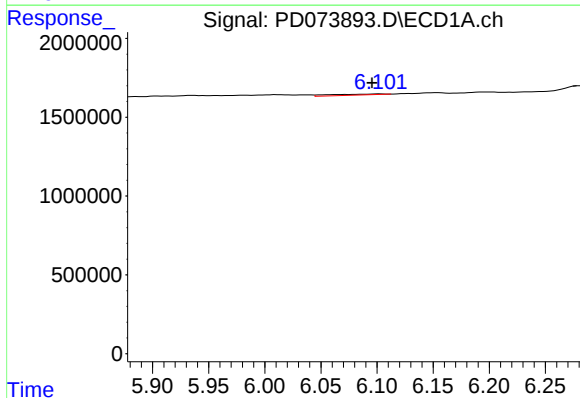


#9 Endosulfan I

R.T.: 6.103 min
Delta R.T.: 0.007 min
Response: 201857
Conc: 0.07 ng/ml

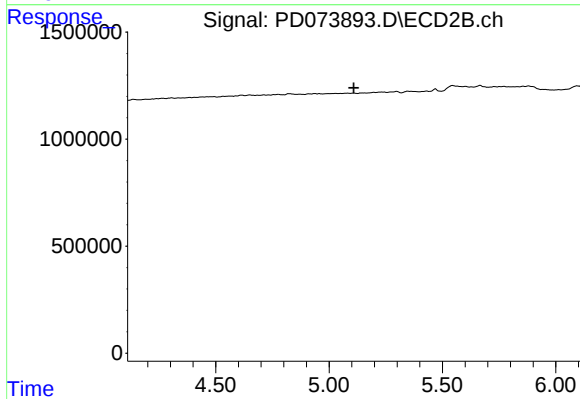

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

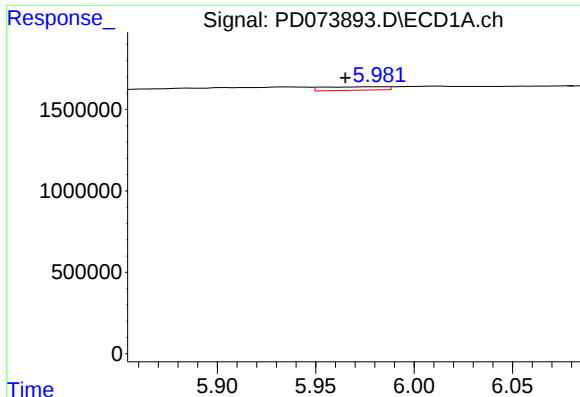

#10 gamma-Chlordane


R.T.: 5.983 min
Delta R.T.: 0.018 min
Response: 477487
Conc: 0.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

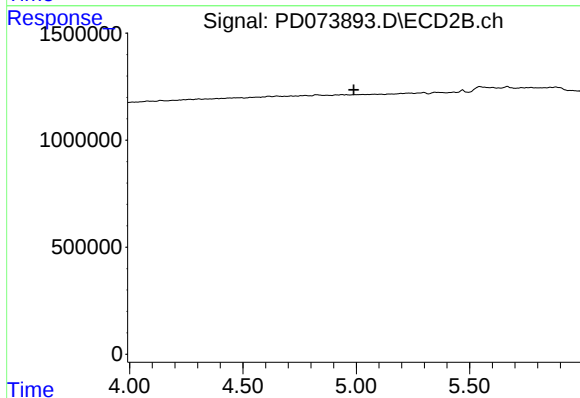


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

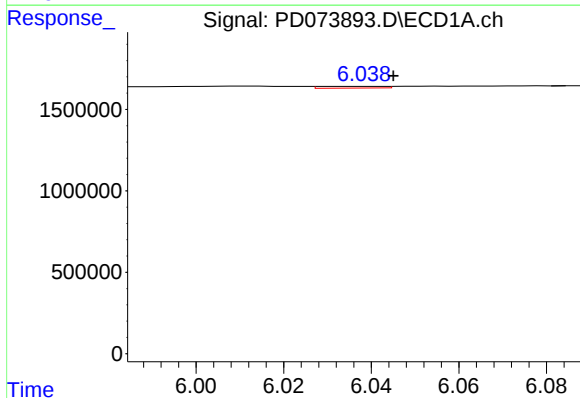


#11 alpha-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.005 min
Response: 107247
Conc: 0.03 ng/ml

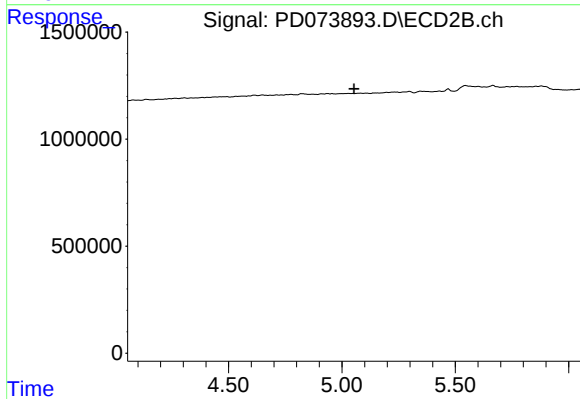

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

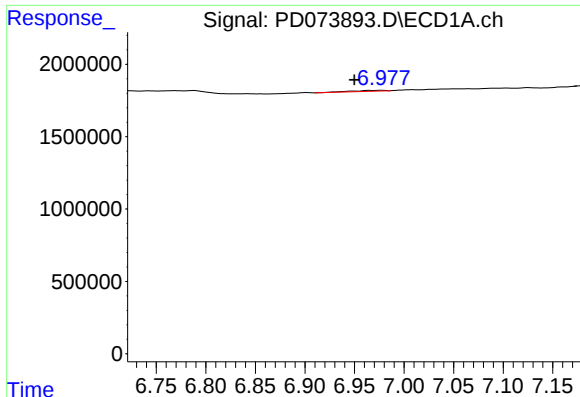

#18 Endrin aldehyde


R.T.: 6.978 min
Delta R.T.: 0.028 min
Response: 134293
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

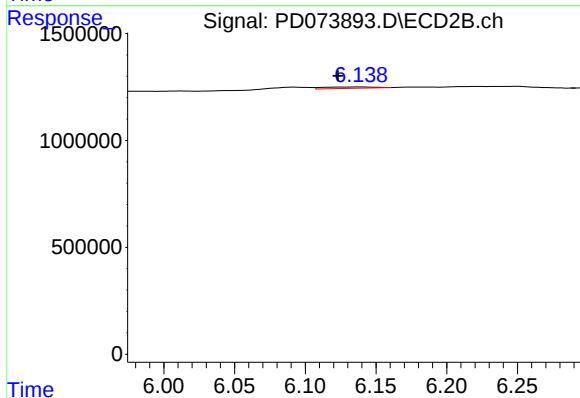


#18 Endrin aldehyde

R.T.: 6.140 min
Delta R.T.: 0.016 min
Response: 155662
Conc: 0.18 ng/ml

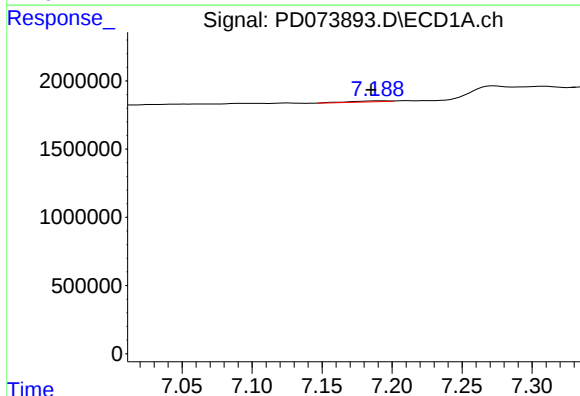


#19 Endosulfan Sulfate

R.T.: 7.190 min
Delta R.T.: 0.005 min
Response: 136440
Conc: 0.05 ng/ml

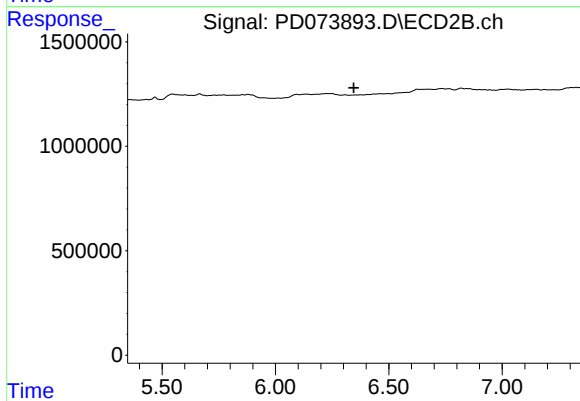

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.346 min
Response: 0
Conc: N.D.

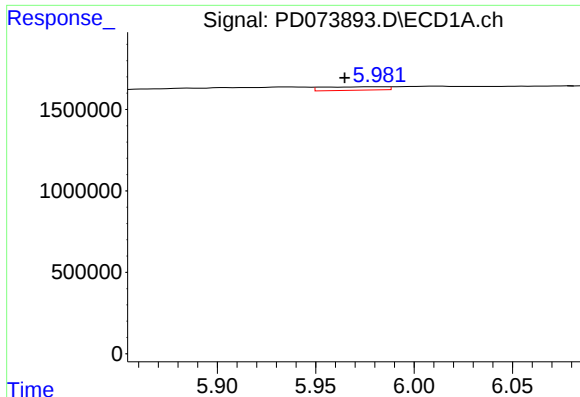

#25 Chlordane-3


R.T.: 5.983 min
Delta R.T.: 0.018 min
Response: 477487
Conc: 1.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

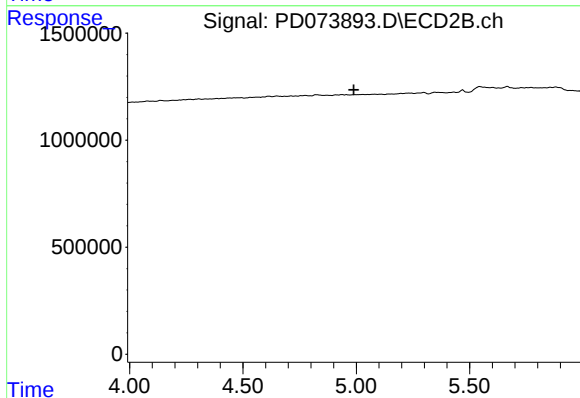


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

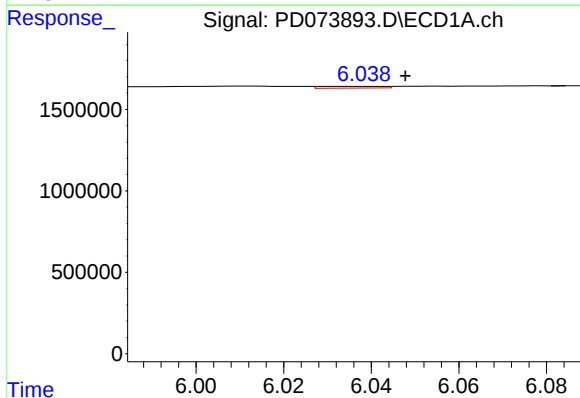


#26 Chlordane-4

R.T.: 6.040 min
Delta R.T.: -0.008 min
Response: 107247
Conc: 0.19 ng/ml

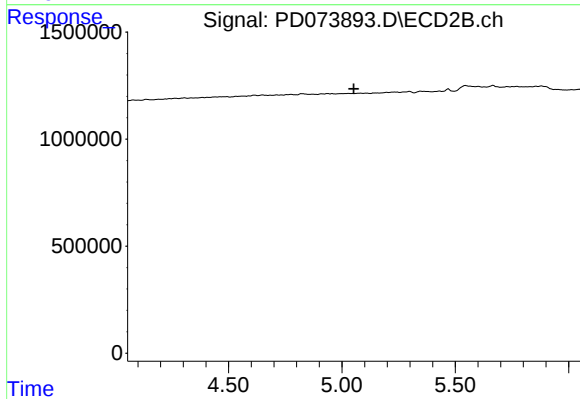

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.053 min
Response: 0
Conc: N.D.

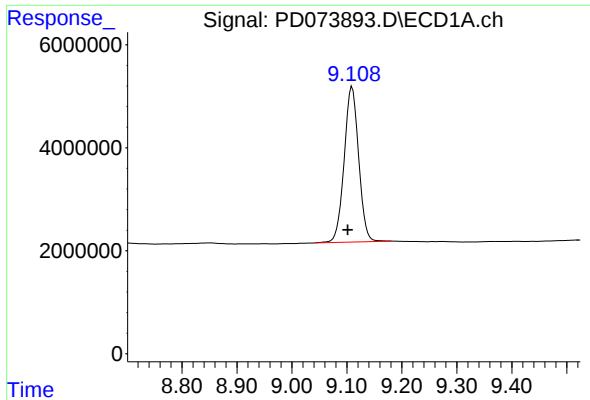

#28 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: 0.008 min
Response: 55187552
Conc: 19.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

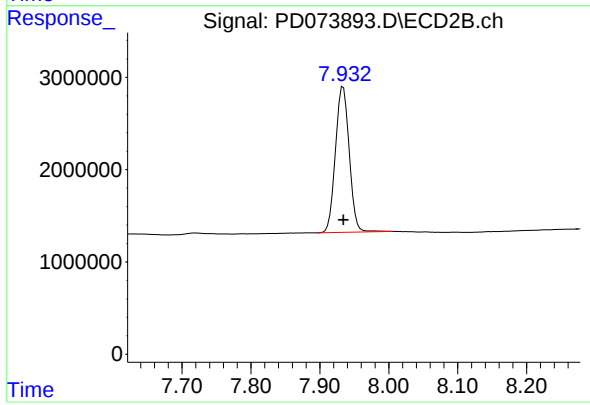

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 21976686
Conc: 18.89 ng/ml