

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020923\
 Data File : PD073908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2023 20:25
 Operator : AR\AJ
 Sample : 01462-23
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:06:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.777	39901722	19224149	17.070	15.101
28)	SA Decachlor...	9.099	7.931	43886126	16949871	15.573	14.568
Target Compounds							
3)	MA gamma-BHC...	4.330	0.000	948094	0	0.258	N.D. #
6)	B beta-BHC	4.532	0.000	439550	0	0.283	N.D. #
7)	B delta-BHC	4.781	0.000	7011453	0	2.084	N.D. #
8)	B Heptachlo...	5.701	0.000	1226199	0	0.384	N.D. #
13)	MA Dieldrin	6.387	0.000	322116	0	0.101	N.D. #
15)	B Endosulfa...	6.844f	0.000	231437	0	0.087	N.D. #
17)	MA 4,4'-DDT	7.060	0.000	55261	0	0.020	N.D. #
19)	B Endosulfa...	7.209f	0.000	95355	0	0.036	N.D. #
21)	B Endrin ke...	7.697f	0.000	297483	0	0.098	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020923\
Data File : PD073908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2023 20:25
Operator : AR\AJ
Sample : 01462-23
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:06:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

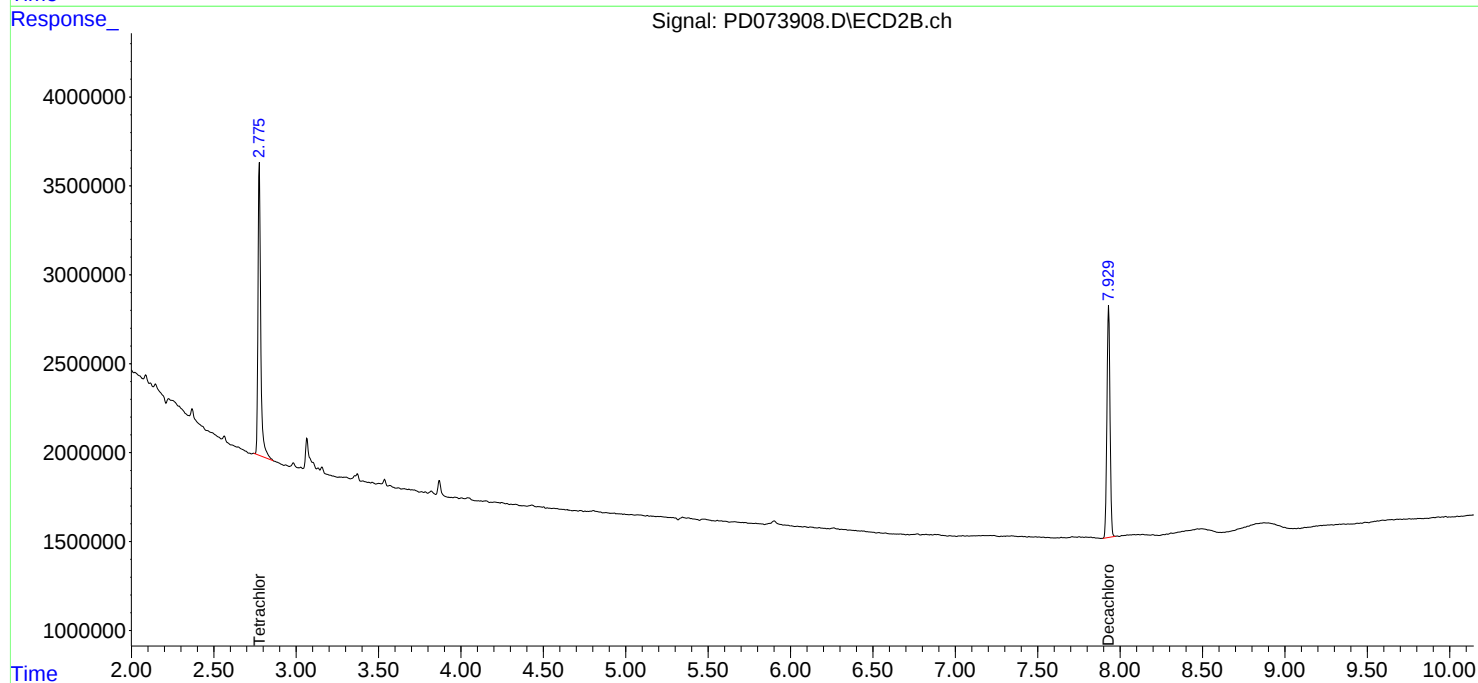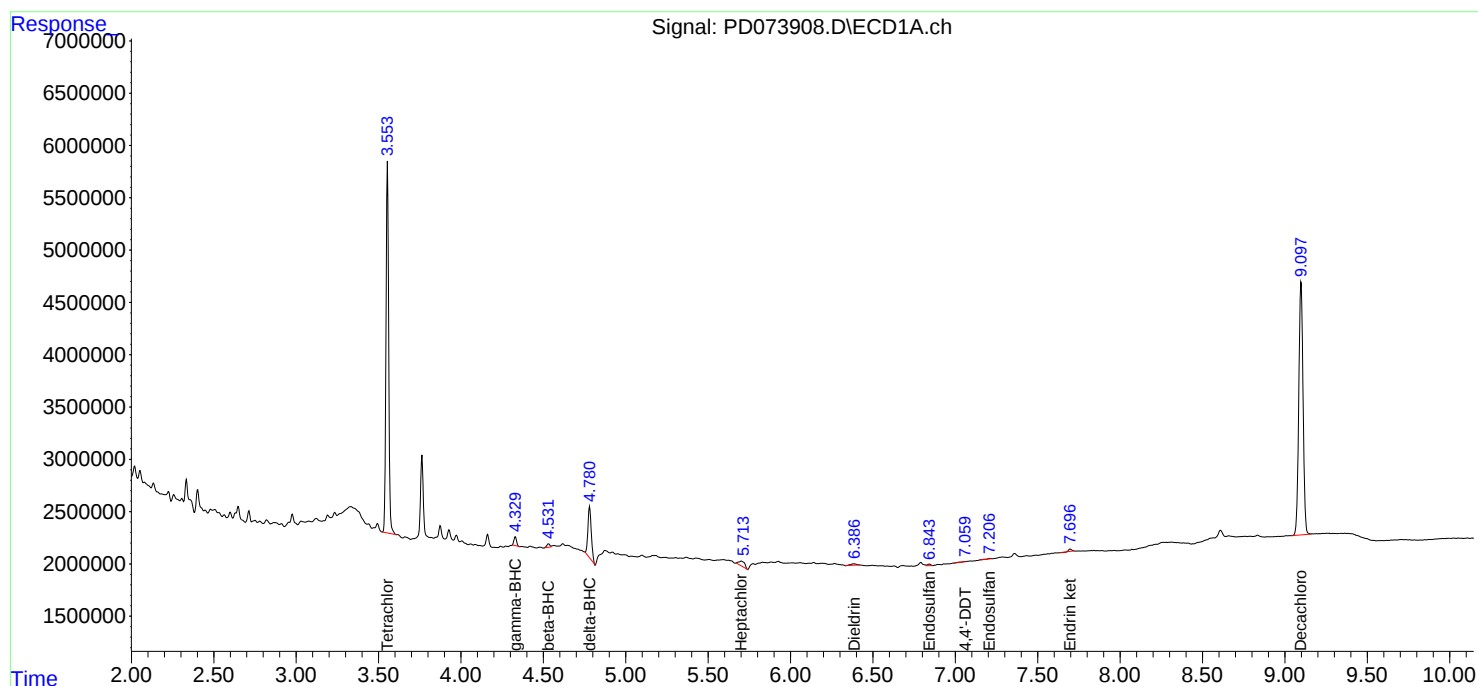


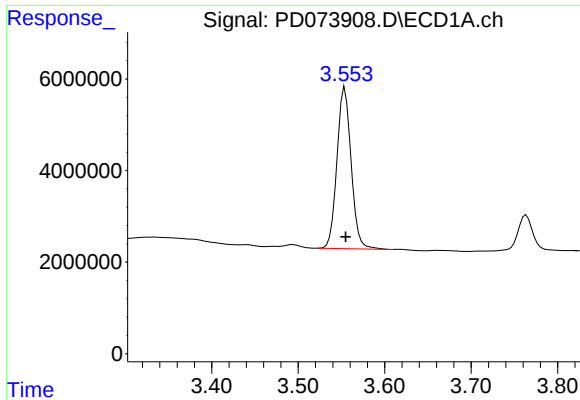

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 39901722
Conc: 17.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

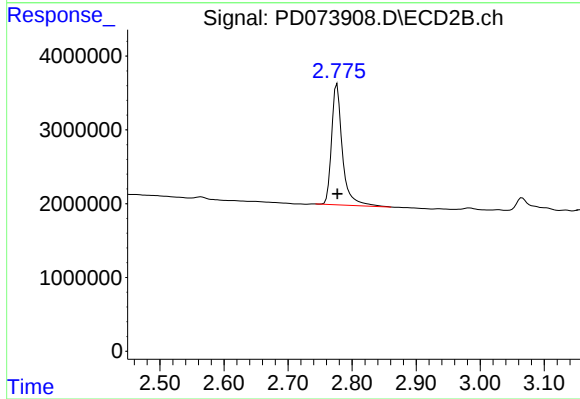


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 19224149
Conc: 15.10 ng/ml

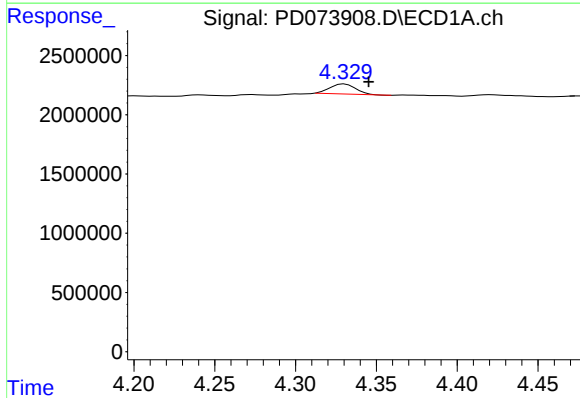


#3 gamma-BHC (Lindane)

R.T.: 4.330 min
Delta R.T.: -0.015 min
Response: 948094
Conc: 0.26 ng/ml

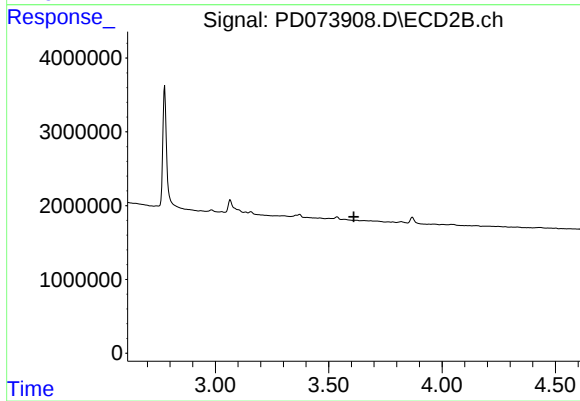

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.611 min
Response: 0
Conc: N.D.

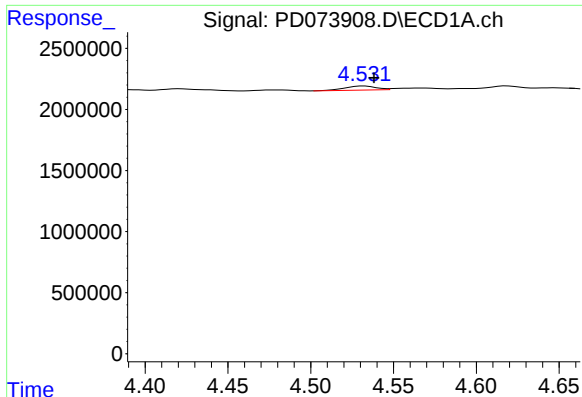

#6 beta-BHC


R.T.: 4.532 min
Delta R.T.: -0.006 min
Response: 439550
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

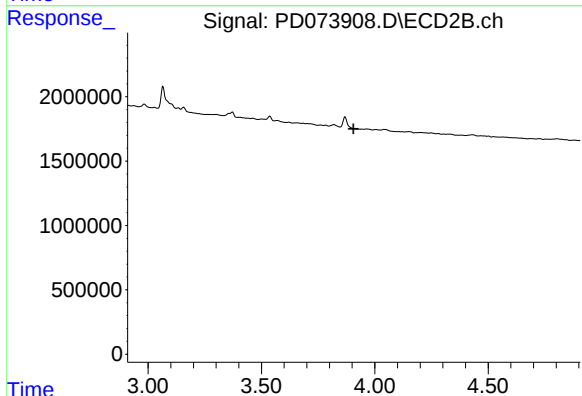


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.906 min
Response: 0
Conc: N.D.

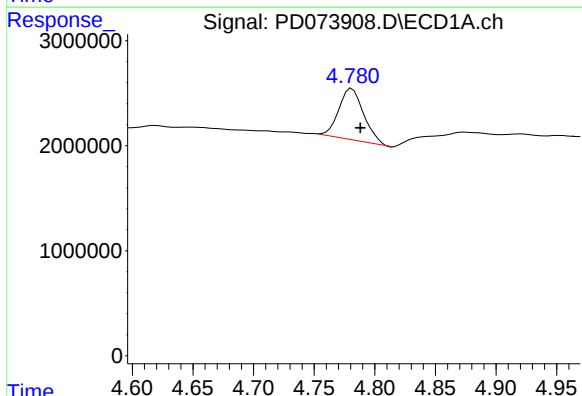


#7 delta-BHC

R.T.: 4.781 min
Delta R.T.: -0.007 min
Response: 7011453
Conc: 2.08 ng/ml

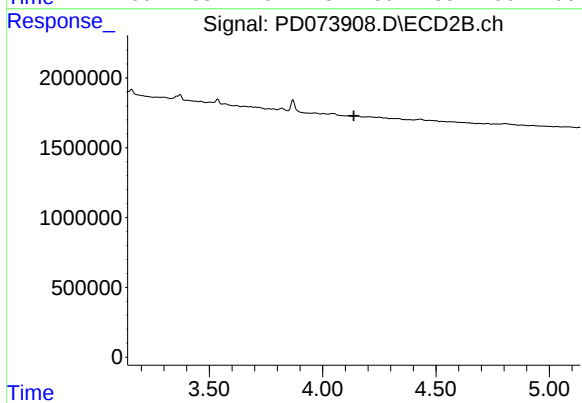

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

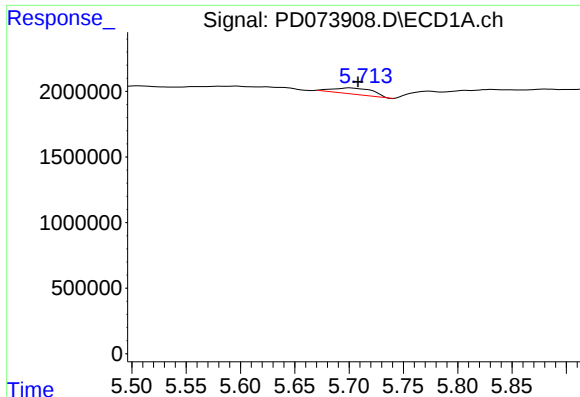

#8 Heptachlor epoxide


R.T.: 5.701 min
Delta R.T.: -0.007 min
Response: 1226199
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

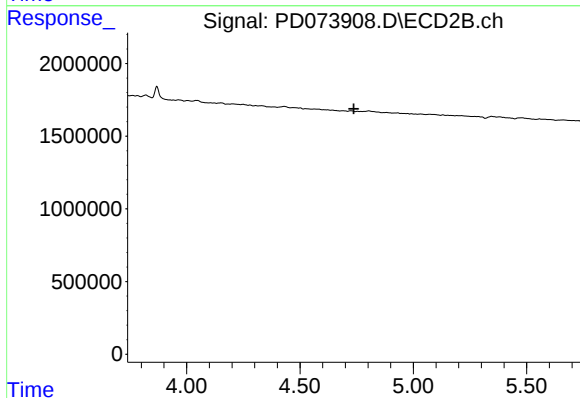


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

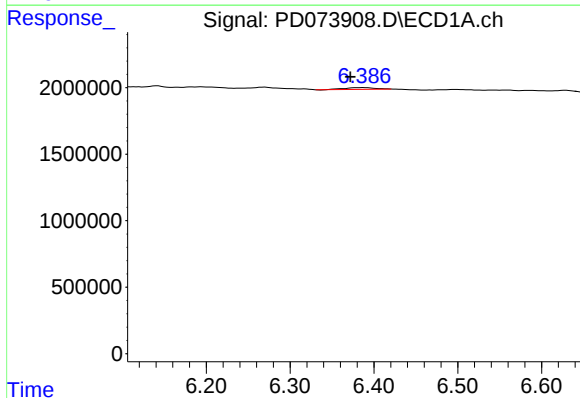


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.014 min
Response: 322116
Conc: 0.10 ng/ml

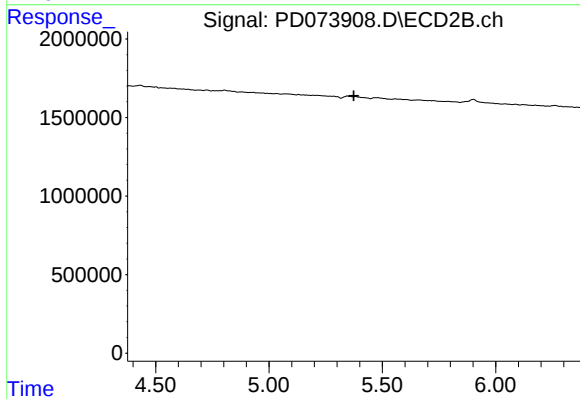

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.374 min
Response: 0
Conc: N.D.

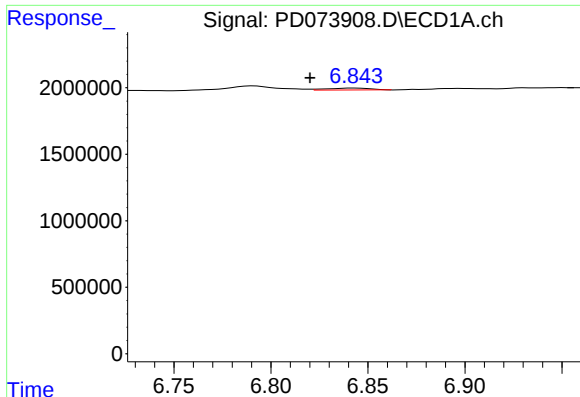

#15 Endosulfan II


R.T.: 6.844 min
Delta R.T.: 0.024 min
Response: 231437
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

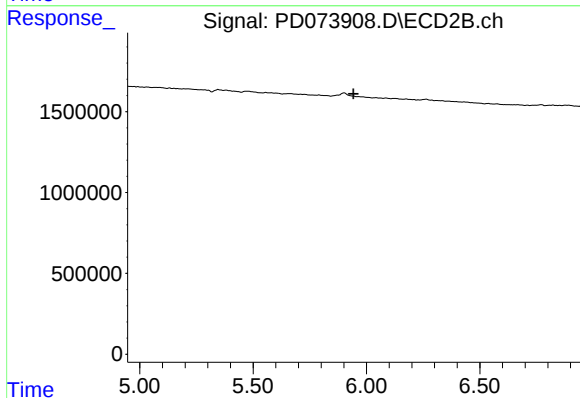


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

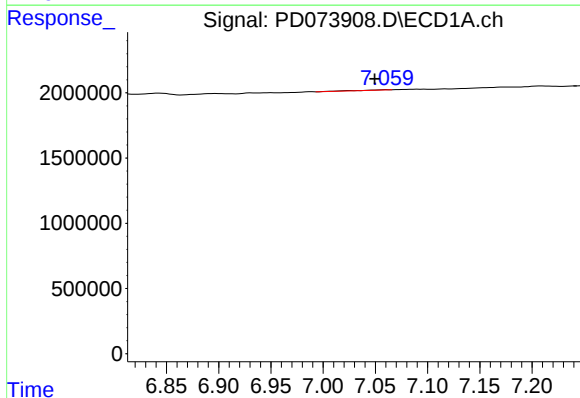


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.010 min
Response: 55261
Conc: 0.02 ng/ml

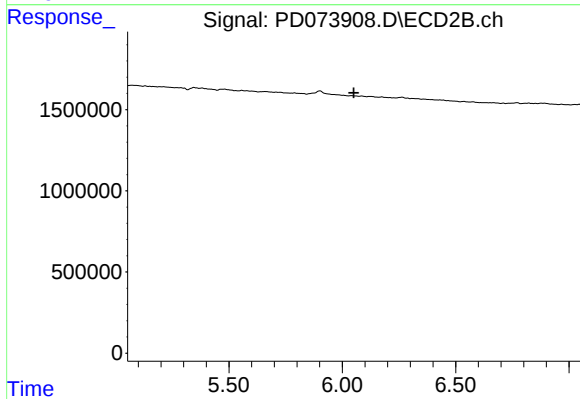

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

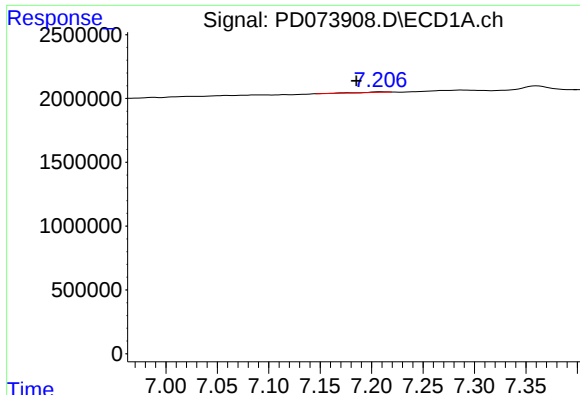

#19 Endosulfan Sulfate


R.T.: 7.209 min
Delta R.T.: 0.024 min
Response: 95355
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

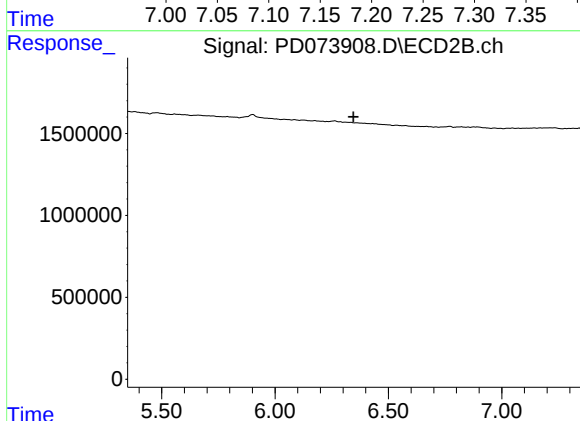


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.346 min
Response: 0
Conc: N.D.

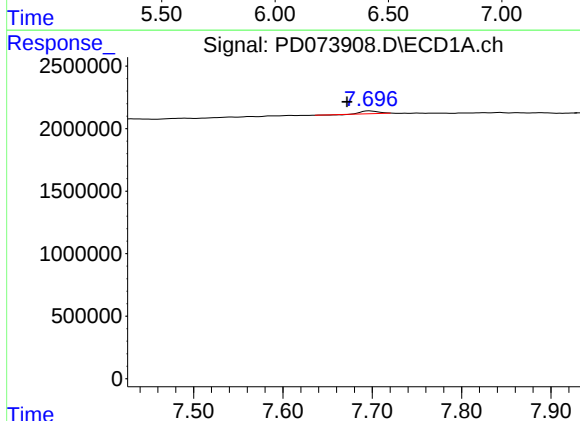


#21 Endrin ketone

R.T.: 7.697 min
Delta R.T.: 0.025 min
Response: 297483
Conc: 0.10 ng/ml

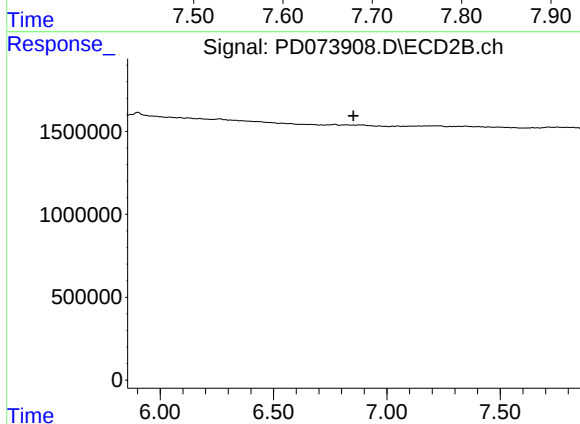

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

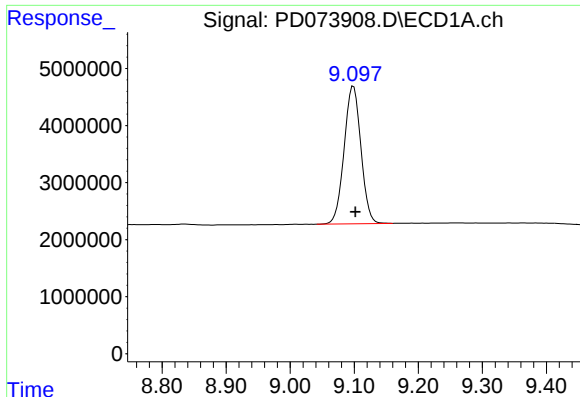

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.003 min
Response: 43886126
Conc: 15.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

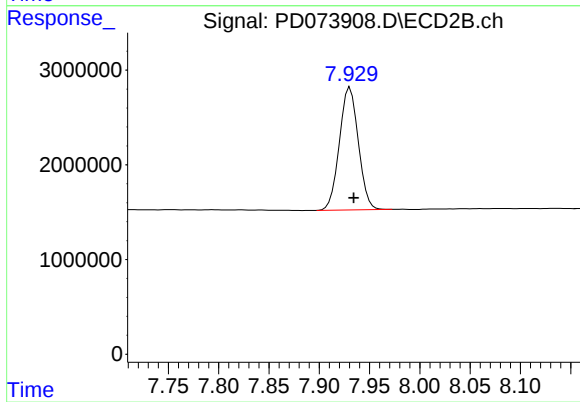

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: -0.004 min
Response: 16949871
Conc: 14.57 ng/ml