

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
 Data File : PD057150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2020 14:58
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA101

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 04:51:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:43:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	4128585	9227444	4.955	4.910
27)	SA Decachlor...	7.956	8.996	10775752	24261253	10.374	10.785
Target Compounds							
2)	A alpha-BHC	3.712	4.347	6134591	13240987	4.760	4.619
3)	MA gamma-BHC...	3.987	4.630	6911991	13978132	5.629	4.922
4)	MA Heptachlor	4.271	5.135	3878793	11650526	5.101	4.951
9)	A Endosulfan I	5.277	6.178	5096667	12271799	5.110	5.062
13)	MA Dieldrin	5.517	6.434	10682989	25816793	10.219	9.562
14)	MA Endrin	5.770	6.650	9240267	20304630	10.595	9.586
16)	A 4,4'-DDD	5.904	6.774	7208031	20407435	10.490	9.836
17)	MA 4,4'-DDT	6.140	7.071	5809082	18002614	8.885	9.433
20)	A Methoxychlor	6.687	7.528	14323579	46204280	50.324	50.413


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
Data File : PD057150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2020 14:58
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 04:51:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:43:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

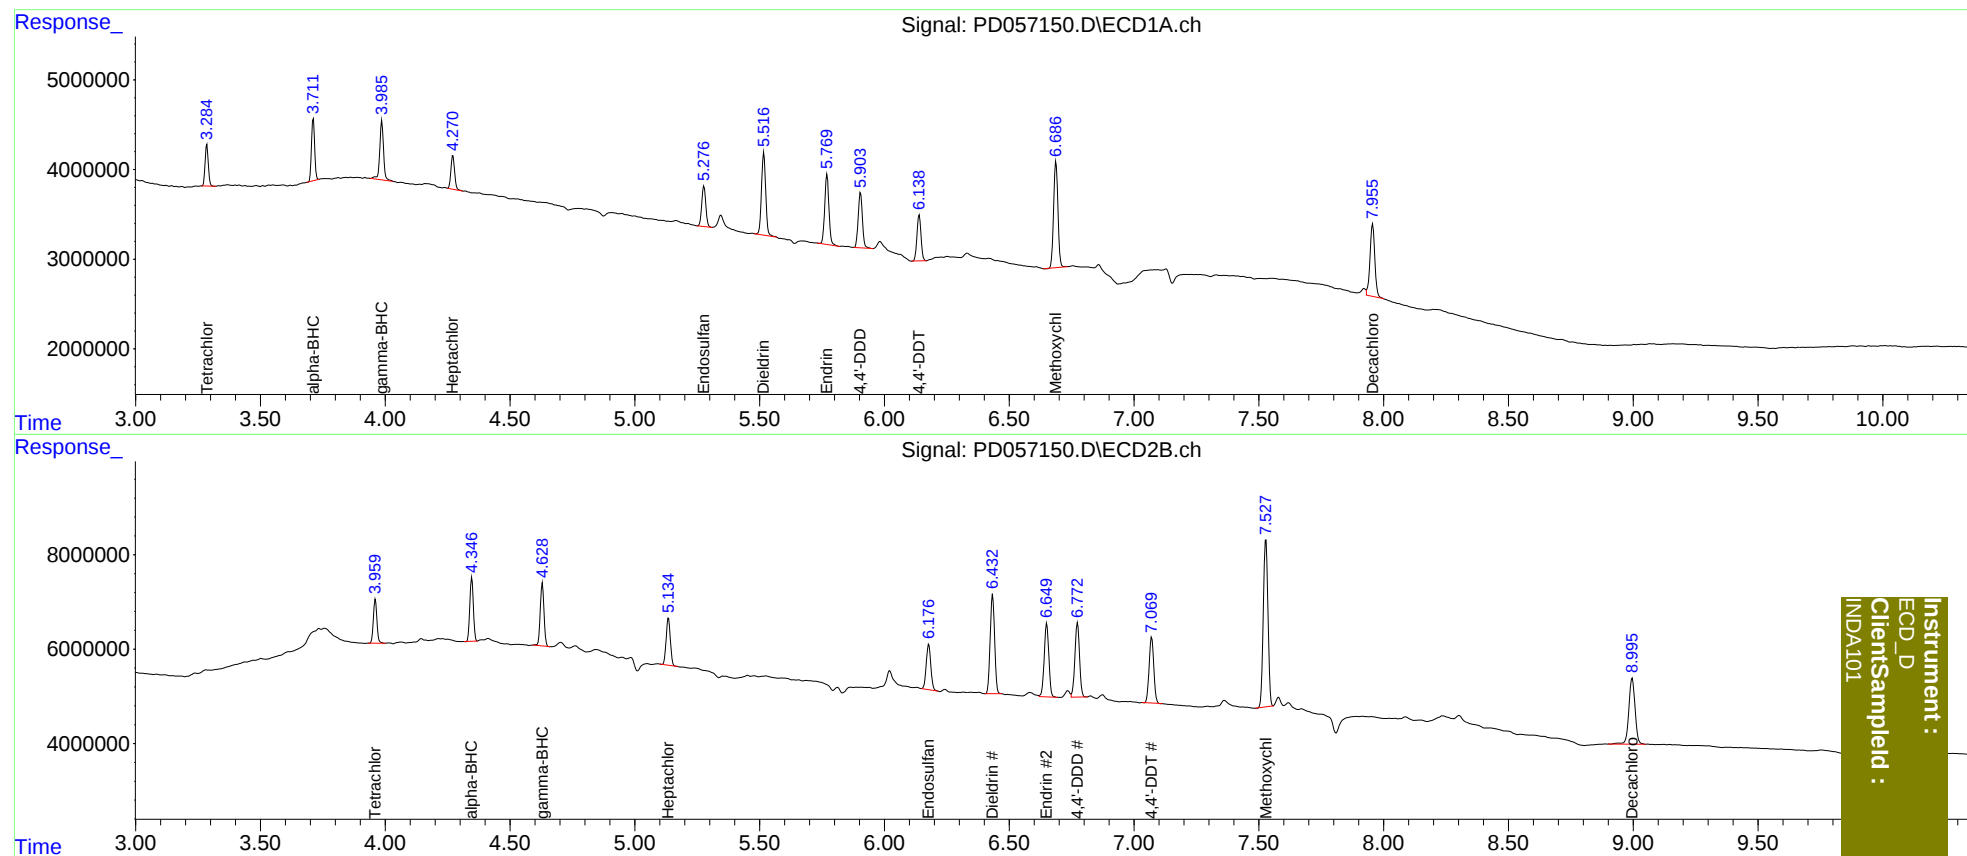


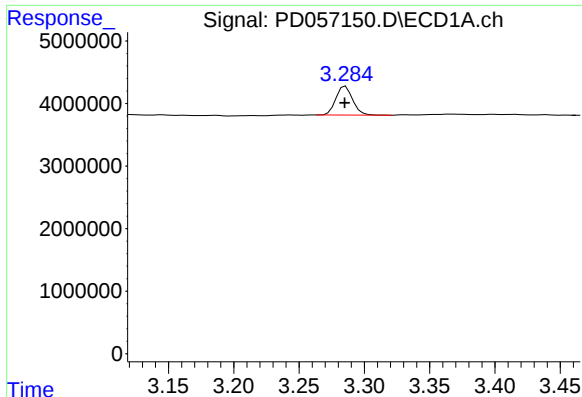

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: 0.000 min
Response: 4128585
Conc: 4.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

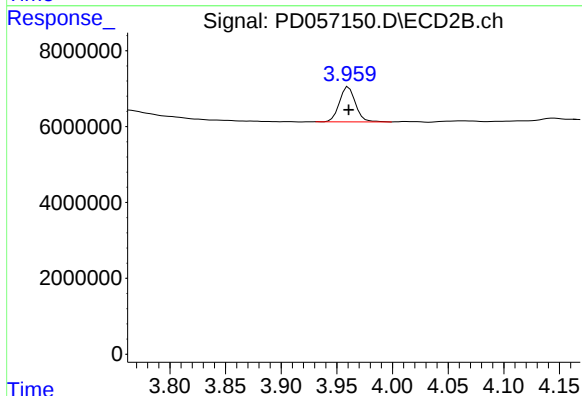


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 9227444
Conc: 4.91 ng/ml

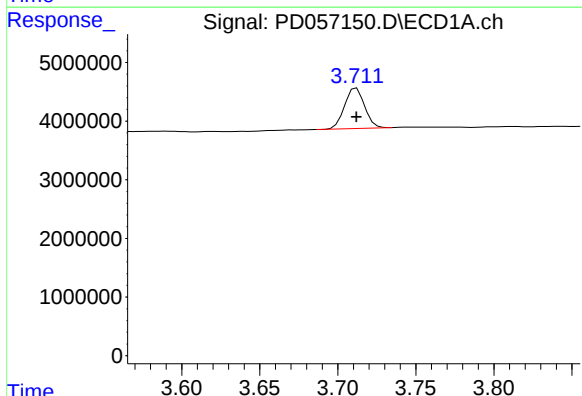


#2 alpha-BHC

R.T.: 3.712 min
Delta R.T.: 0.000 min
Response: 6134591
Conc: 4.76 ng/ml

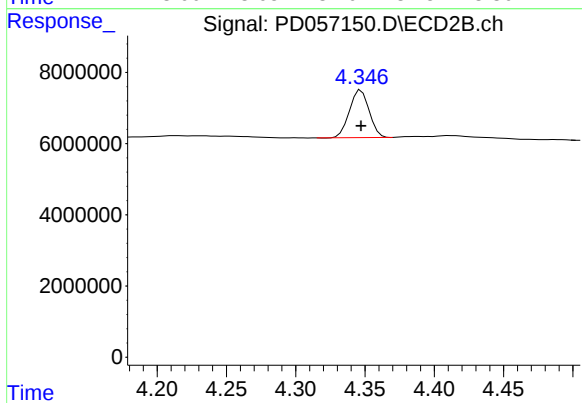

#2 alpha-BHC


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 13240987
Conc: 4.62 ng/ml

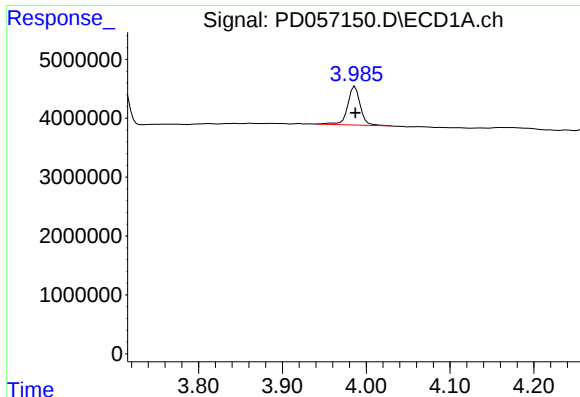

#3 gamma-BHC (Lindane)


R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 6911991
Conc: 5.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

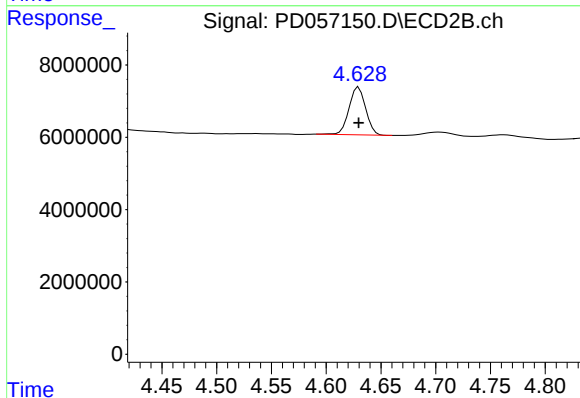


#3 gamma-BHC (Lindane)

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 13978132
Conc: 4.92 ng/ml

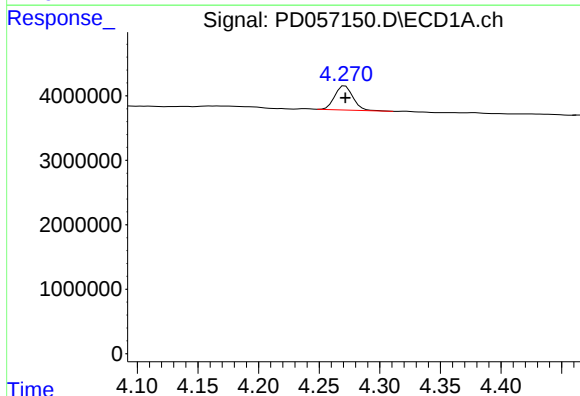


#4 Heptachlor

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 3878793
Conc: 5.10 ng/ml

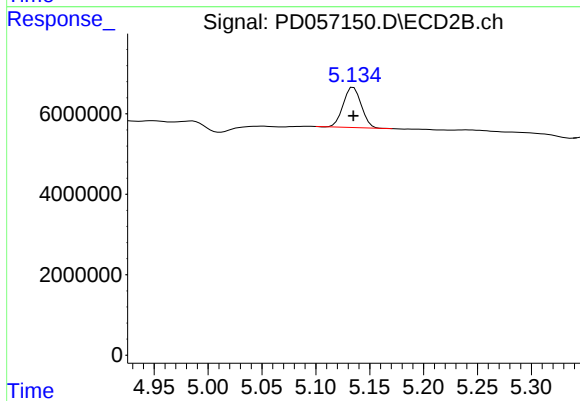

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 11650526
Conc: 4.95 ng/ml

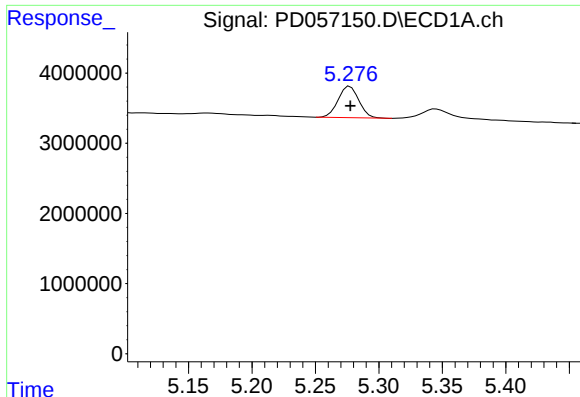

#9 Endosulfan I


R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 5096667
Conc: 5.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

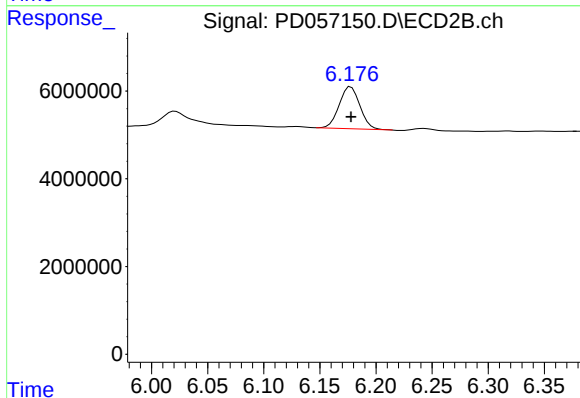


#9 Endosulfan I

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 12271799
Conc: 5.06 ng/ml

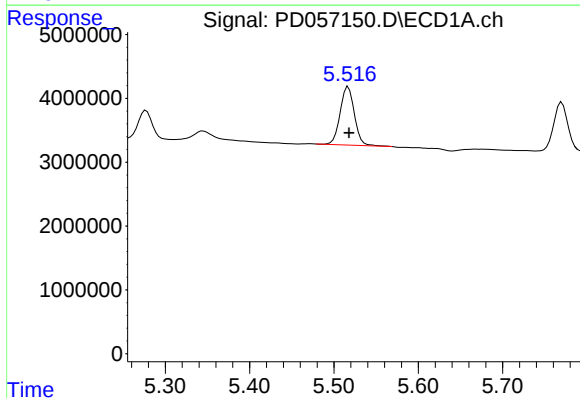


#13 Dieldrin

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 10682989
Conc: 10.22 ng/ml

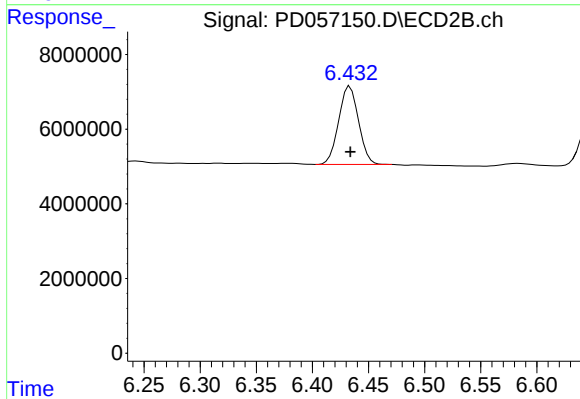

#13 Dieldrin


R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 25816793
Conc: 9.56 ng/ml

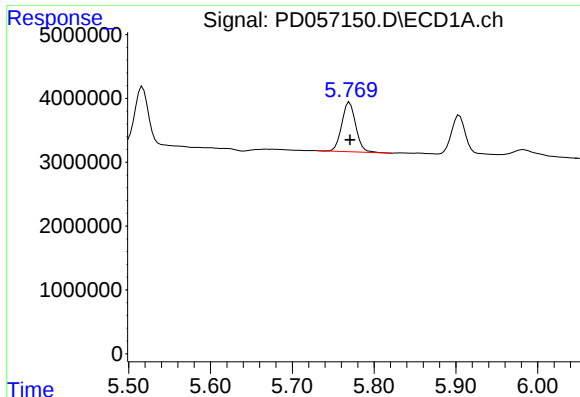

#14 Endrin


R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 9240267
Conc: 10.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

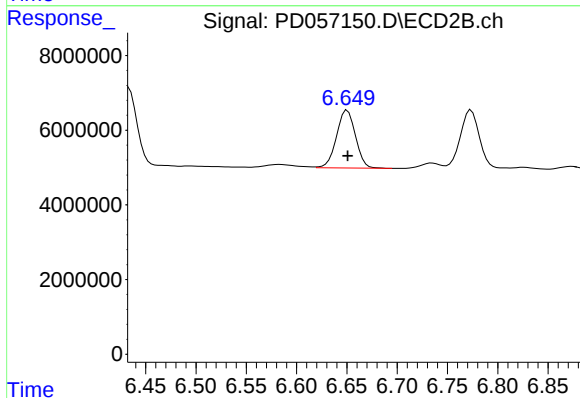


#14 Endrin

R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 20304630
Conc: 9.59 ng/ml

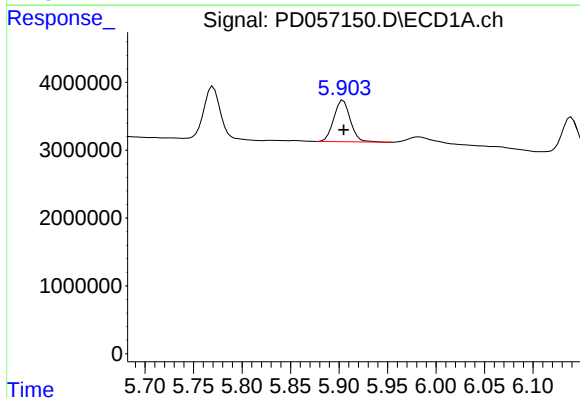


#16 4,4'-DDD

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 7208031
Conc: 10.49 ng/ml

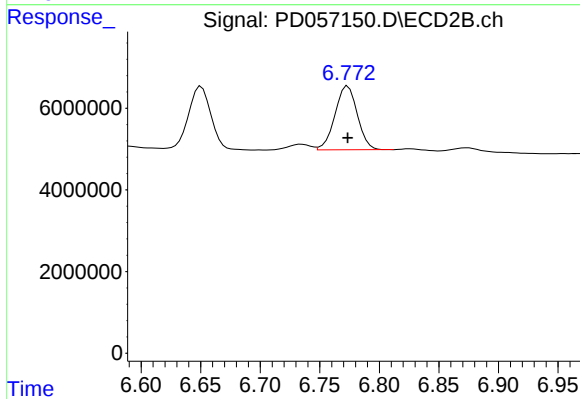

#16 4,4'-DDD


R.T.: 6.774 min
Delta R.T.: 0.000 min
Response: 20407435
Conc: 9.84 ng/ml

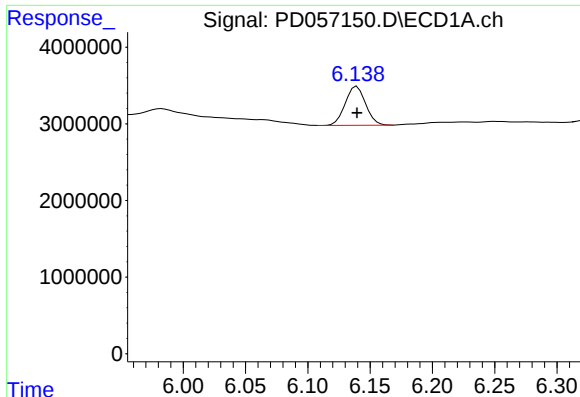

#17 4,4'-DDT


R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 5809082
Conc: 8.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

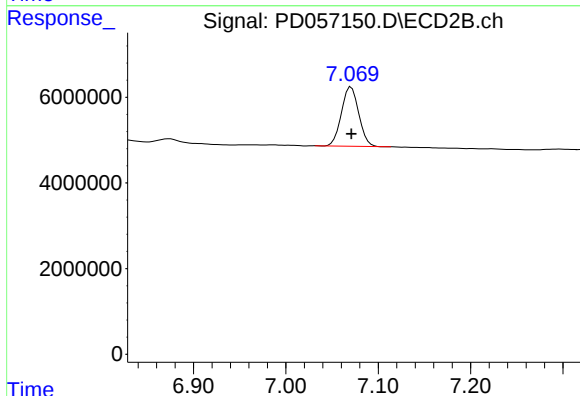


#17 4,4'-DDT

R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 18002614
Conc: 9.43 ng/ml

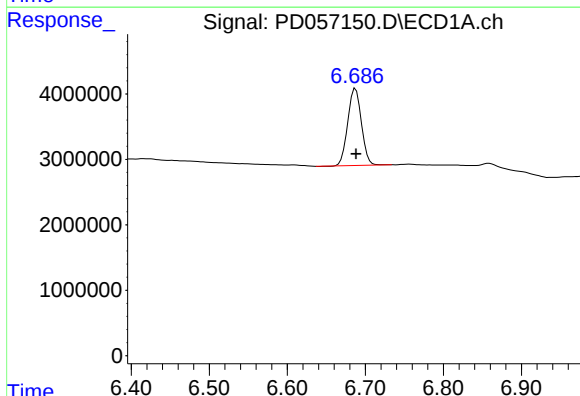


#20 Methoxychlor

R.T.: 6.687 min
Delta R.T.: 0.000 min
Response: 14323579
Conc: 50.32 ng/ml

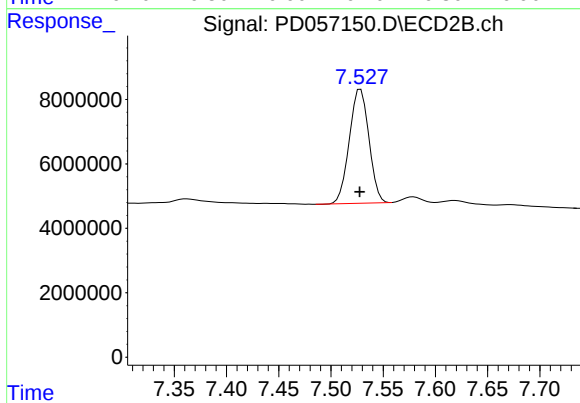

#20 Methoxychlor


R.T.: 7.528 min
Delta R.T.: 0.000 min
Response: 46204280
Conc: 50.41 ng/ml

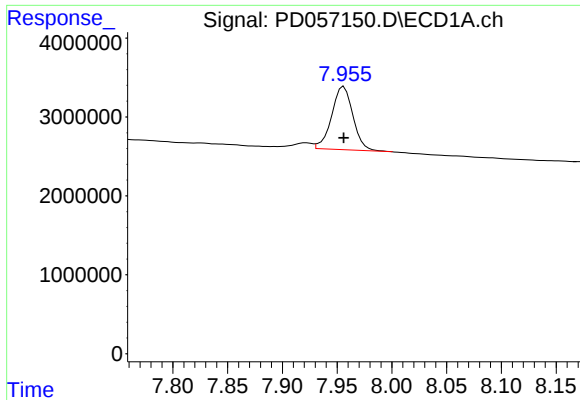

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 10775752
Conc: 10.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

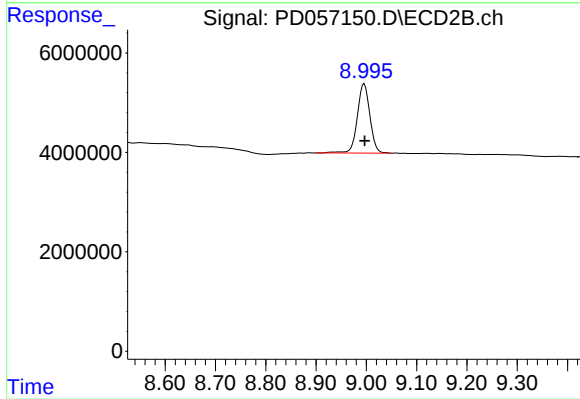

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.001 min
Response: 24261253
Conc: 10.79 ng/ml