

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
 Data File : PD057156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2020 16:22
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 04:45:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:43:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	33033019	74370314	39.649	39.575
27)	SA Decachlor...	7.955	8.995	80745077	174.2E6	77.738	77.445
Target Compounds							
2)	A alpha-BHC	3.712	4.347	52450834	116.1E6	40.695	40.505
3)	MA gamma-BHC...	3.987	4.630	48868247	112.7E6	39.795	39.689
4)	MA Heptachlor	4.271	5.135	30338735	92596022	39.896	39.350
9)	A Endosulfan I	5.278	6.178	39890138	96636673	39.993	39.865
13)	MA Dieldrin	5.517	6.434	83448868	218.4E6	79.821	80.901
14)	MA Endrin	5.771	6.650	68665804	171.2E6	78.732	80.821
16)	A 4,4'-DDD	5.905	6.773	53935000	164.9E6	78.492	79.461
17)	MA 4,4'-DDT	6.140	7.071	54692532	155.0E6	83.656	81.234
20)	A Methoxychlor	6.687	7.527	110.6E6	355.5E6	388.649	387.887


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
Data File : PD057156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2020 16:22
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 04:45:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:43:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

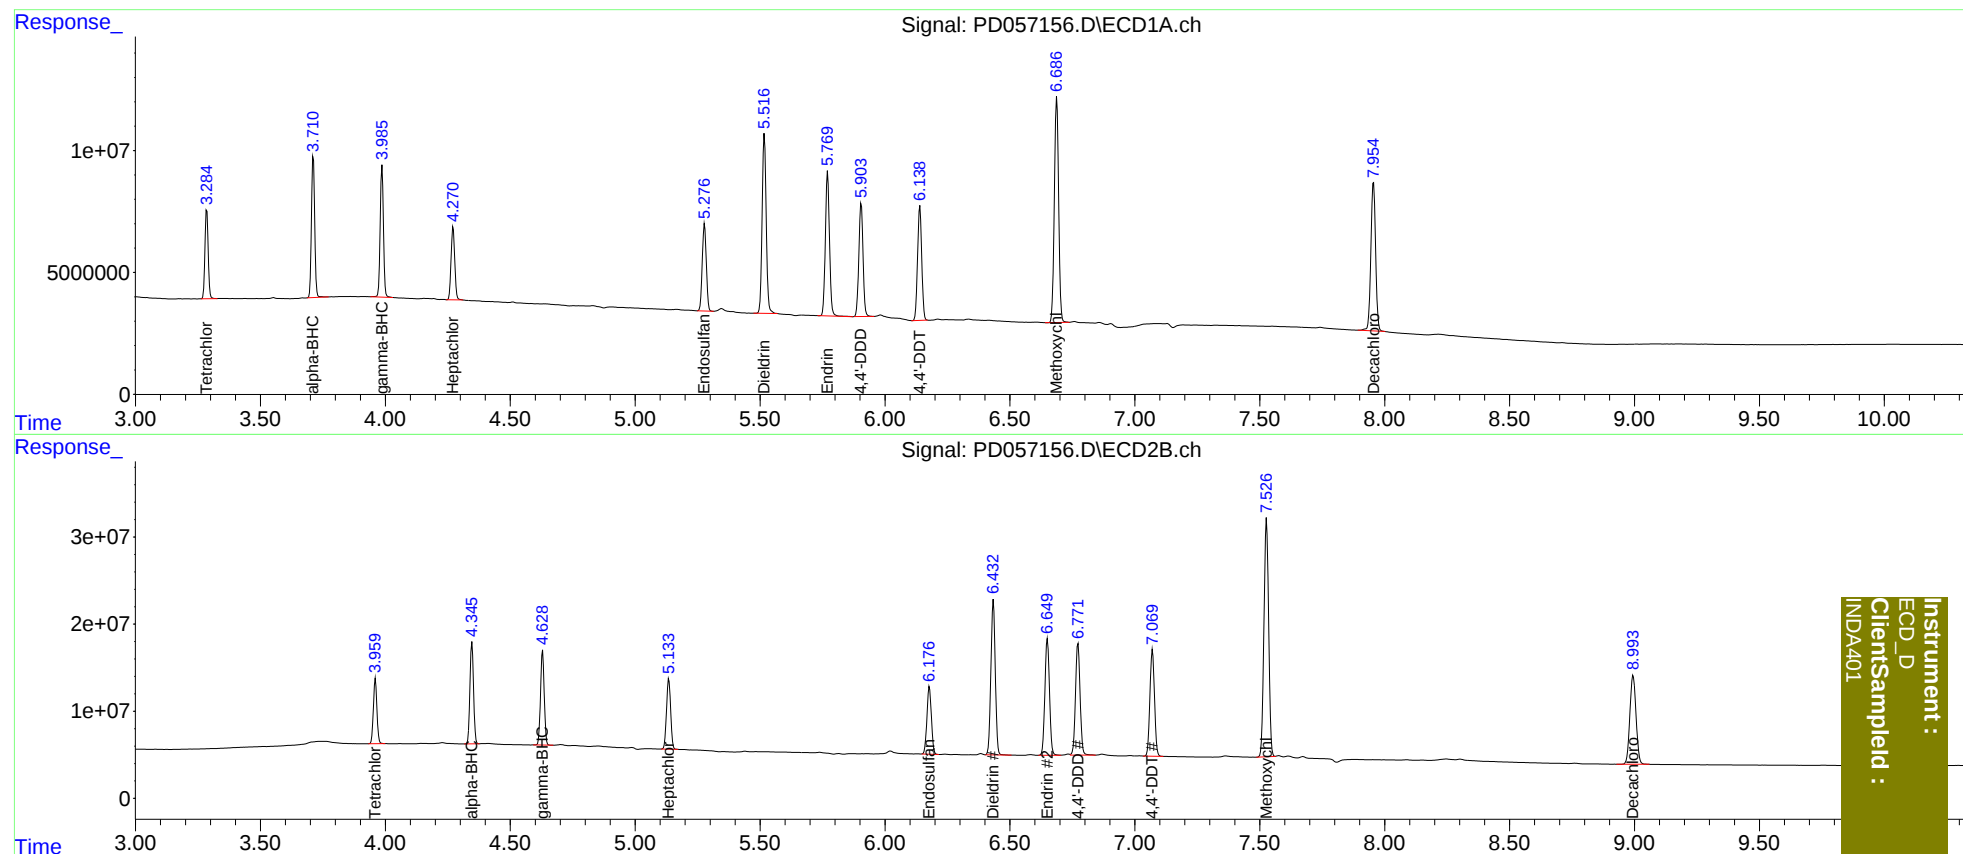


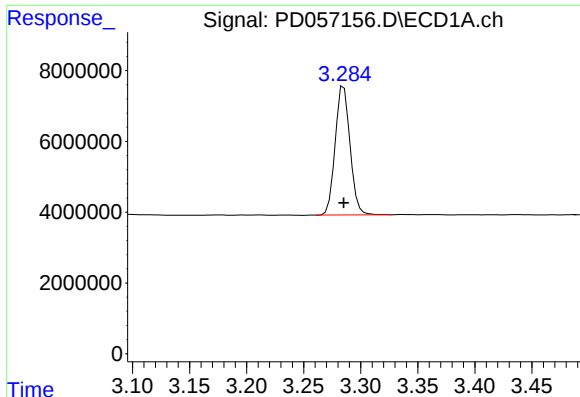

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 33033019
Conc: 39.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

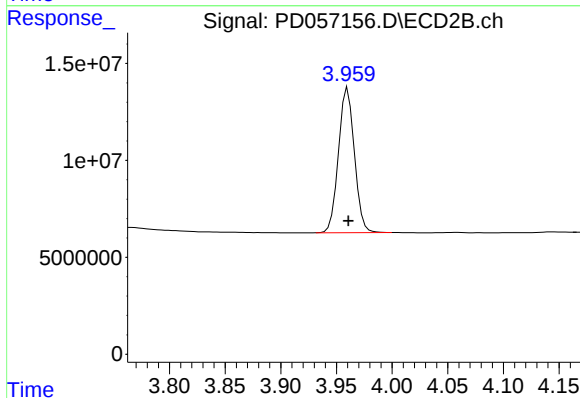


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 74370314
Conc: 39.58 ng/ml

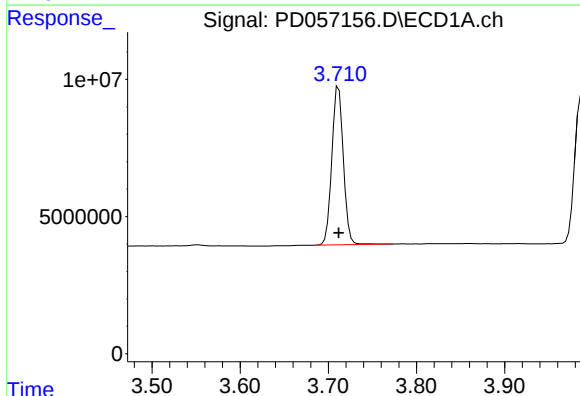


#2 alpha-BHC

R.T.: 3.712 min
Delta R.T.: 0.000 min
Response: 52450834
Conc: 40.69 ng/ml

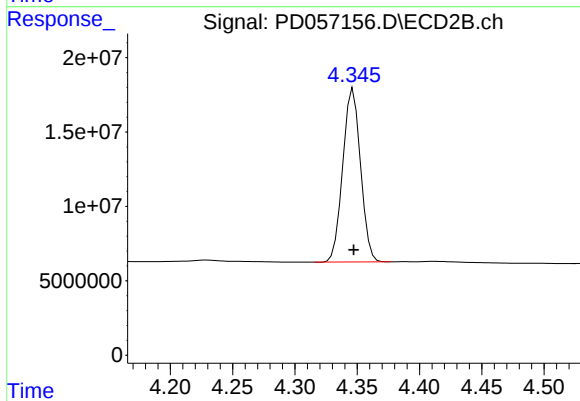

#2 alpha-BHC


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 116120987
Conc: 40.50 ng/ml

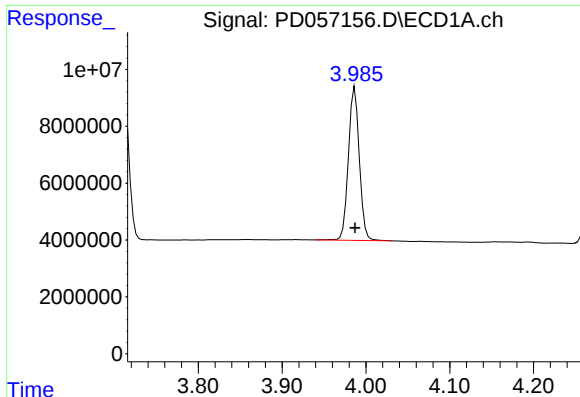

#3 gamma-BHC (Lindane)


R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 48868247
Conc: 39.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

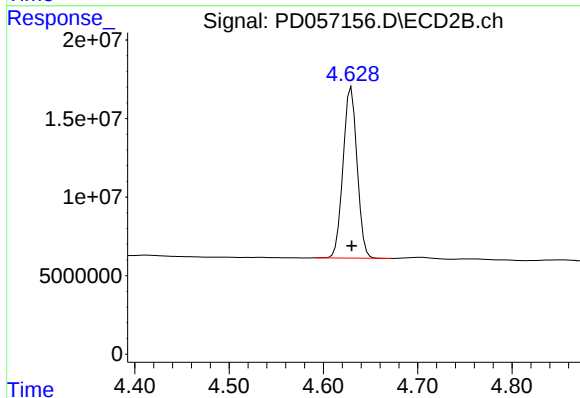


#3 gamma-BHC (Lindane)

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 112724970
Conc: 39.69 ng/ml

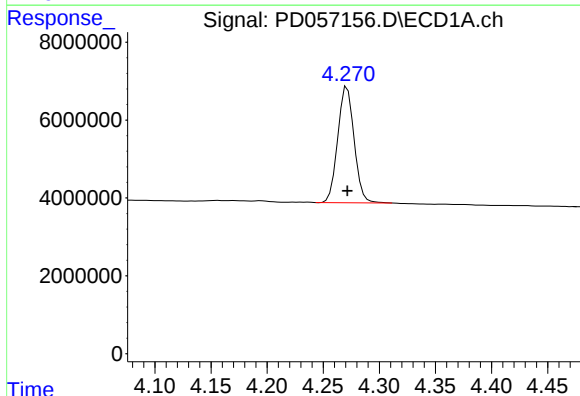


#4 Heptachlor

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 30338735
Conc: 39.90 ng/ml

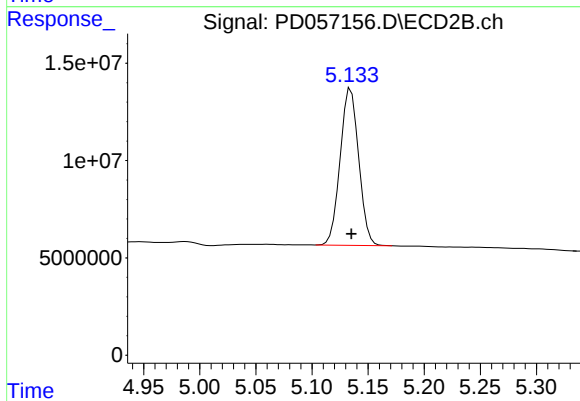

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 92596022
Conc: 39.35 ng/ml

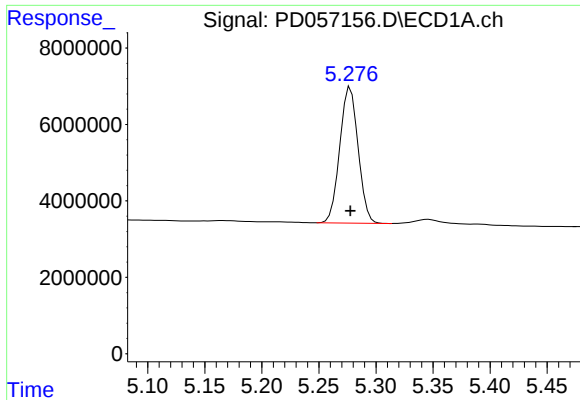

#9 Endosulfan I


R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 39890138
Conc: 39.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

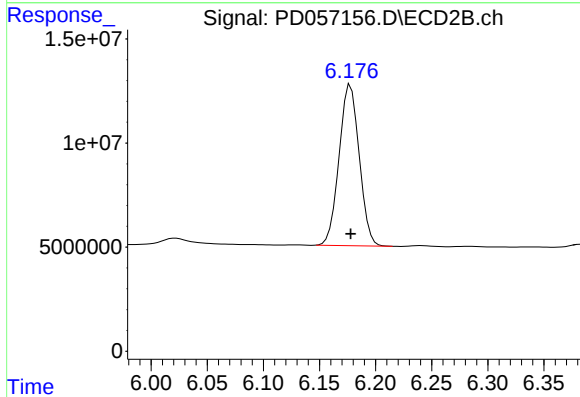


#9 Endosulfan I

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 96636673
Conc: 39.86 ng/ml

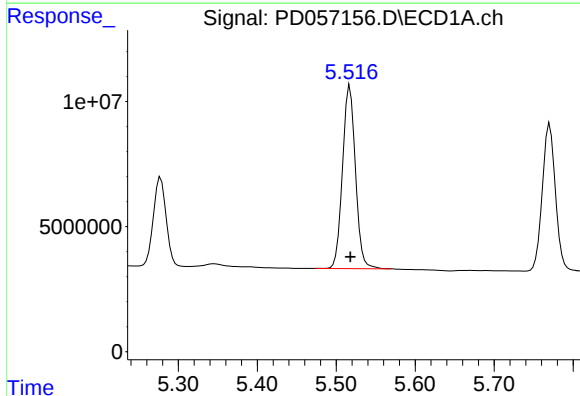


#13 Dieldrin

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 83448868
Conc: 79.82 ng/ml

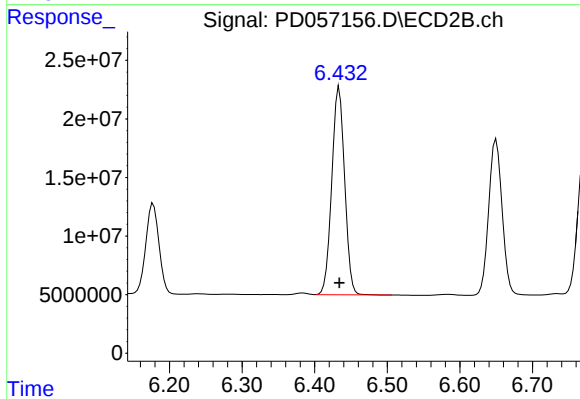

#13 Dieldrin


R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 218432192
Conc: 80.90 ng/ml

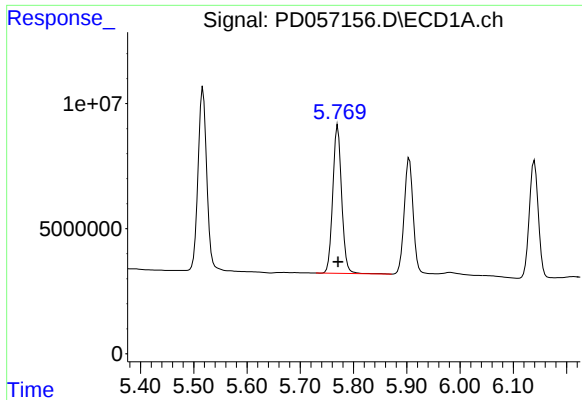

#14 Endrin


R.T.: 5.771 min
Delta R.T.: 0.000 min
Response: 68665804
Conc: 78.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

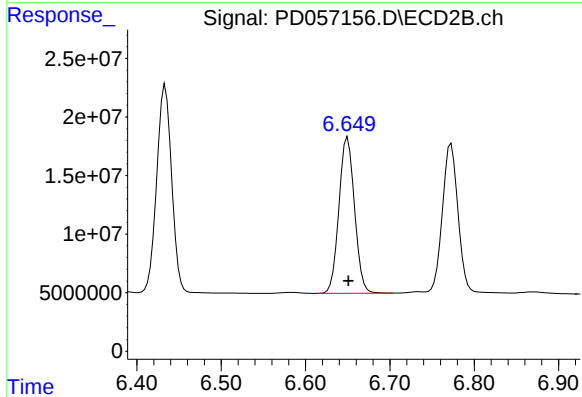


#14 Endrin

R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 171188487
Conc: 80.82 ng/ml

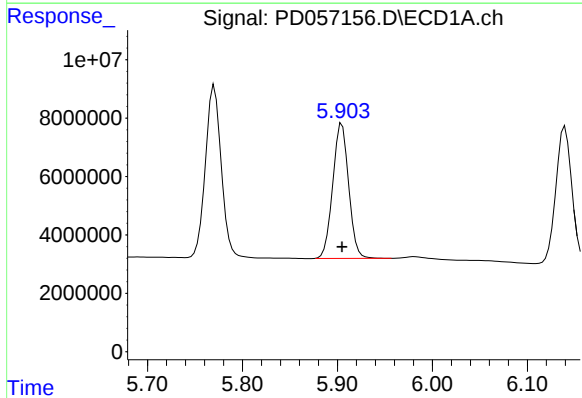


#16 4,4'-DDD

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 53935000
Conc: 78.49 ng/ml

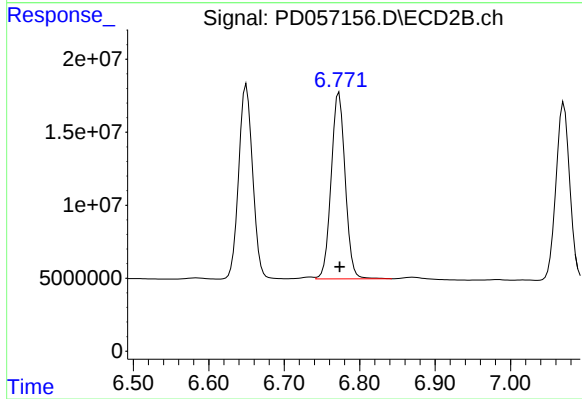

#16 4,4'-DDD


R.T.: 6.773 min
Delta R.T.: 0.000 min
Response: 164856247
Conc: 79.46 ng/ml

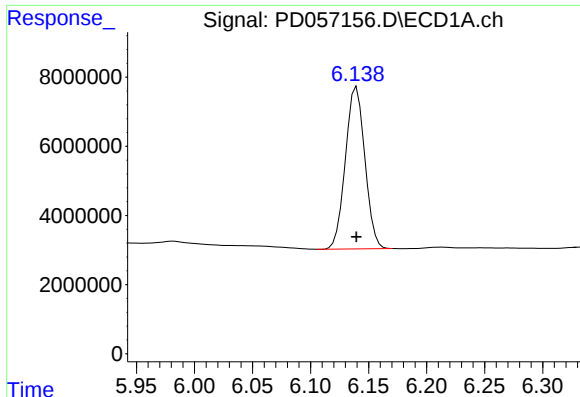

#17 4,4'-DDT


R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 54692532
Conc: 83.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

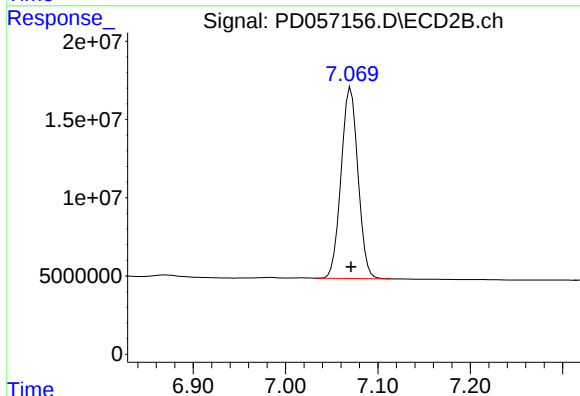


#17 4,4'-DDT

R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 155027871
Conc: 81.23 ng/ml

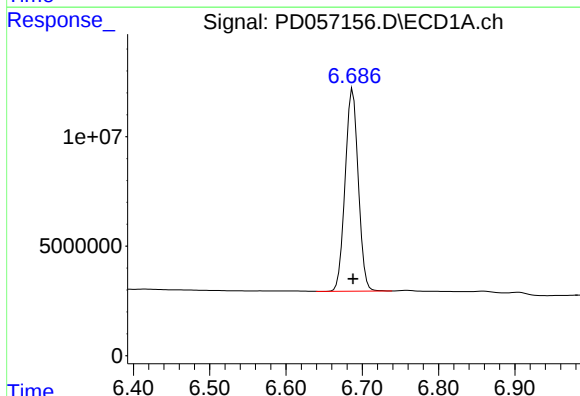


#20 Methoxychlor

R.T.: 6.687 min
Delta R.T.: 0.000 min
Response: 110619174
Conc: 388.65 ng/ml

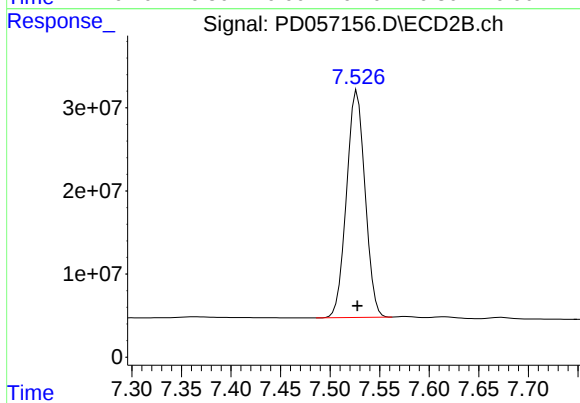

#20 Methoxychlor


R.T.: 7.527 min
Delta R.T.: 0.000 min
Response: 355506558
Conc: 387.89 ng/ml

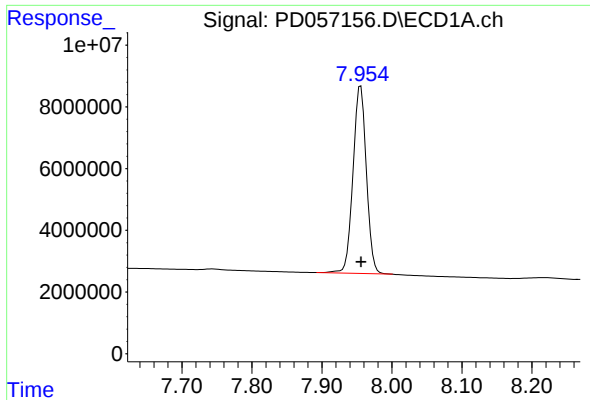

#27 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 80745077
Conc: 77.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

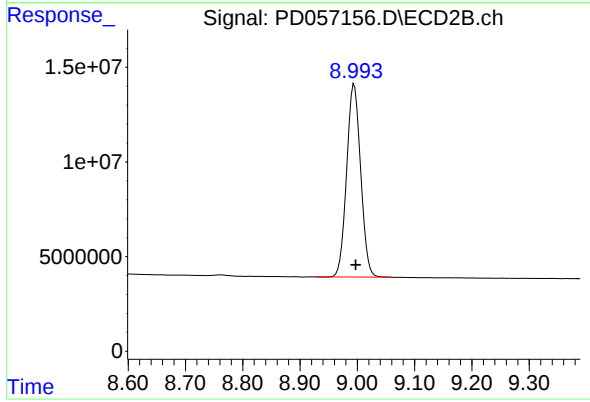

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.002 min
Response: 174209952
Conc: 77.44 ng/ml