

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD021020\  
 Data File : PD057182.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 10 Feb 2020 22:30  
 Operator : AJ\MA  
 Sample : L1302-02  
 Misc :  
 ALS Vial : 41 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 C5AK8

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 11 06:28:41 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD021020CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Feb 11 04:58:40 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.285 | 3.960 | 9020483  | 20125660 | 10.859 | 10.800 |
| 27)                         | SA Decachlor... | 7.956 | 8.995 | 17337332 | 31962161 | 16.712 | 14.139 |

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD021020\  
Data File : PD057182.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 10 Feb 2020 22:30  
Operator : AJ\MA  
Sample : L1302-02  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
C5AK8

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 11 06:28:41 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD021020CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Feb 11 04:58:40 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

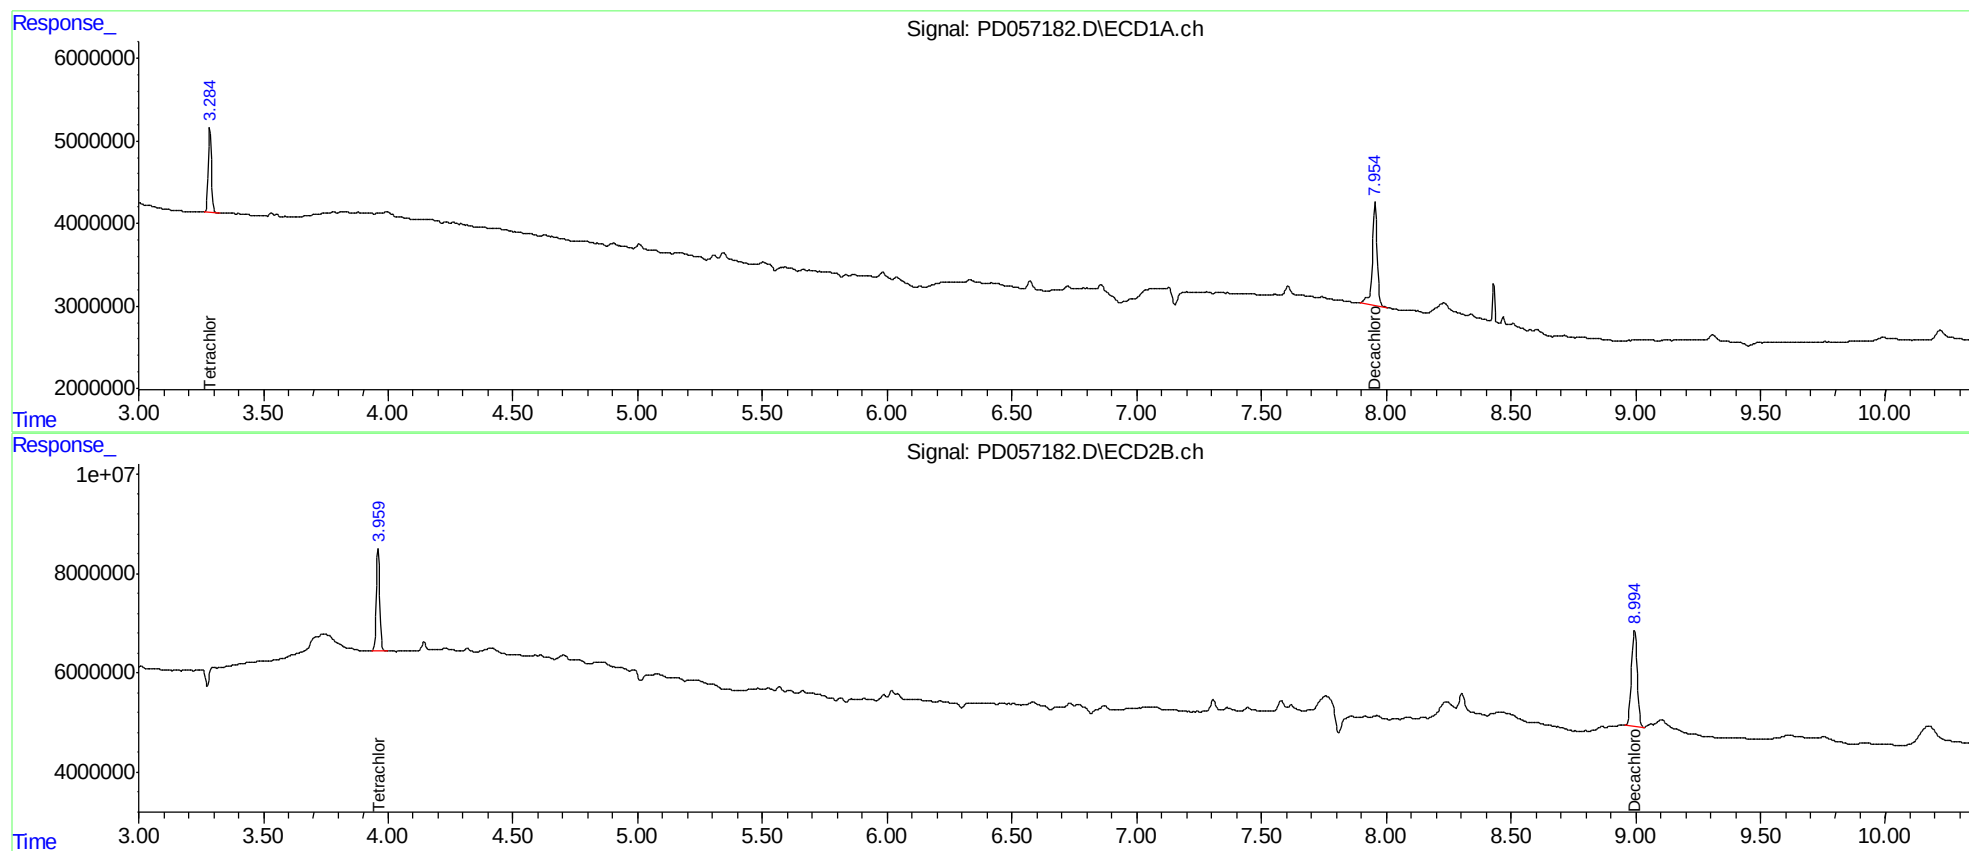


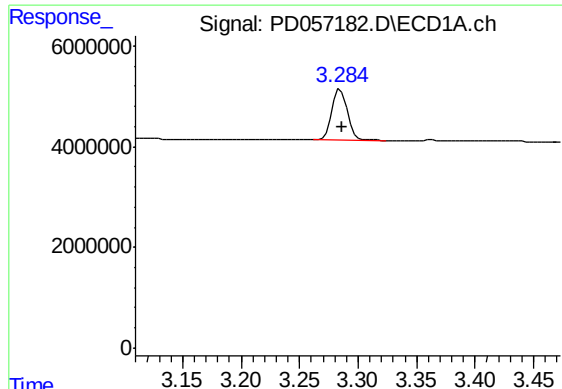

#1 Tetrachloro-m-xylene


R.T.: 3.285 min  
Delta R.T.: 0.000 min  
Response: 9020483  
Conc: 10.86 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
C5AK8

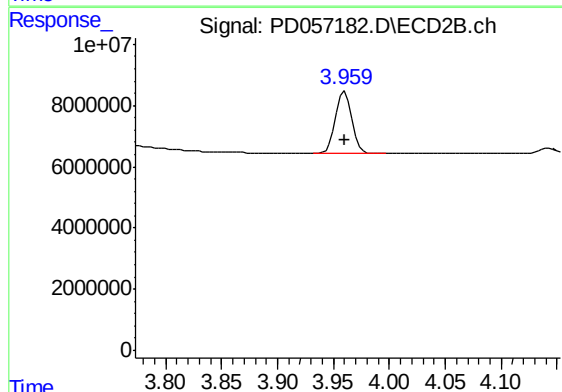


#1 Tetrachloro-m-xylene

R.T.: 3.960 min  
Delta R.T.: 0.000 min  
Response: 20125660  
Conc: 10.80 ng/ml

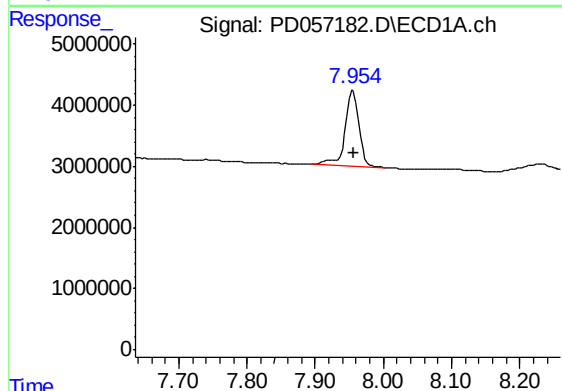

#27 Decachlorobiphenyl

R.T.: 7.956 min  
Delta R.T.: 0.000 min  
Response: 17337332  
Conc: 16.71 ng/ml

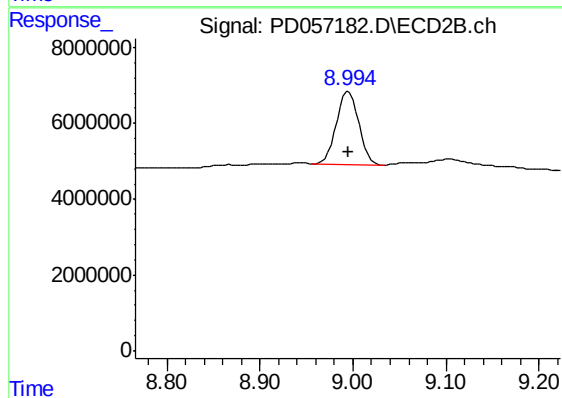

#27 Decachlorobiphenyl

R.T.: 8.995 min  
Delta R.T.: 0.000 min  
Response: 31962161  
Conc: 14.14 ng/ml