

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
 Data File : PD057173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2020 20:22
 Operator : AJ\MA
 Sample : L1302-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
ClientSampled :
 C5AN0

Manual Integrations
APPROVED
 mohammad
 2/12/2020 3:30:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 06:34:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.285	3.960	8517193	17947753	10.253	9.631
27) SA Decachlor...	7.954	8.994	16728961	27555511	16.125m	12.189m
Target Compounds						
10) B trans-Chl...	5.188	6.045	6586161	18750079	6.093m	6.858
11) B cis-Chlor...	5.223	6.130	754864	15122410	0.706m	5.903m#
16) A 4,4'-DDD	5.908	6.770	587147	5022836	0.848m	2.436m#
17) MA 4,4'-DDT	6.137	7.070	1106287	2504348	1.700m	1.319m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
 Data File : PD057173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2020 20:22
 Operator : AJ\MA
 Sample : L1302-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 06:34:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

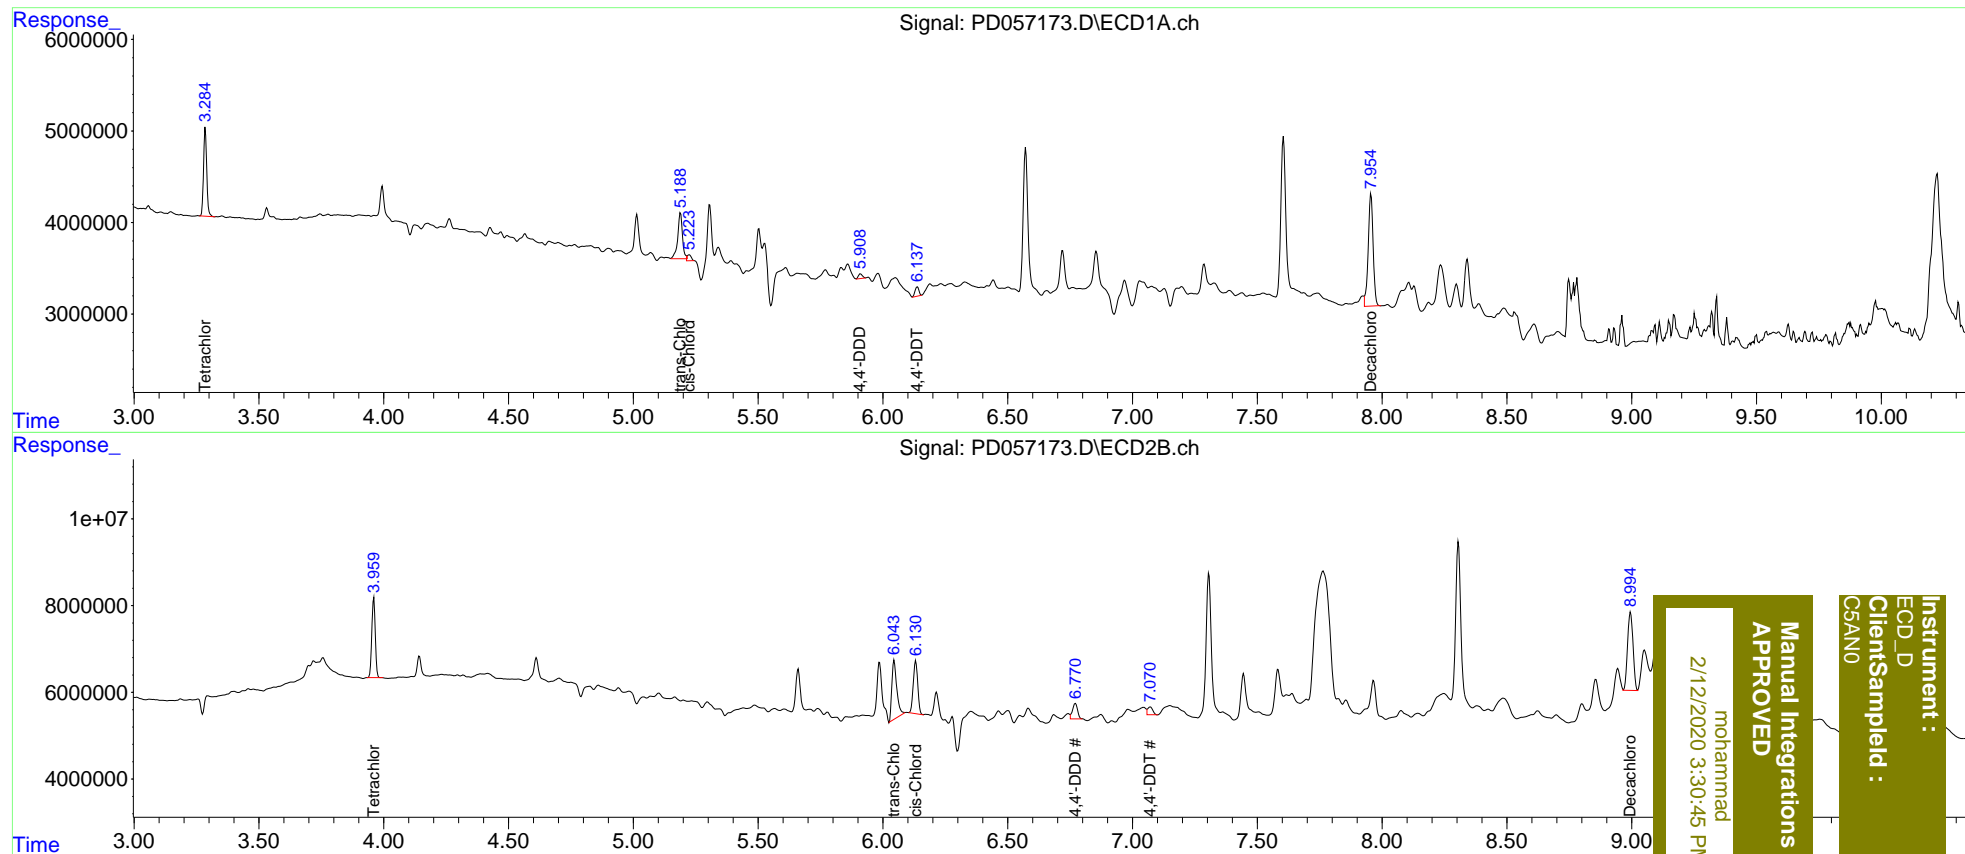

Instrument : ECD_D
 ClientSampleId : CSANO
 Manual Integrations APPROVED
 mohammad
 2/12/2020 3:30:45 PM