

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
 Data File : PD057171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2020 19:54
 Operator : AJ\MA
 Sample : L1302-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AM6

Manual Integrations
 APPROVED

mohammad
 2/12/2020 3:30:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 06:33:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	9905454	21784662	11.924	11.690
27)	SA Decachlor...	7.955	8.995	19782036	30558913	19.068	13.518 #
Target Compounds							
8)	B Heptachlo...	4.947	5.822	34017854	90666257	32.807	36.777m
10)	B trans-Chl...	5.172	6.056	49445027	348.1E6	45.744m	127.333 #
11)	B cis-Chlor...	5.224	6.129	150.2E6	716.3E6	140.495	279.620m#
12)	B 4,4'-DDE	5.392	6.282	2215523	8637331	2.004m	3.375m#
15)	B Endosulfa...	6.048	6.860	35458051	51450976	37.212	21.971 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021020\
Data File : PD057171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2020 19:54
Operator : AJ\MA
Sample : L1302-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 06:33:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

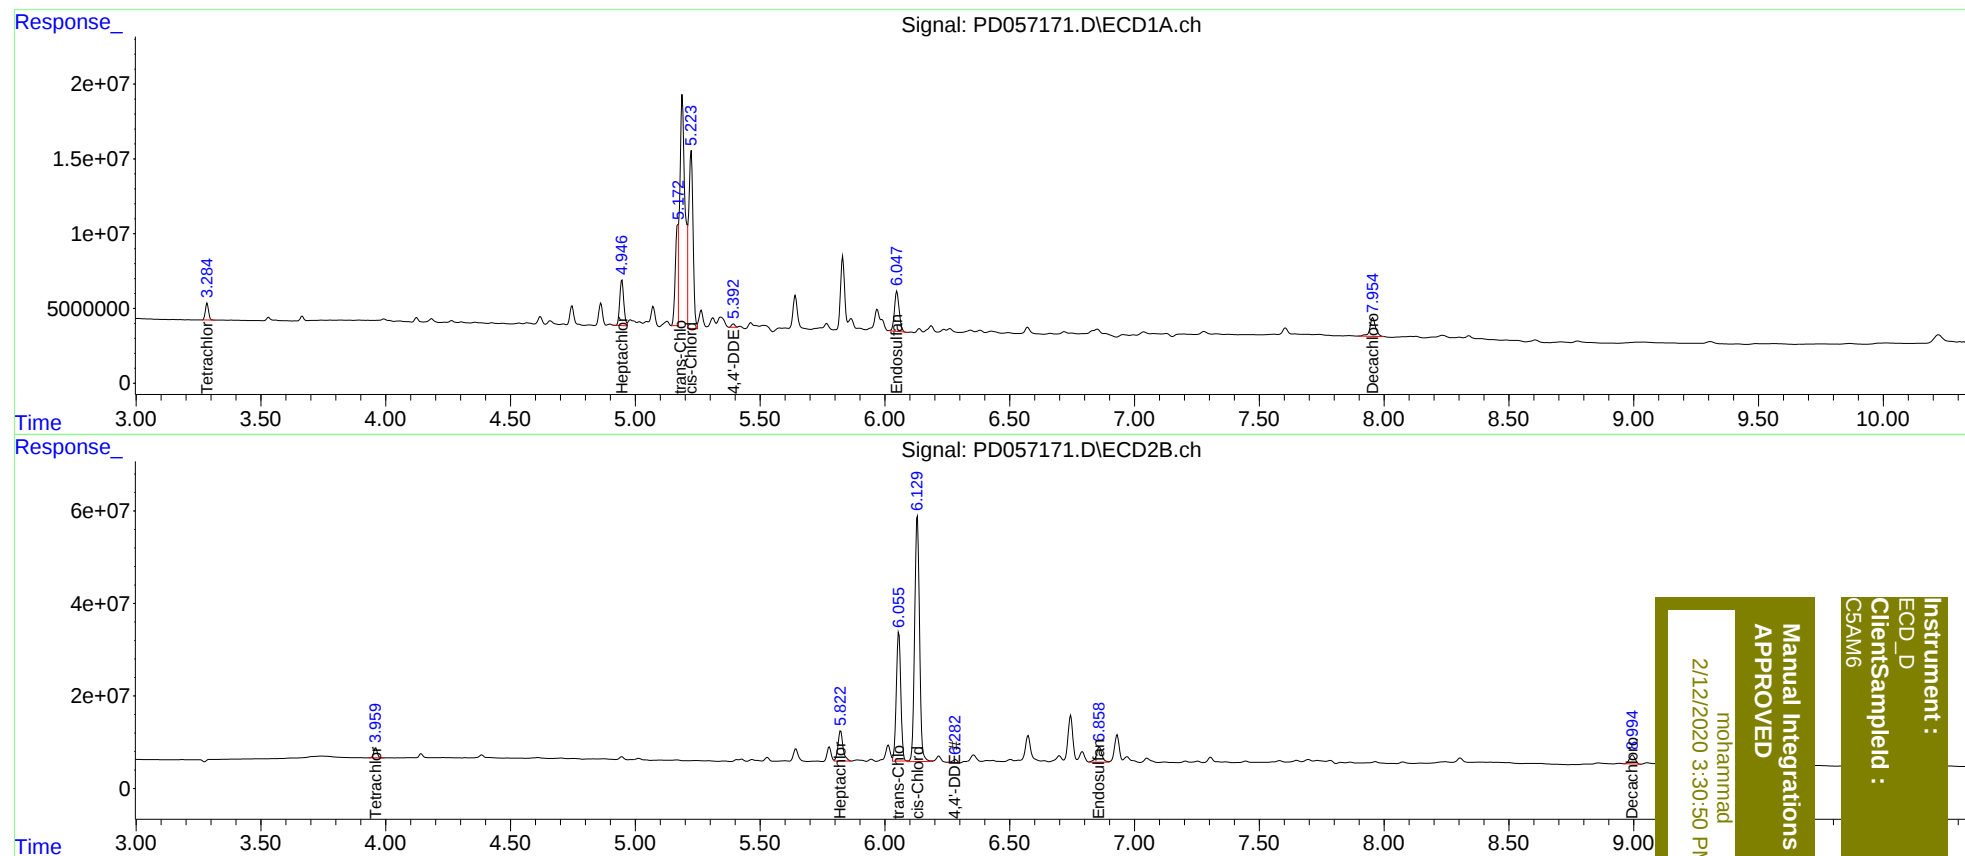

Manual Integrations
APPROVED

mohammad
2/12/2020 3:30:50 PM

Instrument :
ECD_D
Client Sampled :
CSAM6