

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021120\
 Data File : PD057193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 16:24
 Operator : AJ\MA
 Sample : L1424-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5B30

Manual Integrations
 APPROVED

mohammad
 2/24/2020 2:39:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 08:23:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.309	3.938	13622.1E6	25533.3E6	16398.232	13701.794m
27)	SA Decachlor...	7.956	8.997	22968209	39762141	22.139m	17.589m
Target Compounds							
14)	MA Endrin	5.771	6.666	8250875	16899688	9.389m	8.031m
15)	B Endosulfa...	6.051	6.847	17170785	27355571	18.020m	11.681m#
16)	A 4,4'-DDD	5.912	6.770	7113936	48492473	10.269m	23.519m#
20)	A Methoxychlor	6.687	7.518	8805707	9467747	31.452	10.494m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021120\
Data File : PD057193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 16:24
Operator : AJ\MA
Sample : L1424-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 08:23:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

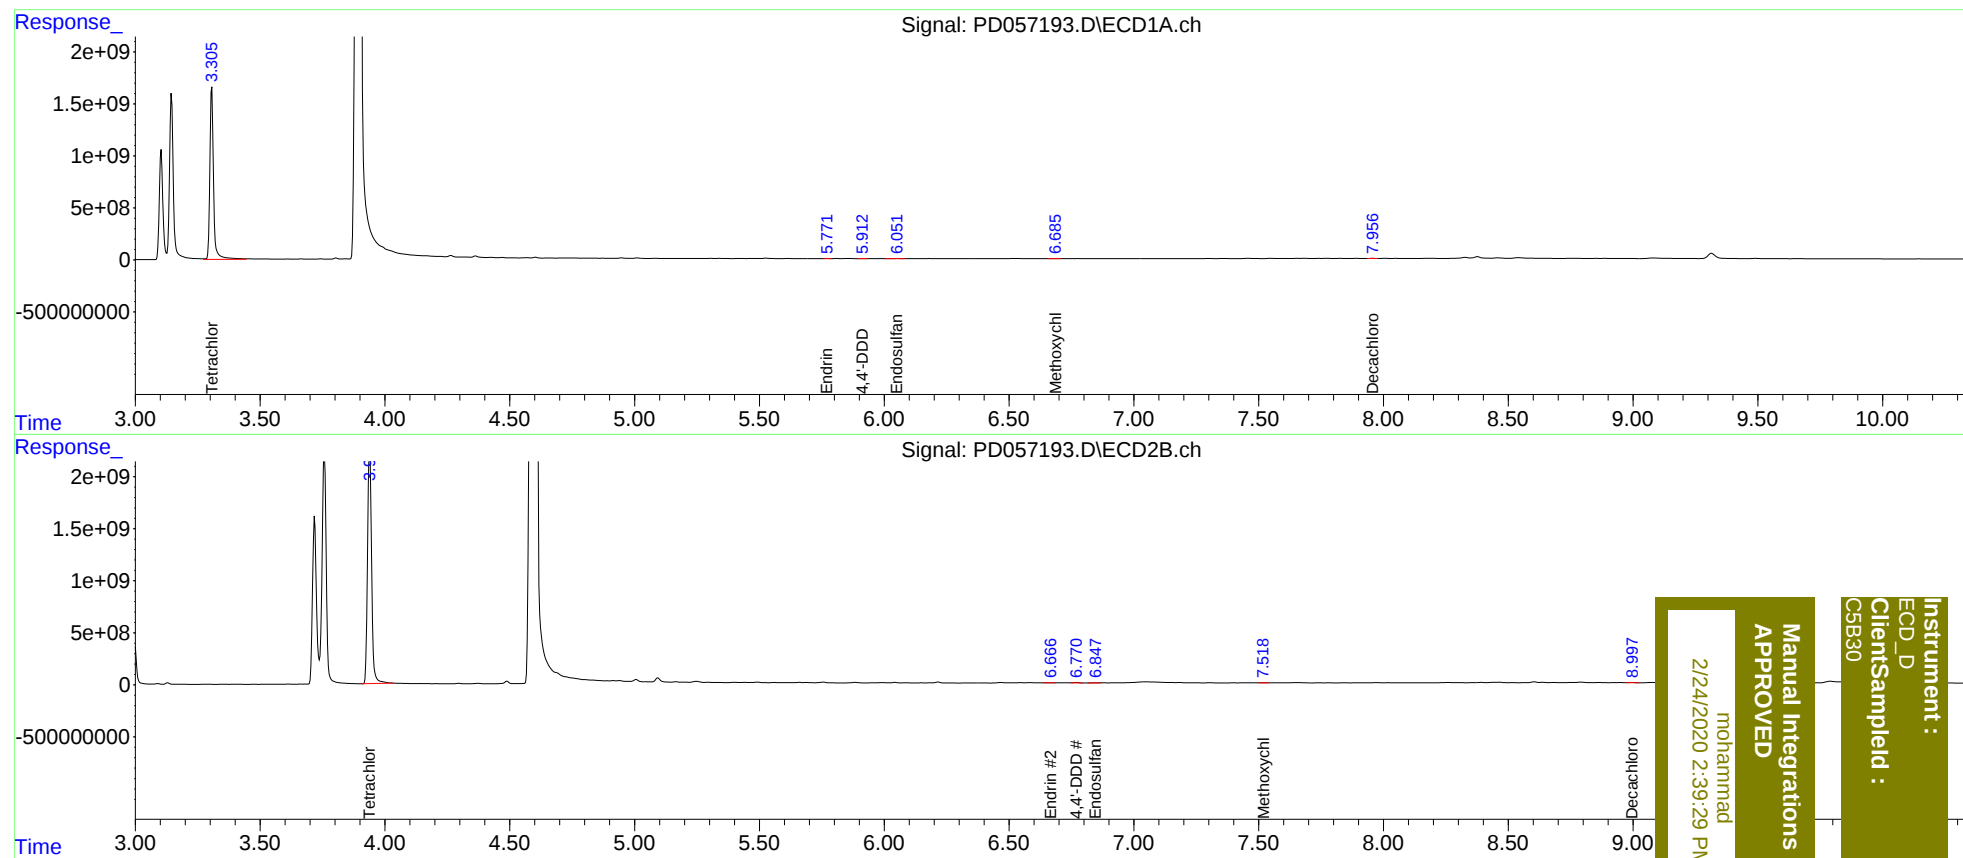

Manual Integrations
APPROVED

mohammad
2/24/2020 2:39:29 PM

Instrument :
ECD_D
ClientSampled :
C5B30