

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021120\
 Data File : PD057206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 21:23
 Operator : AJ\MA
 Sample : L1302-11DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 C5AM6DL

Manual Integrations
 APPROVED

mohammad
 2/13/2020 11:32:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 02:54:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.952	1709020	7092105	2.057	3.806m#
27)	SA Decachlor...	7.957	8.997	3769938	6734189	3.634	2.979m
Target Compounds							
8)	B Heptachlo...	4.948	5.822	6094588	19360137	5.878	7.853m#
10)	B trans-Chl...	5.176	6.056	13844135	66980567	12.808m	24.500m#
11)	B cis-Chlor...	5.226	6.132	26466085	137.9E6	24.763	53.824 #
15)	B Endosulfa...	6.050	6.860	7018490	10557460	7.366	4.508m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021120\
Data File : PD057206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 21:23
Operator : AJ\MA
Sample : L1302-11DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 02:54:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

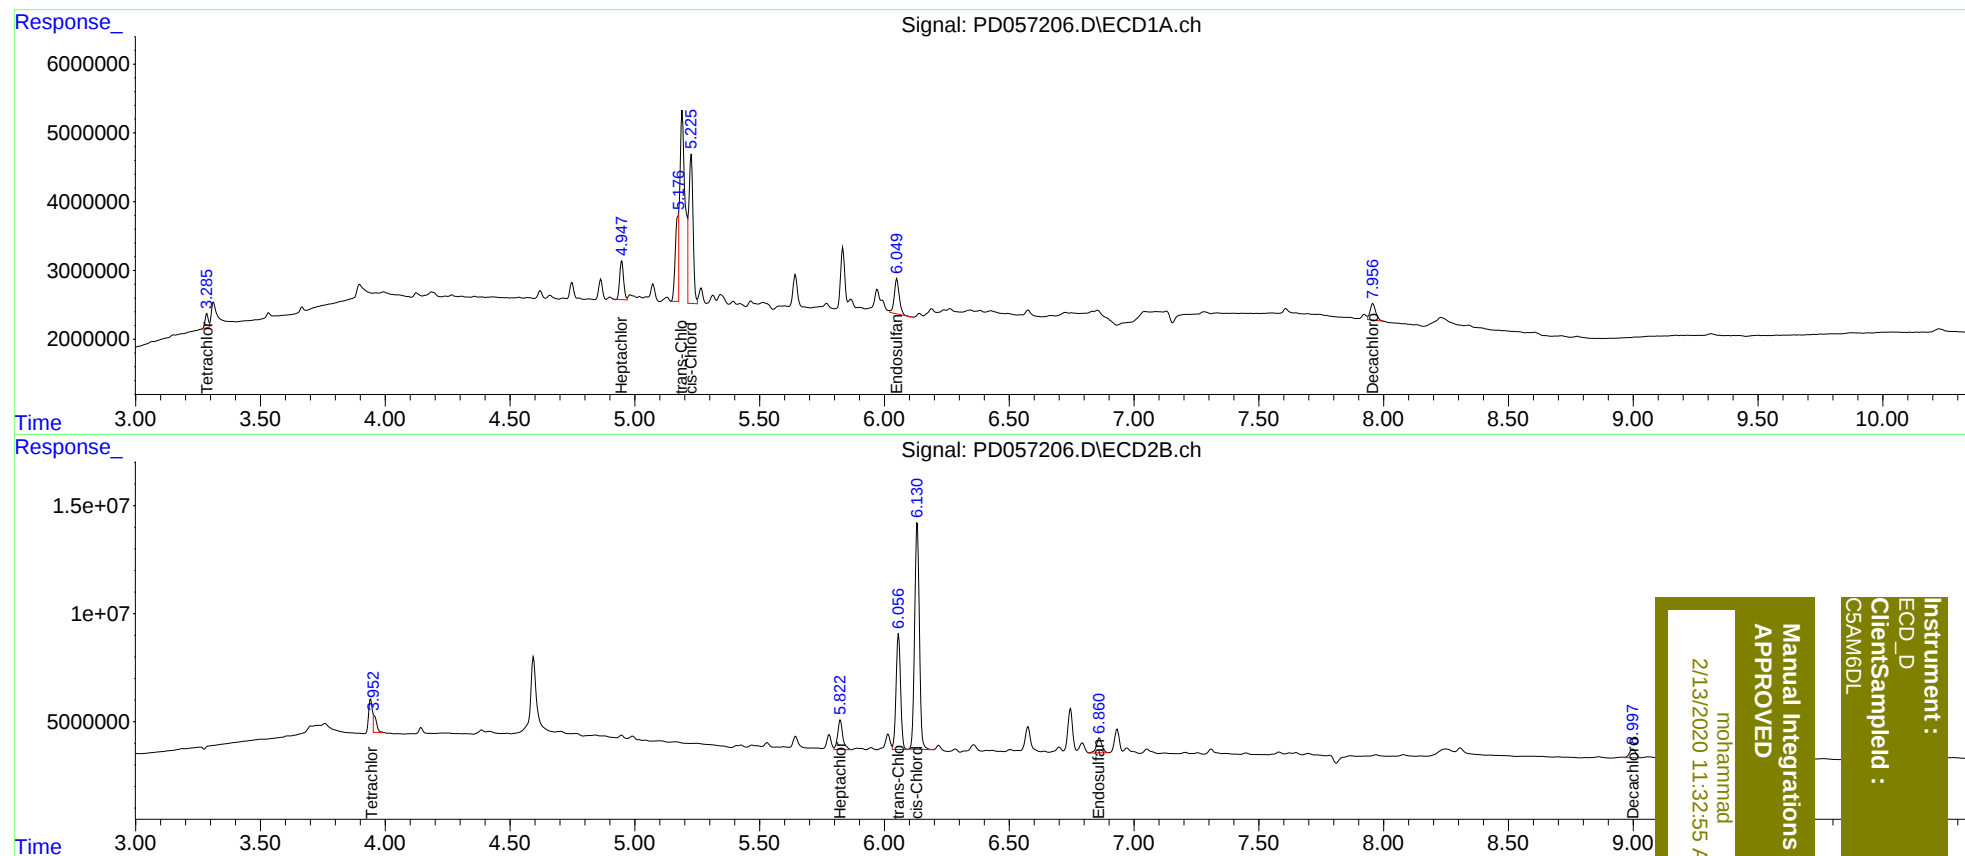

Manual Integrations
APPROVED

mohammad
2/13/2020 11:32:55 AM

Instrument :
ECD_D
ClientSampled :
C5AM6DL