

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021121\
 Data File : PD061204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2021 14:35
 Operator : DD\AJ
 Sample : M1310-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0A39

Manual Integrations
 APPROVED

Ankita
 2/12/2021 10:12:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 04:18:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.019	4505667	20703726	4.439	2.893m#
27)	SA Decachlor...	8.269	9.104	19598588	171.1E6	15.554	25.199m#
Target Compounds							
3)	MA gamma-BHC...	4.227	4.677	32793137	159.1E6	22.413	15.684 #
10)	B trans-Chl...	5.440	6.118	2421918	963.9E6	1.712m	102.536m#
11)	B cis-Chlor...	5.520	6.205	11085306	8182886	8.079	0.921 #
15)	B Endosulfa...	6.338	6.931	10071605	39280846	9.269	5.458 #
16)	A 4,4'-DDD	6.189	6.851	21635170	161.9E6	18.432m	22.752

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021121\
Data File : PD061204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2021 14:35
Operator : DD\AJ
Sample : M1310-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 04:18:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

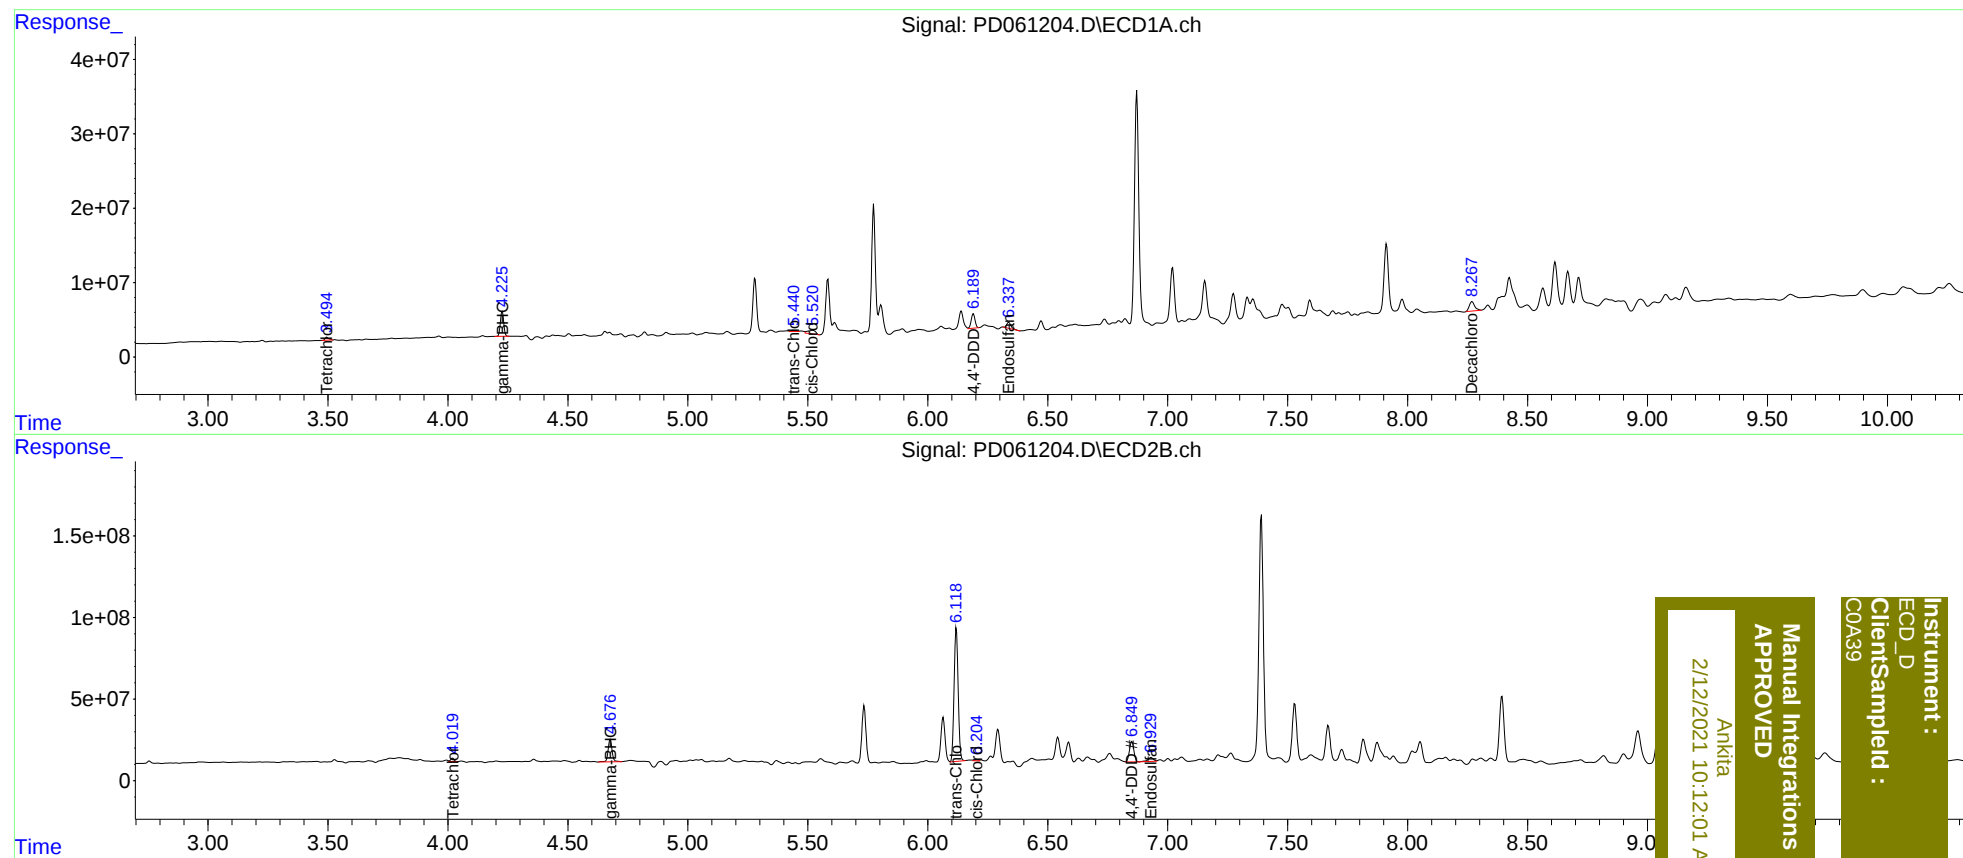

2/12/2021 10:12:01 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSample :
C0A39