

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021221\
 Data File : PD061224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2021 11:41
 Operator : DD\AJ
 Sample : M1375-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BJ2

Manual Integrations
 APPROVED

Ankita
 2/16/2021 8:20:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 01:33:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.020	24669618	148.9E6	24.305	20.812
2)	SA Decachlor...	8.279	9.105	34496258	184.2E6	27.377	27.131
Target Compounds							
10)	B trans-Chl...	5.436	6.133	2760939	8274875	1.952m	0.880m#
11)	B cis-Chlor...	5.509	6.208	787627	5862765	0.574m	0.660m
13)	MA Dieldrin	5.810	6.516	1997068	16004541	1.360m	1.722 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021221\
Data File : PD061224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2021 11:41
Operator : DD\AJ
Sample : M1375-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 01:33:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

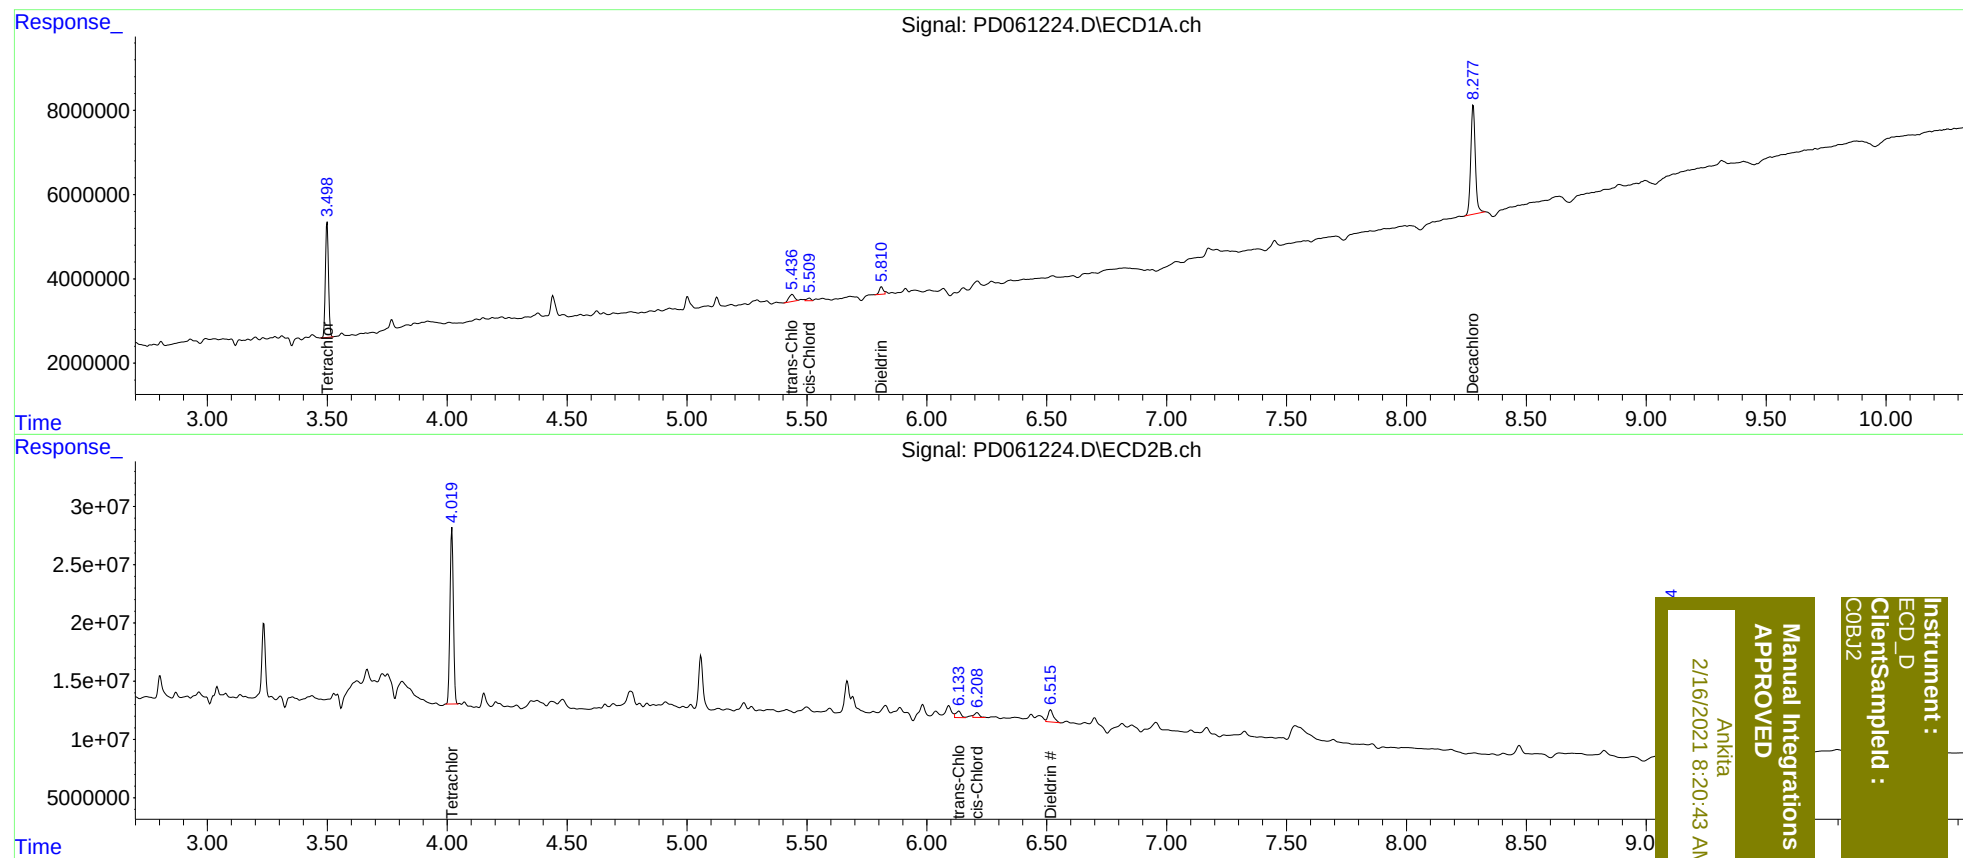

2/16/2021 8:20:43 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C0B32