

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
 Data File : PD073944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 09:17
 Operator : AR\AJ
 Sample : PIBLK206
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:06:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.776	50641444	29018498	21.385	22.861
27)	SA Decachlor...	9.106	7.934	97812320	52376414	35.453	43.519
Target Compounds							
3)	MA gamma-BHC...	4.387f	0.000	143323	0	<MDL	N.D. #
4)	MA Heptachlor	4.953	0.000	1092123	0	0.300	N.D. #
6)	B beta-BHC	4.565f	0.000	261611	0	0.156	N.D. #
7)	B delta-BHC	4.782	0.000	1098332	0	0.336	N.D. #
8)	B Heptachlo...	5.704	0.000	713215	0	0.219	N.D. #
9)	A Endosulfan I	6.078	0.000	852143	0	0.278	N.D. #
11)	B cis-Chlor...	6.078f	0.000	852143	0	0.256	N.D. #
12)	B 4,4'-DDE	6.190	0.000	1336145	0	0.424	N.D. #
13)	MA Dieldrin	6.415f	0.000	1381076	0	0.411	N.D. #
21)	B Endrin ke...	7.702	0.000	939884	0	0.295	N.D. #
23)	Toxaphene-2	6.452	0.000	958219	0	32.557	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
Data File : PD073944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 09:17
Operator : AR\AJ
Sample : PIBLK206
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:06:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

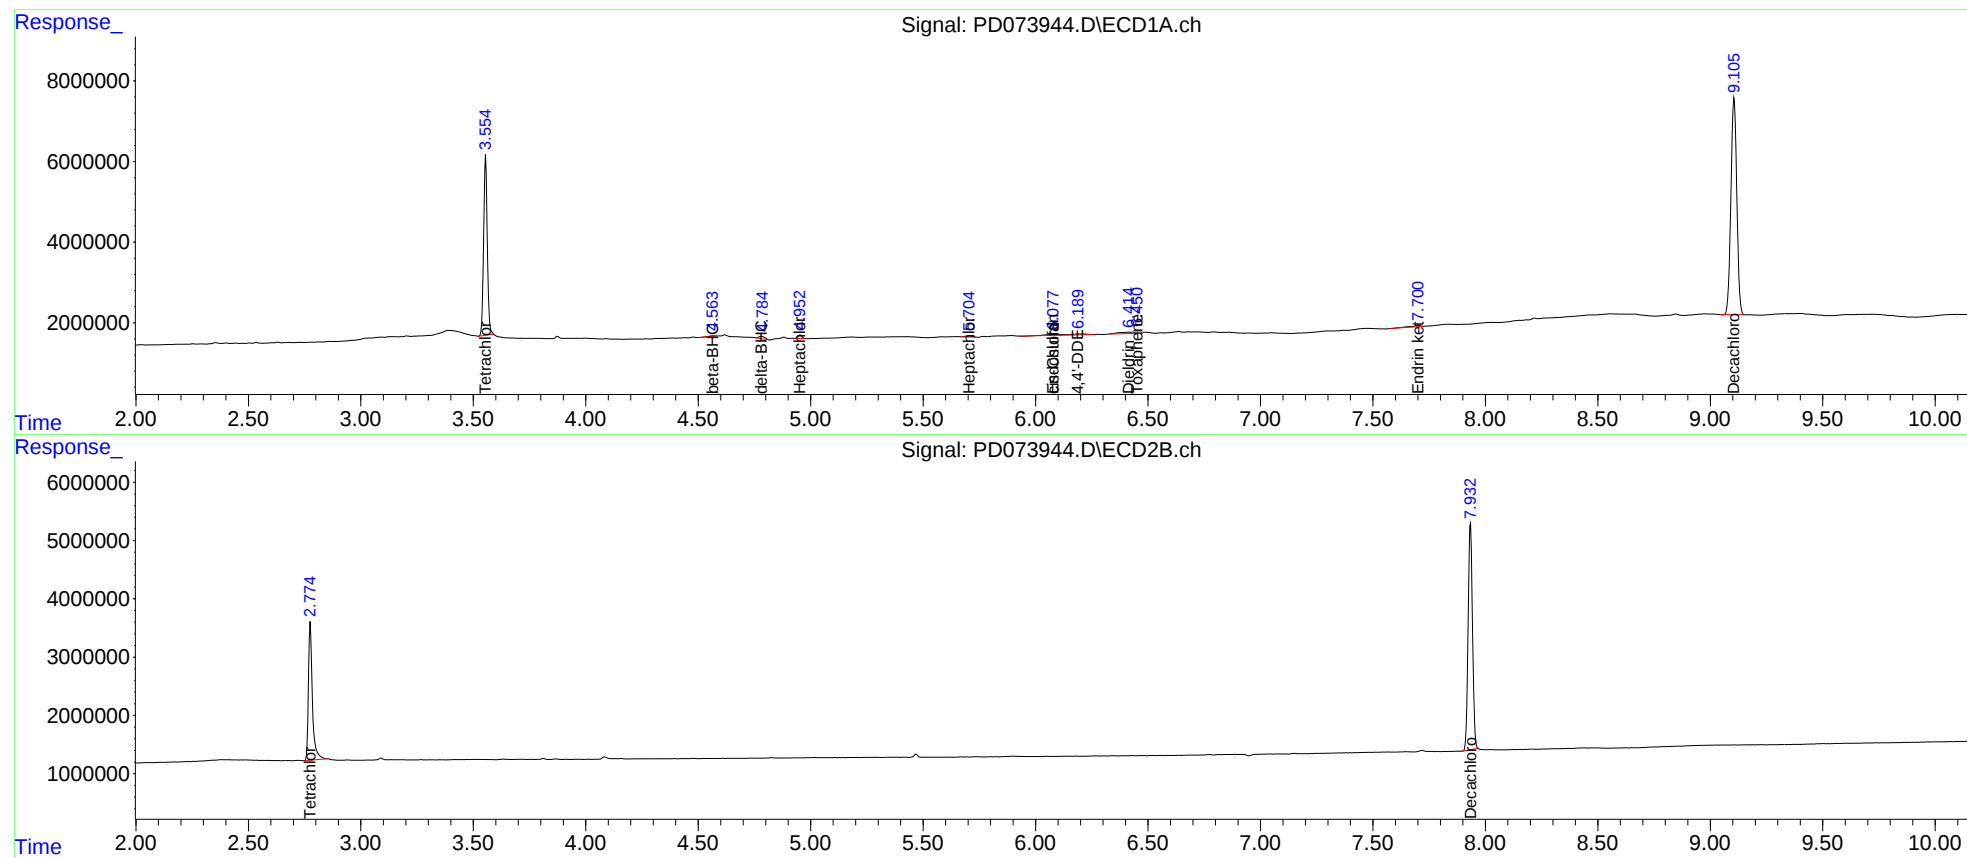

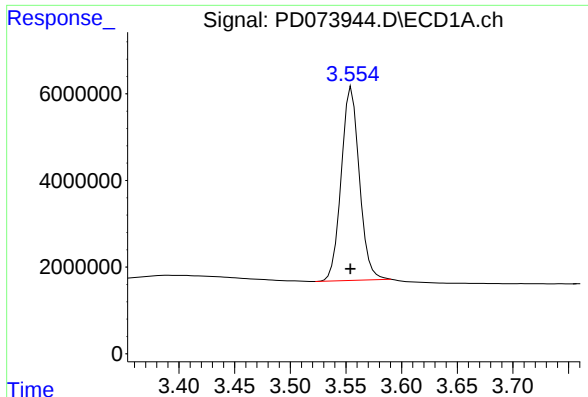


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.001 min
Response: 50641444
Conc: 21.38 ng/ml

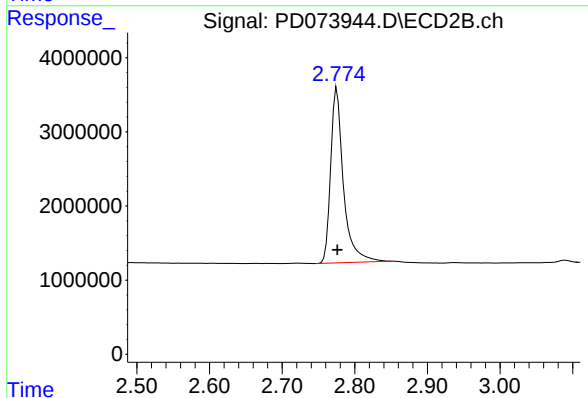


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 29018498
Conc: 22.86 ng/ml

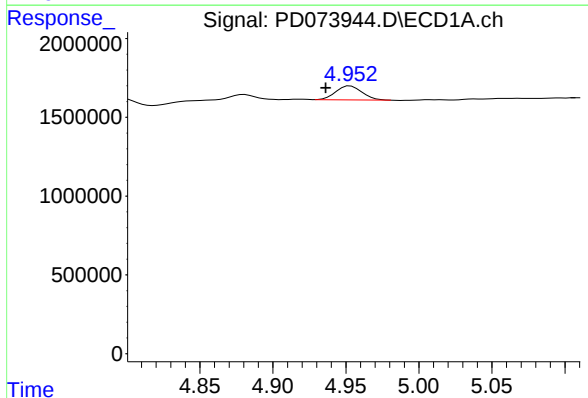


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.017 min
Response: 1092123
Conc: 0.30 ng/ml

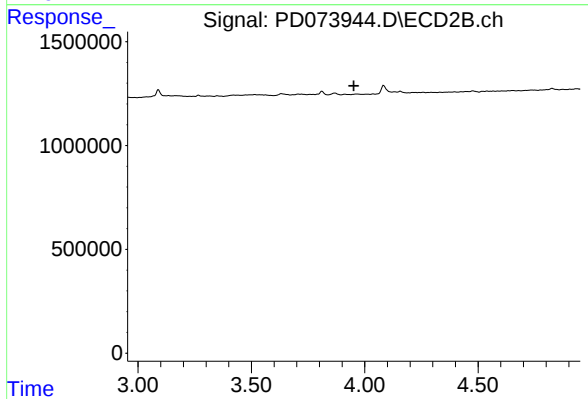


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 3.952 min
Response: 0
Conc: N.D.

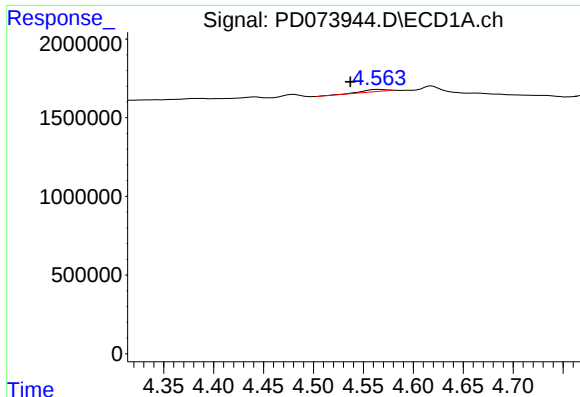


#6 beta-BHC

R.T.: 4.565 min
Delta R.T.: 0.028 min
Response: 261611
Conc: 0.16 ng/ml

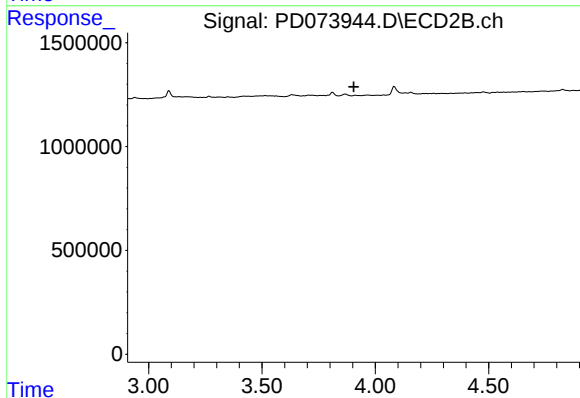


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.905 min
Response: 0
Conc: N.D.

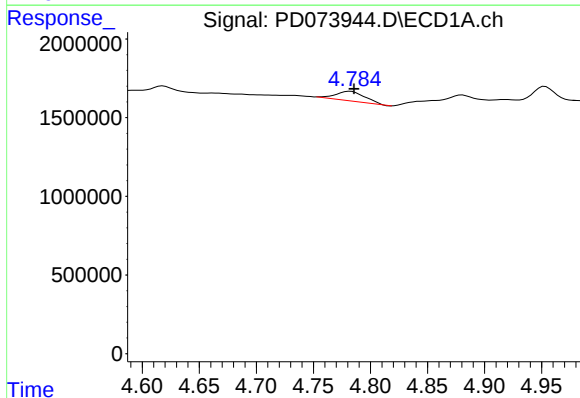


#7 delta-BHC

R.T.: 4.782 min
Delta R.T.: -0.003 min
Response: 1098332
Conc: 0.34 ng/ml

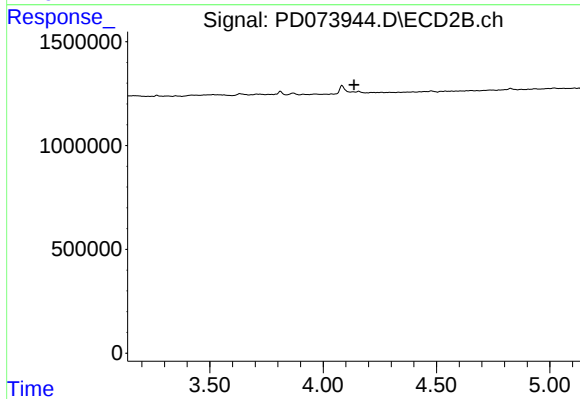


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

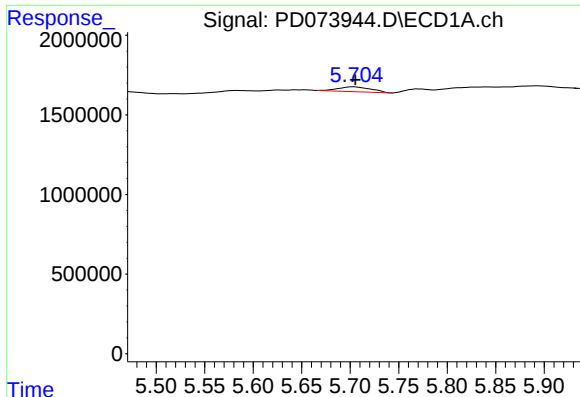


#8 Heptachlor epoxide

R.T.: 5.704 min
Delta R.T.: -0.002 min
Response: 713215
Conc: 0.22 ng/ml

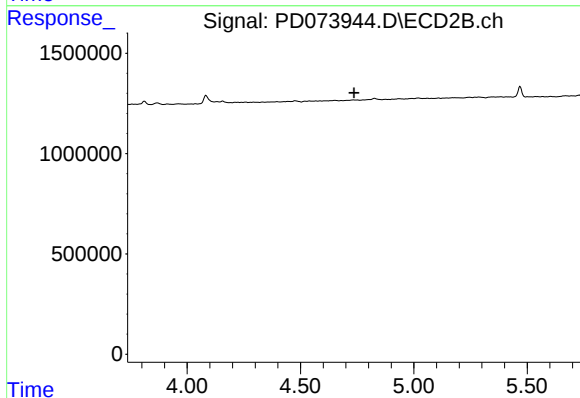


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.737 min
Response: 0
Conc: N.D.

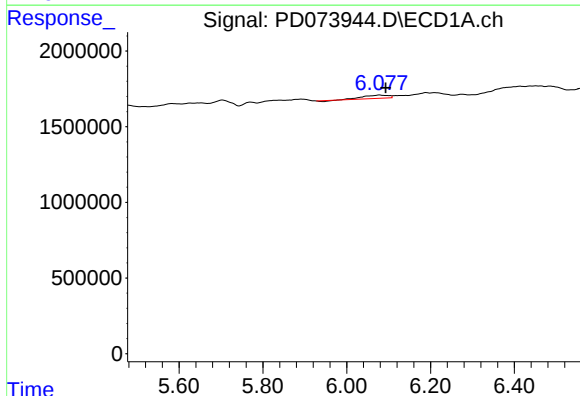


#9 Endosulfan I

R.T.: 6.078 min
Delta R.T.: -0.015 min
Response: 852143
Conc: 0.28 ng/ml

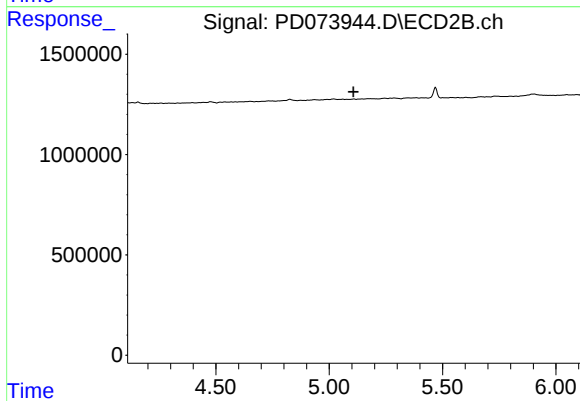


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.107 min
Response: 0
Conc: N.D.

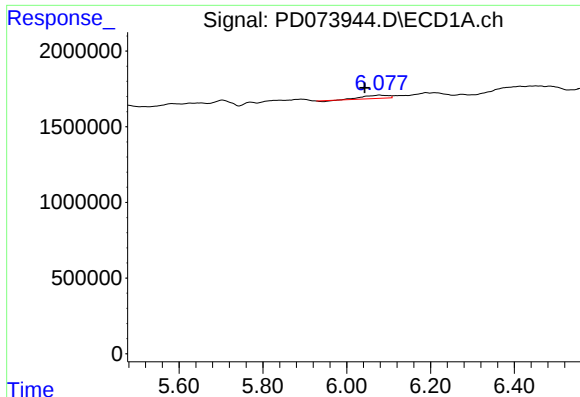


#11 cis-Chlordane

R.T.: 6.078 min
Delta R.T.: 0.036 min
Response: 852143
Conc: 0.26 ng/ml

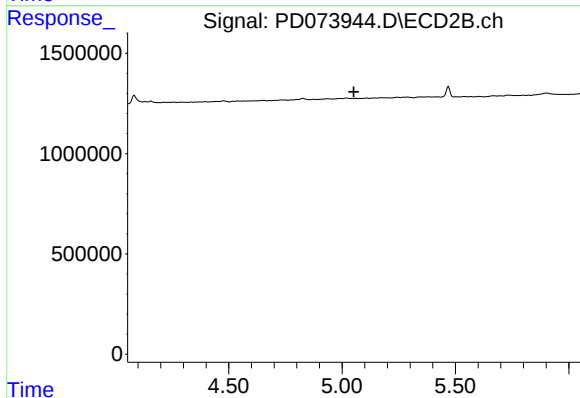


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.052 min
Response: 0
Conc: N.D.

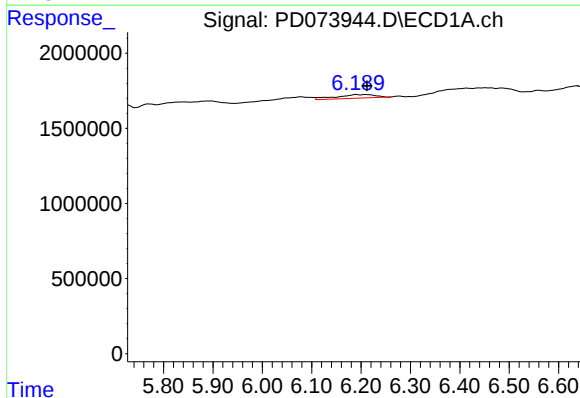


#12 4,4'-DDE

R.T.: 6.190 min
Delta R.T.: -0.022 min
Response: 1336145
Conc: 0.42 ng/ml

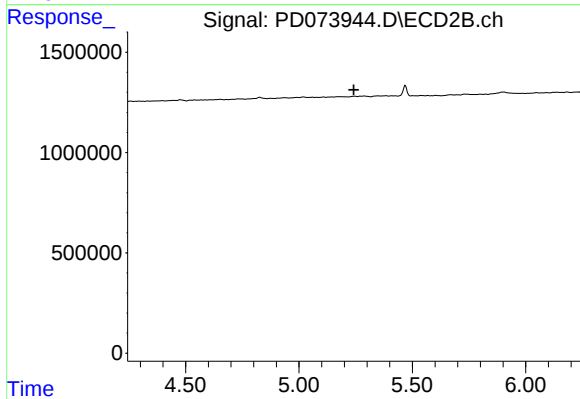


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

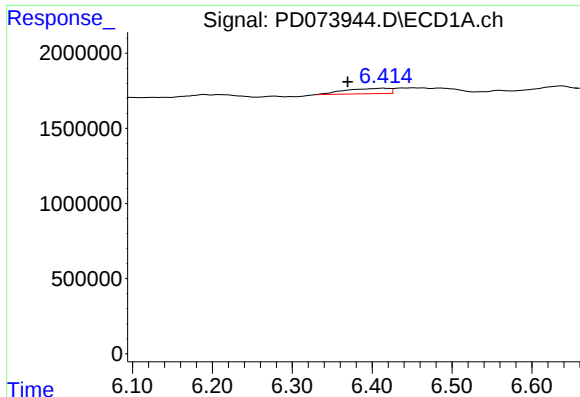


#13 Dieldrin

R.T.: 6.415 min
Delta R.T.: 0.046 min
Response: 1381076
Conc: 0.41 ng/ml

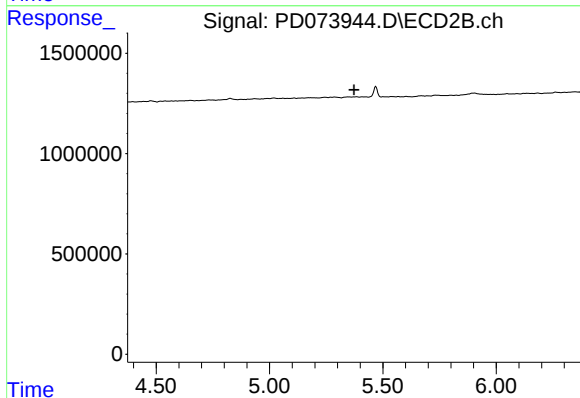


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.373 min
Response: 0
Conc: N.D.

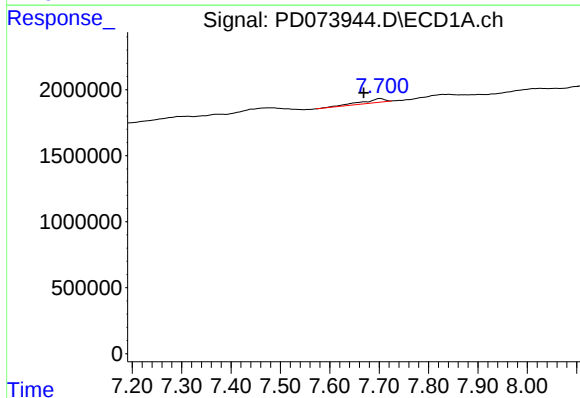


#21 Endrin ketone

R.T.: 7.702 min
Delta R.T.: 0.033 min
Response: 939884
Conc: 0.29 ng/ml

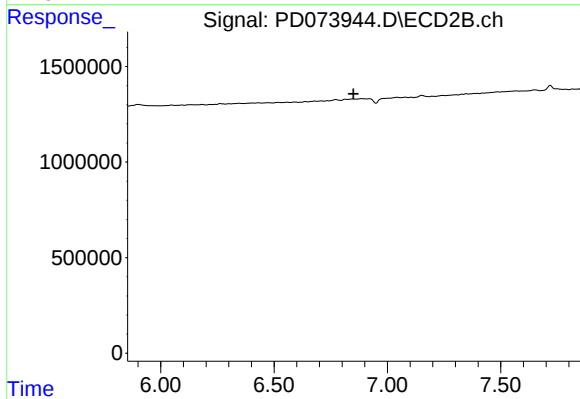


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.851 min
Response: 0
Conc: N.D.

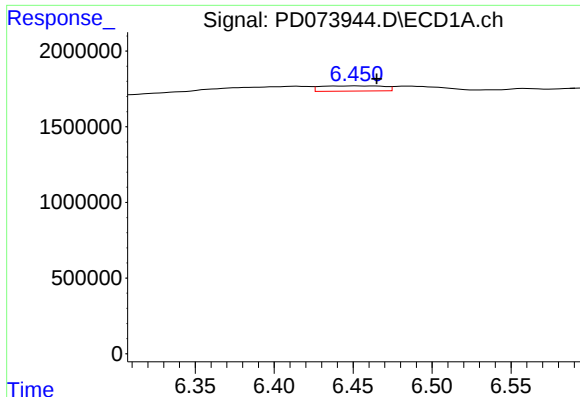


#23 Toxaphene-2

R.T.: 6.452 min
Delta R.T.: -0.013 min
Response: 958219
Conc: 32.56 ng/ml

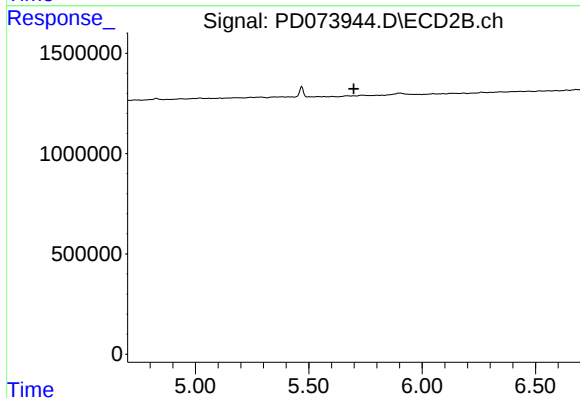


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 5.698 min
Response: 0
Conc: N.D.

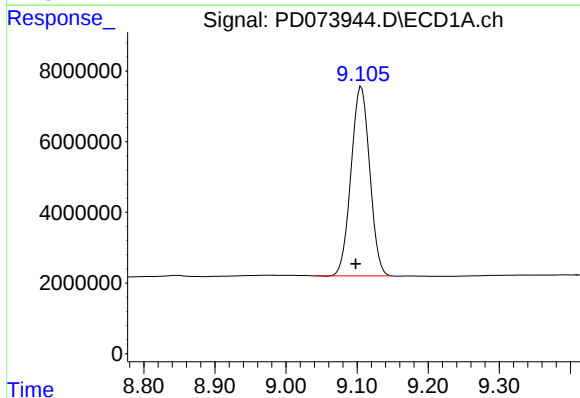

#27 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.008 min
Response: 97812320
Conc: 35.45 ng/ml

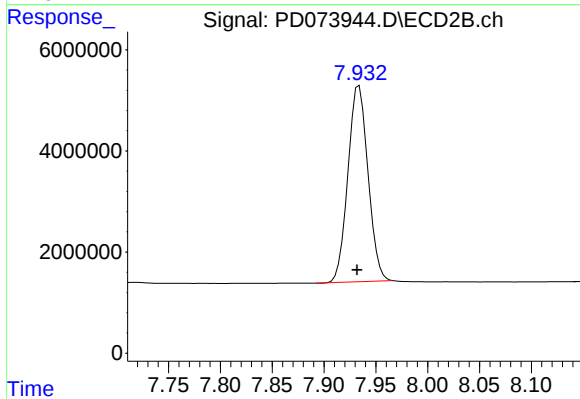

#27 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.002 min
Response: 52376414
Conc: 43.52 ng/ml