

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
 Data File : PD073955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 15:05
 Operator : AR\AJ
 Sample : INDA363
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:14:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.775	48658051	27446322	20.547	21.622
27)	SA Decachlor...	9.107	7.934	103.2E6	50519650	37.419	41.976
Target Compounds							
2)	A alpha-BHC	4.012	3.280	78800969	38304376	20.689	21.615
3)	MA gamma-BHC...	4.346	3.610	76709980	36201616	21.061	21.534
4)	MA Heptachlor	4.939	3.953	77889865	34019579	21.407	22.557
9)	A Endosulfan I	6.097	5.109	64455671	30539586	21.004	21.281
13)	MA Dieldrin	6.373	5.374	140.4E6	66854450	41.770	42.953
14)	MA Endrin	6.604	5.650	117.6E6	57023171	42.035	44.305
16)	A 4,4'-DDD	6.736	5.798	107.0E6	51837470	42.052	42.977
17)	MA 4,4'-DDT	7.052	6.050	114.4E6	52025460	41.933	44.070
20)	A Methoxychlor	7.527	6.626	312.5E6	125.2E6	209.988	227.041

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
Data File : PD073955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 15:05
Operator : AR\AJ
Sample : INDA363
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:14:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

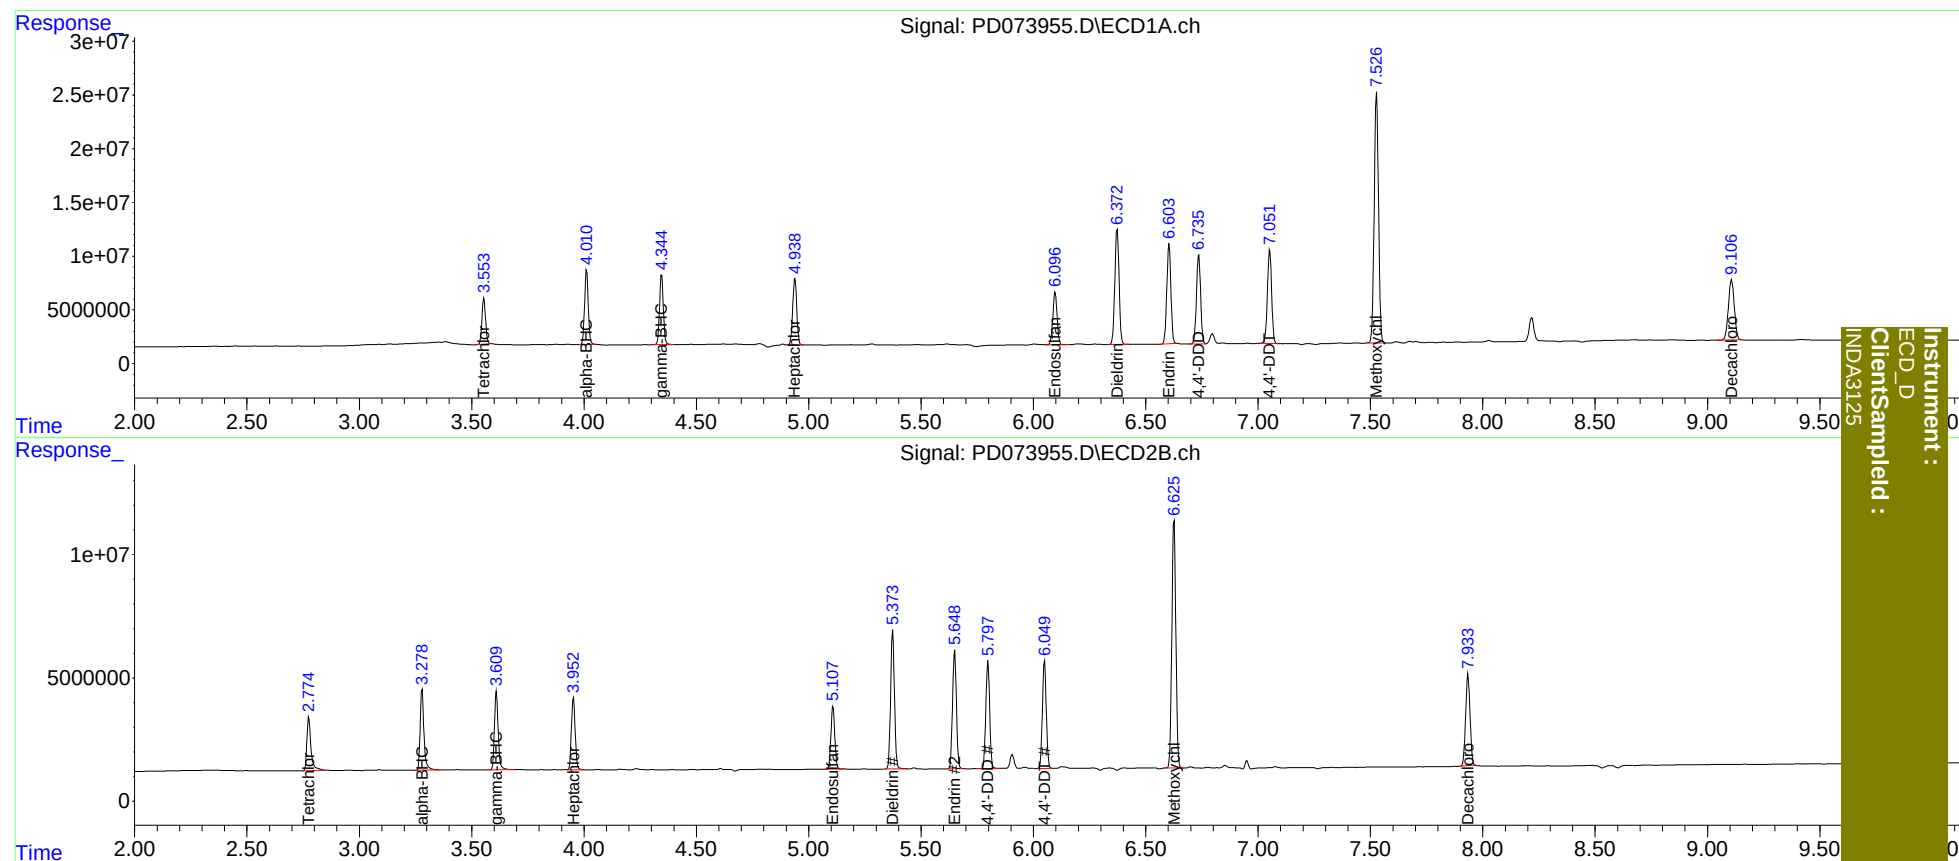

Instrument :
ECD_D
ClientSampled :
INDA3125