

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
 Data File : PD073949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 11:30
 Operator : AR\AJ
 Sample : 01422-06MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B64MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/14/2023
 Supervised By :Ankita Jodhani 02/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:10:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.775	32142620	16858971	13.573	13.281
27)	SA Decachlor...	9.105	7.933	50555332	26220592	18.324	21.786
Target Compounds							
2)	A alpha-BHC	4.012	3.279	224.4E6	103.2E6	58.911	58.241
3)	MA gamma-BHC...	4.345	3.610	207.2E6	96666540	56.900	57.500
4)	MA Heptachlor	4.938	3.953	210.6E6	87478196	57.869	58.003
5)	MB Aldrin	5.282	4.234	215.0E6	100.8E6	60.087	59.357
6)	B beta-BHC	4.539	3.905	88532859	42553473	52.712	52.058
7)	B delta-BHC	4.788	4.137	191.1E6	91161672	58.483	52.558
8)	B Heptachlo...	5.707	4.736	185.9E6	87498846	57.149m	56.194m
9)	A Endosulfan I	6.096	5.108	176.5E6	82832883	57.528	57.721
10)	B trans-Chl...	5.965	4.988	189.4E6	91539740	58.816	58.615
11)	B cis-Chlor...	6.045	5.053	195.6E6	90682673	58.685	56.415
12)	B 4,4'-DDE	6.217	5.243	372.1E6	174.9E6	118.020	119.118
13)	MA Dieldrin	6.372	5.374	403.9E6	184.9E6	120.207	118.804
14)	MA Endrin	6.603	5.650	336.8E6	156.4E6	120.388	121.491
15)	B Endosulfa...	6.821	5.943	326.8E6	157.1E6	110.558	114.179
16)	A 4,4'-DDD	6.735	5.799	297.9E6	135.8E6	117.080	112.551
17)	MA 4,4'-DDT	7.051	6.050	334.5E6	143.9E6	122.560	121.933
18)	B Endrin al...	6.951	6.123	234.0E6	110.5E6	97.867	101.212
19)	B Endosulfa...	7.186	6.346	300.2E6	140.8E6	108.049	111.995
20)	A Methoxychlor	7.526	6.626	838.9E6	307.9E6	563.620	558.305
21)	B Endrin ke...	7.674	6.853	352.9E6	172.9E6	110.702	114.922

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
Data File : PD073949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 11:30
Operator : AR\AJ
Sample : 01422-06MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:10:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

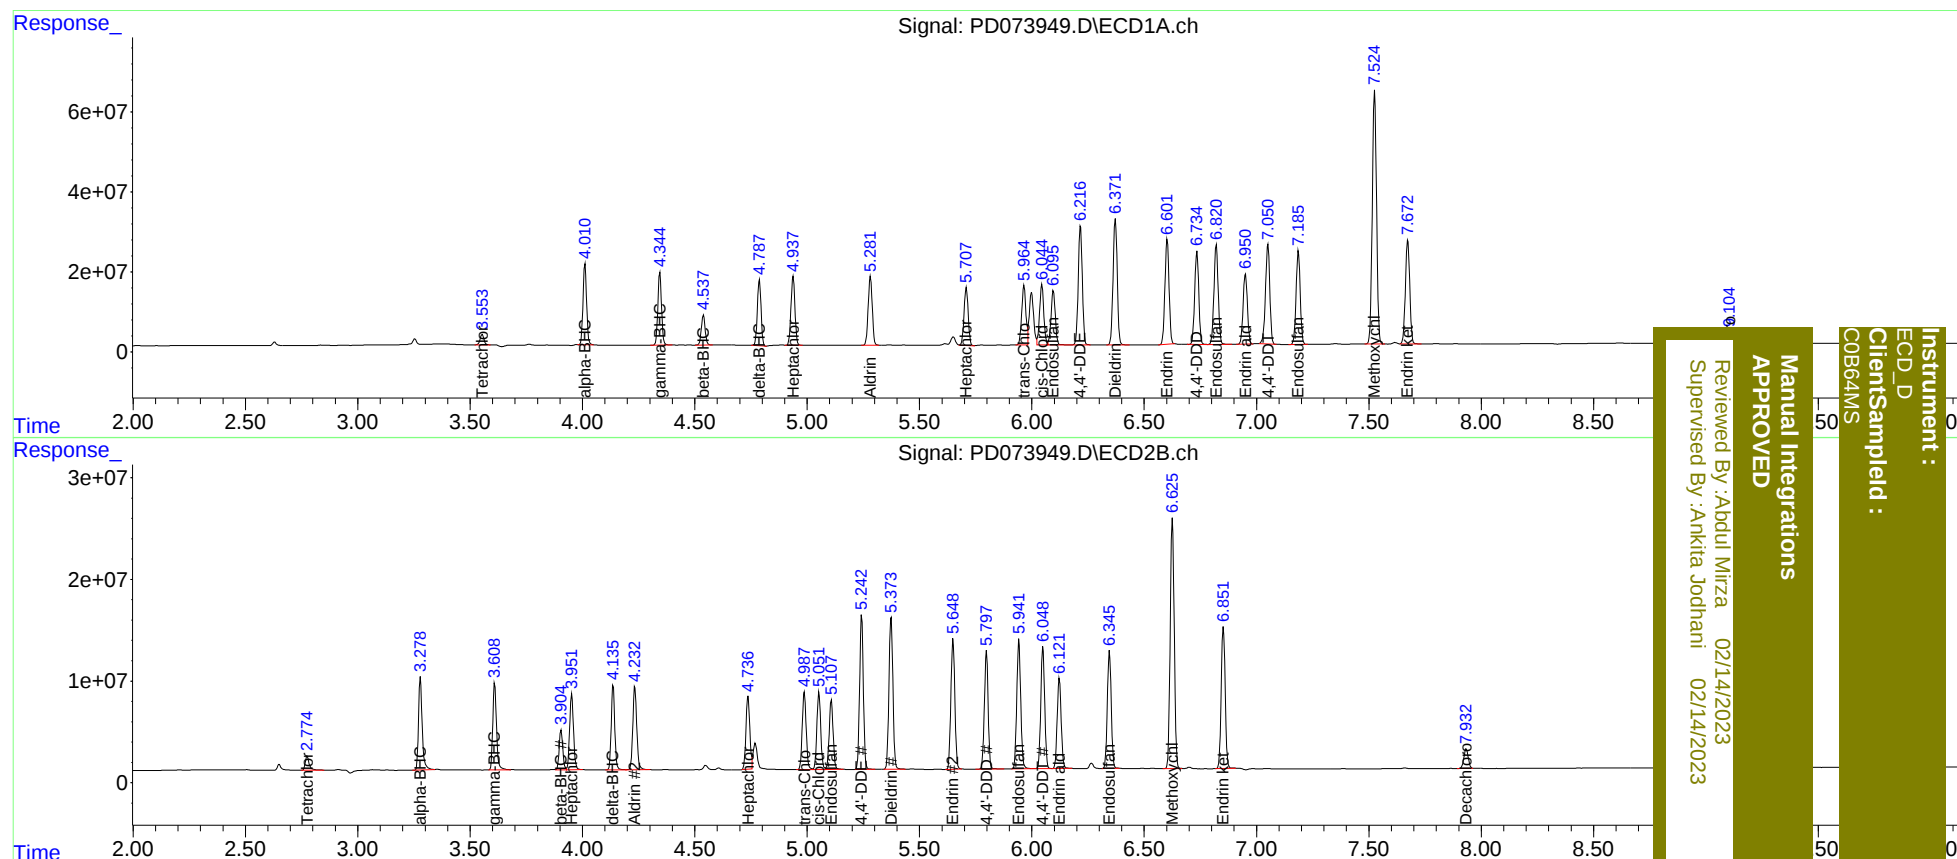

Instrument :
ECD_D
ClientSampled :
C0B64MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 02/14/2023
Supervised By: Ankita Jodhani 02/14/2023