

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
 Data File : PD073950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 11:43
 Operator : AR\AJ
 Sample : 01422-07MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B64MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/14/2023
 Supervised By :Ankita Jodhani 02/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:11:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.775	31690429	16496988	13.382	12.996
2)	SA Decachlor...	9.104	7.933	50522390	26178831	18.312	21.752
Target Compounds							
2)	A alpha-BHC	4.011	3.279	222.5E6	102.7E6	58.411	57.967
3)	MA gamma-BHC...	4.345	3.610	205.7E6	96150181	56.477	57.193
4)	MA Heptachlor	4.938	3.952	209.4E6	87569023	57.540	58.063
5)	MB Aldrin	5.282	4.234	214.1E6	100.5E6	59.847	59.177
6)	B beta-BHC	4.538	3.905	88277563	42292046	52.560	51.738
7)	B delta-BHC	4.788	4.137	189.8E6	90853750	58.072	52.381
8)	B Heptachlo...	5.707	4.735	184.9E6	82964966	56.842m	53.282m
9)	A Endosulfan I	6.096	5.107	176.4E6	82431172	57.469	57.441
10)	B trans-Chl...	5.965	4.988	187.4E6	91067086	58.213	58.312
11)	B cis-Chlor...	6.045	5.052	195.7E6	90338084	58.714	56.201
12)	B 4,4'-DDE	6.217	5.242	370.3E6	174.5E6	117.447	118.802
13)	MA Dieldrin	6.372	5.373	402.1E6	184.9E6	119.663	118.792
14)	MA Endrin	6.603	5.649	335.8E6	156.7E6	120.035	121.781
15)	B Endosulfa...	6.820	5.942	325.6E6	156.7E6	110.164	113.907
16)	A 4,4'-DDD	6.734	5.797	297.2E6	135.9E6	116.818	112.631
17)	MA 4,4'-DDT	7.050	6.049	333.3E6	144.5E6	122.135	122.369
18)	B Endrin al...	6.950	6.122	234.0E6	110.8E6	97.859	101.459
19)	B Endosulfa...	7.186	6.345	299.3E6	140.4E6	107.716	111.622
20)	A Methoxychlor	7.525	6.625	839.6E6	309.5E6	564.106	561.187
21)	B Endrin ke...	7.672	6.852	352.7E6	172.6E6	110.647	114.779

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021323\
Data File : PD073950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 11:43
Operator : AR\AJ
Sample : 01422-07MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:11:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

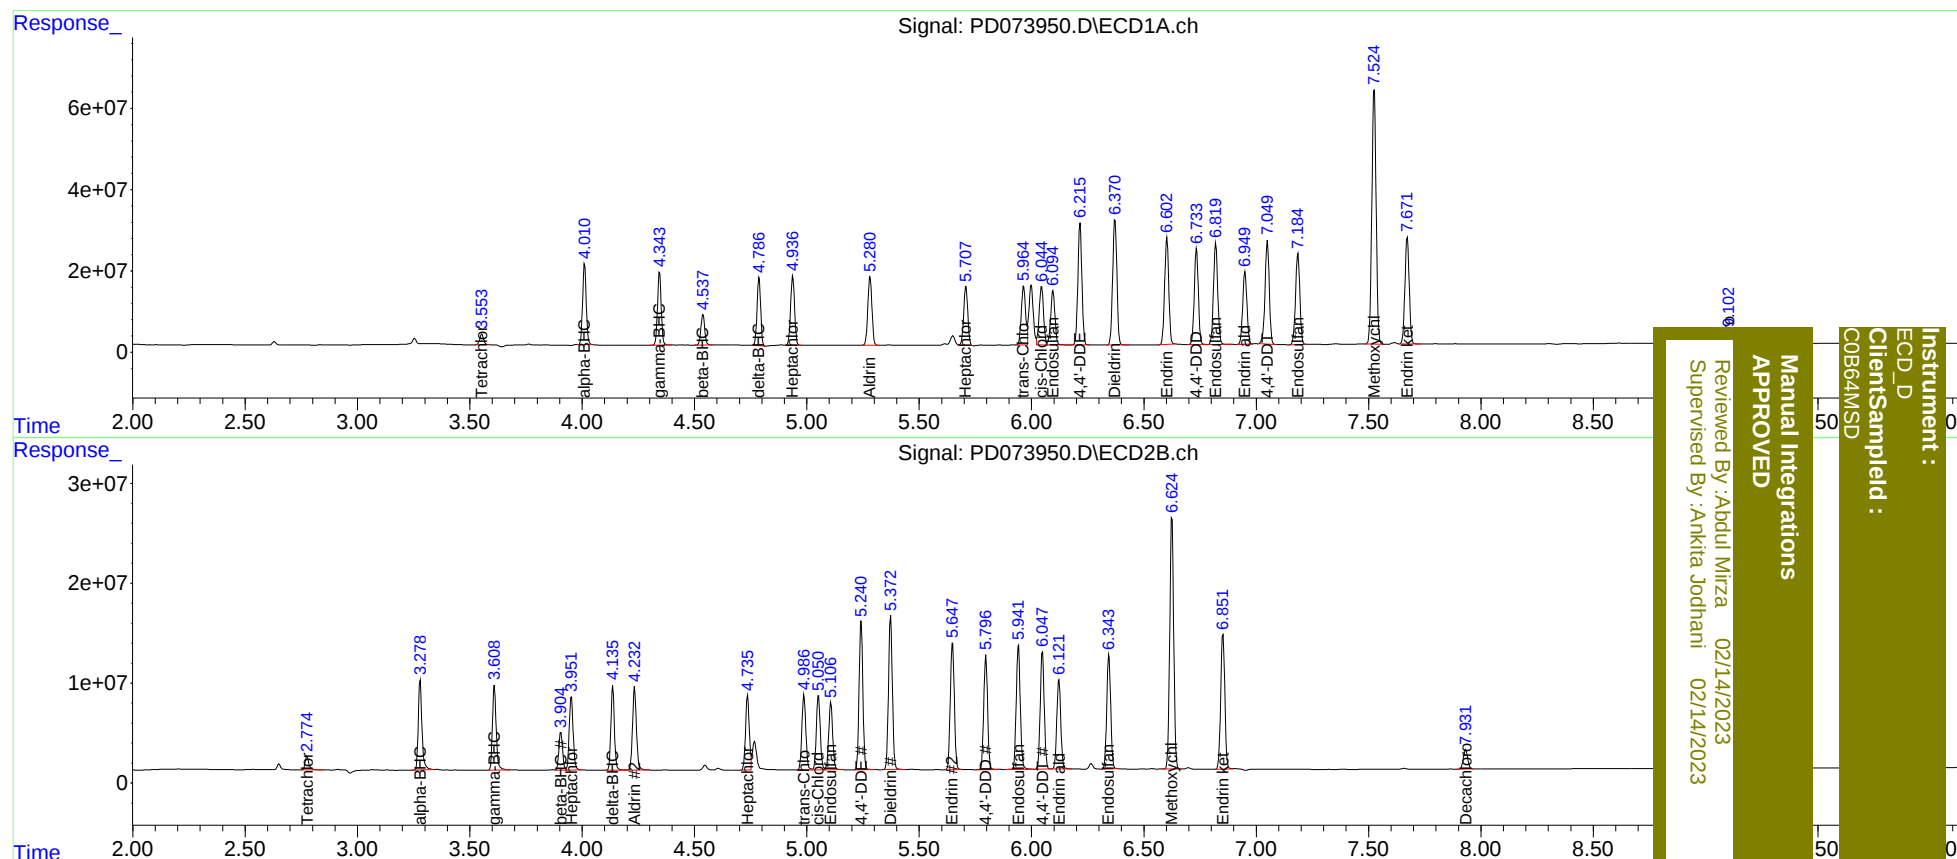

Instrument :
ECD_D
Client Sampled :
C0B64MSD

Manual Integrations
APPROVED

Reviewed By : Abdul Miza 02/14/2023
Supervised By : Ankita Jodhani 02/14/2023