

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
 Data File : PD081312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 21:25
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDB4027

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 11:38:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 13 11:33:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	56647838	97082096	41.100	39.123
27)	SA Decachlor...	9.113	7.932	149.8E6	201.6E6	76.398	77.745
Target Compounds							
5)	MB Aldrin	5.292	4.246	94595391	143.5E6	40.989	40.265
6)	B beta-BHC	4.550	3.920	41831621	67024659	39.498	38.381
7)	B delta-BHC	4.800	4.152	100.6E6	159.0E6	42.128	40.669
8)	B Heptachlo...	5.719	4.748	87128256	132.1E6	39.820	39.747
10)	B trans-Chl...	5.975	4.998	84997272	127.3E6	40.251	39.839
11)	B cis-Chlor...	6.055	5.062	86465498	124.4E6	39.654	39.569
12)	B 4,4'-DDE	6.226	5.250	169.0E6	251.9E6	80.820	81.414
15)	B Endosulfa...	6.830	5.950	152.3E6	230.7E6	79.046	80.094
18)	B Endrin al...	6.960	6.129	117.9E6	177.9E6	79.064	78.314
19)	B Endosulfa...	7.195	6.352	146.1E6	220.1E6	79.458	78.814
21)	B Endrin ke...	7.681	6.858	158.6E6	251.6E6	79.894	79.149

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
Data File : PD081312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 21:25
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 11:38:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 13 11:33:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

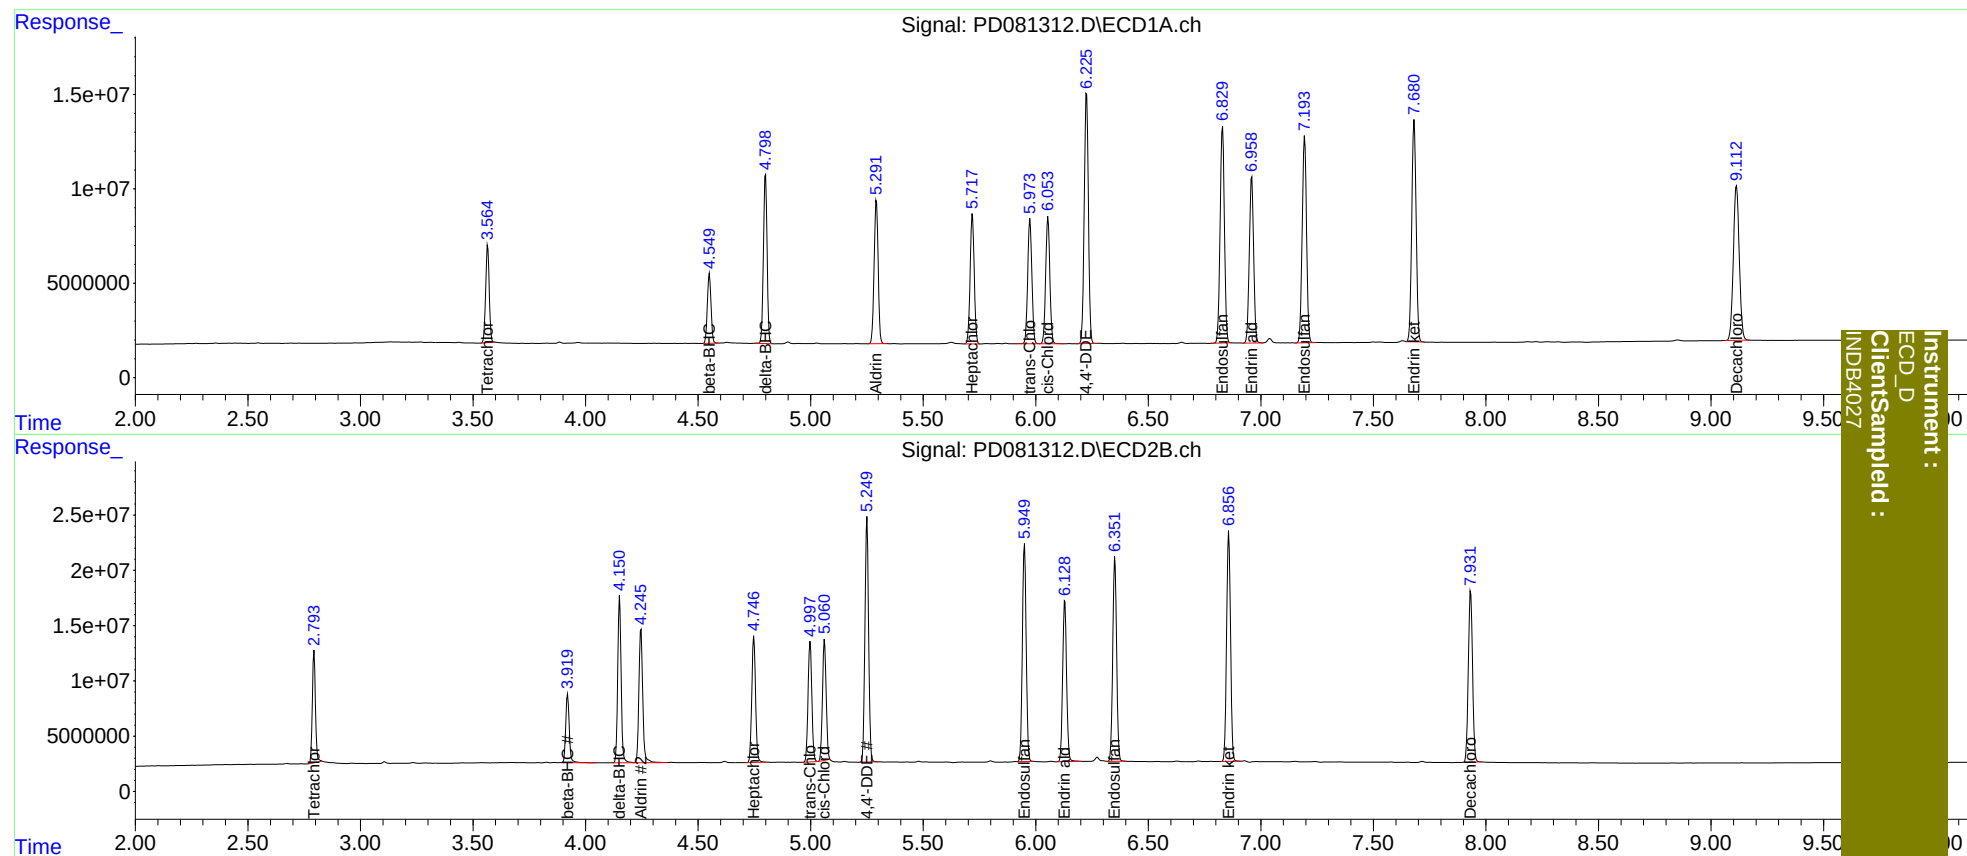


Instrument :
ECD_D
ClientSampled :
INDB4027

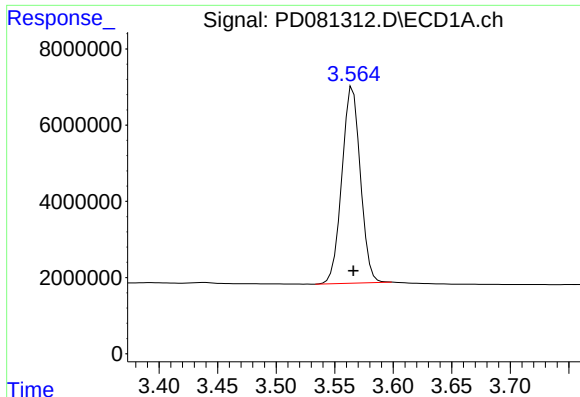

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 56647838
Conc: 41.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

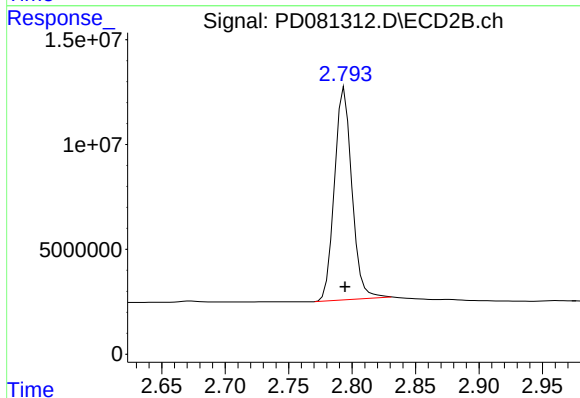


#1 Tetrachloro-m-xylene

R.T.: 2.794 min
Delta R.T.: 0.000 min
Response: 97082096
Conc: 39.12 ng/ml

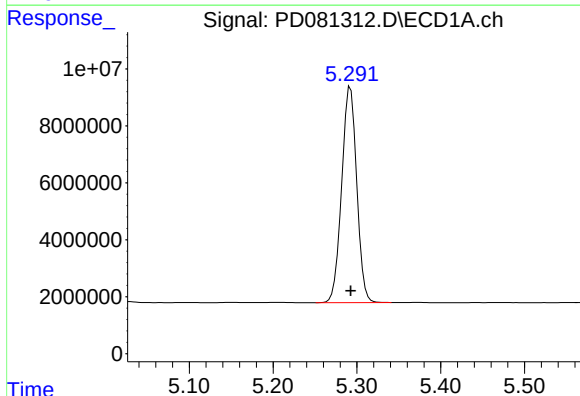


#5 Aldrin

R.T.: 5.292 min
Delta R.T.: 0.000 min
Response: 94595391
Conc: 40.99 ng/ml

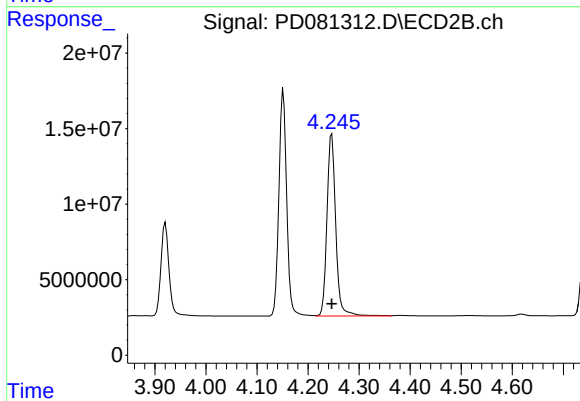

#5 Aldrin


R.T.: 4.246 min
Delta R.T.: 0.000 min
Response: 143512503
Conc: 40.26 ng/ml

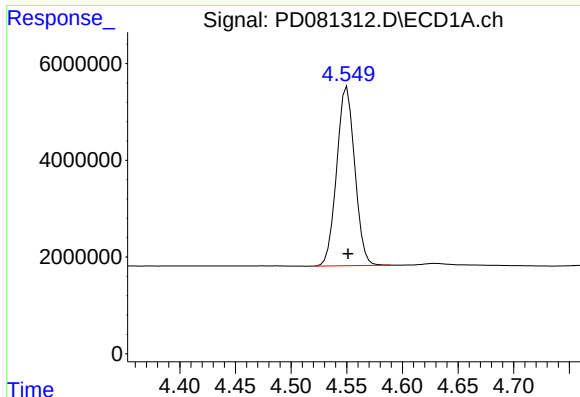

#6 beta-BHC


R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 41831621
Conc: 39.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

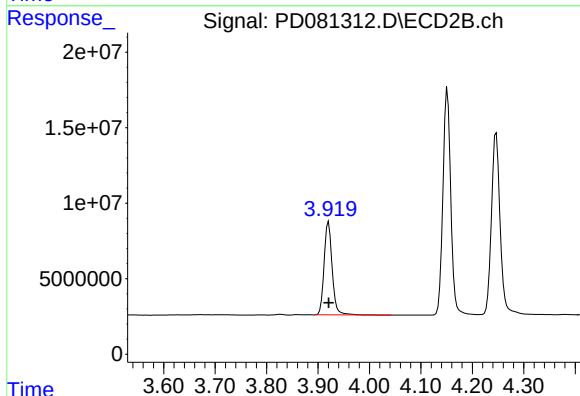


#6 beta-BHC

R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 67024659
Conc: 38.38 ng/ml

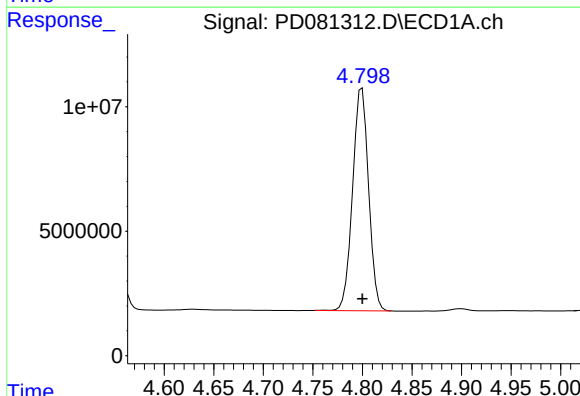


#7 delta-BHC

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 100632588
Conc: 42.13 ng/ml

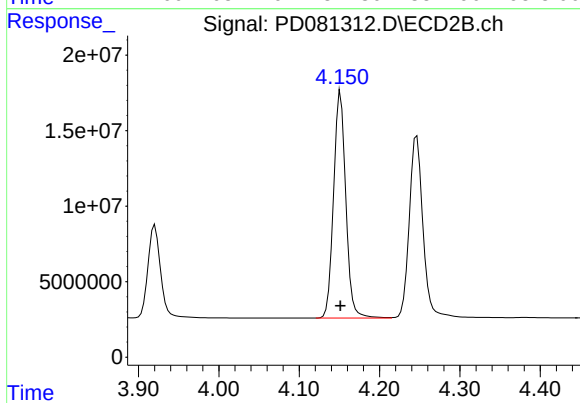

#7 delta-BHC


R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 158965716
Conc: 40.67 ng/ml

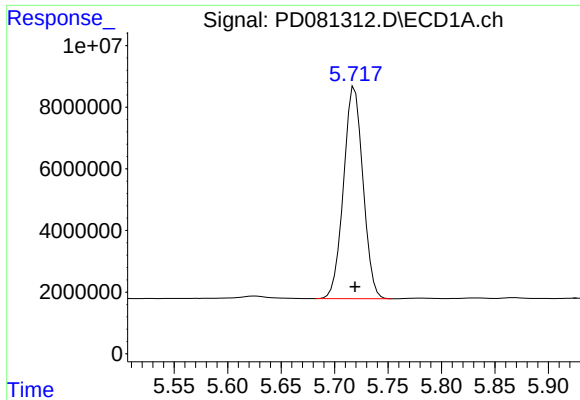

#8 Heptachlor epoxide


R.T.: 5.719 min
Delta R.T.: 0.000 min
Response: 87128256
Conc: 39.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

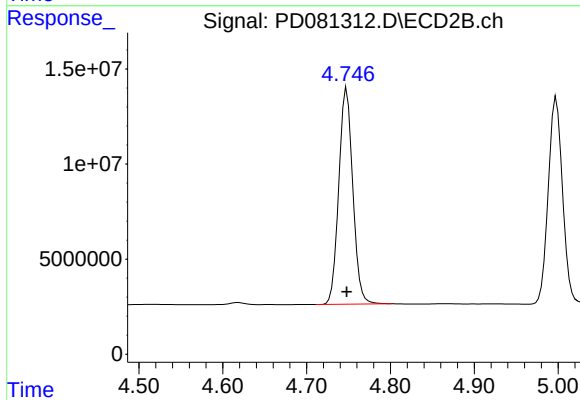


#8 Heptachlor epoxide

R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 132071603
Conc: 39.75 ng/ml

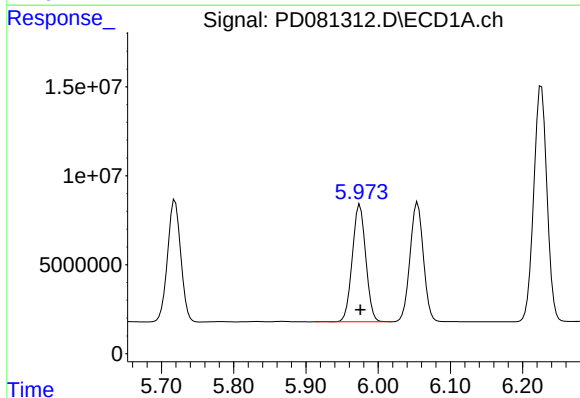


#10 trans-Chlordane

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 84997272
Conc: 40.25 ng/ml

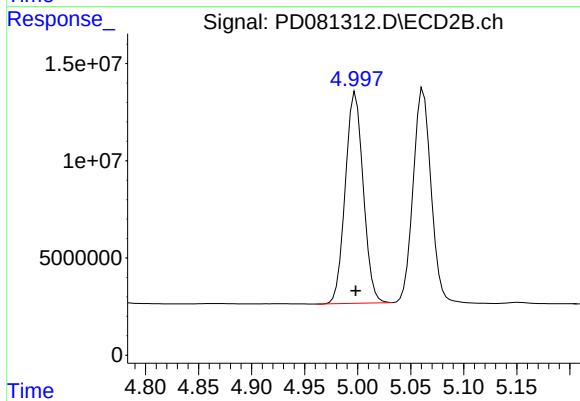

#10 trans-Chlordane


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 127264896
Conc: 39.84 ng/ml

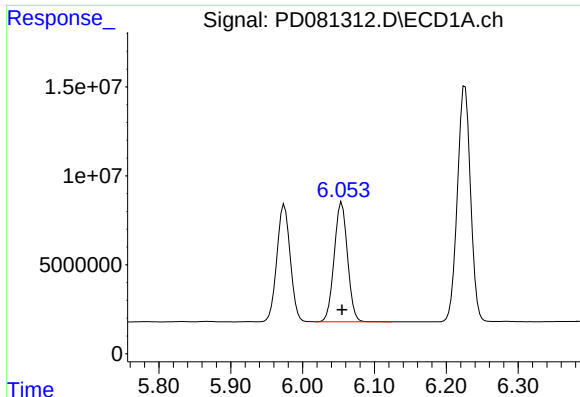

#11 cis-Chlordane


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 86465498
Conc: 39.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

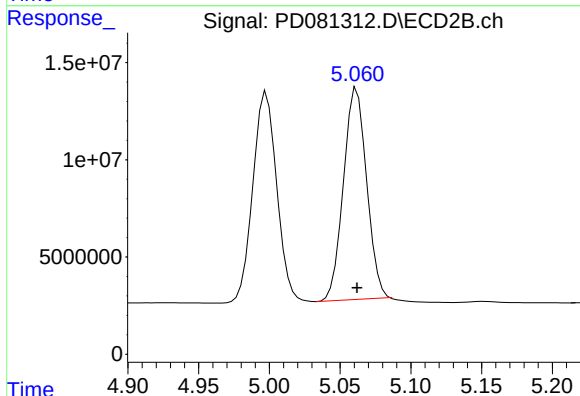


#11 cis-Chlordane

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 124408375
Conc: 39.57 ng/ml

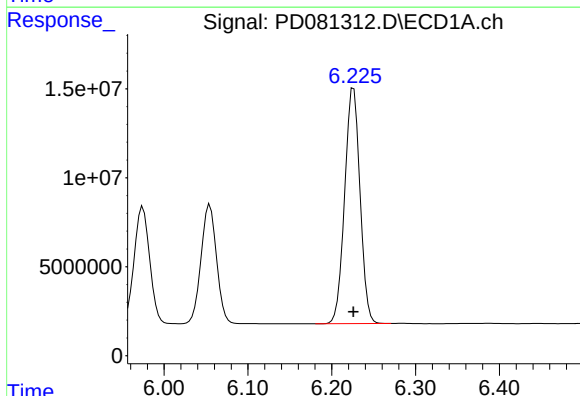


#12 4,4'-DDE

R.T.: 6.226 min
Delta R.T.: 0.000 min
Response: 169049061
Conc: 80.82 ng/ml

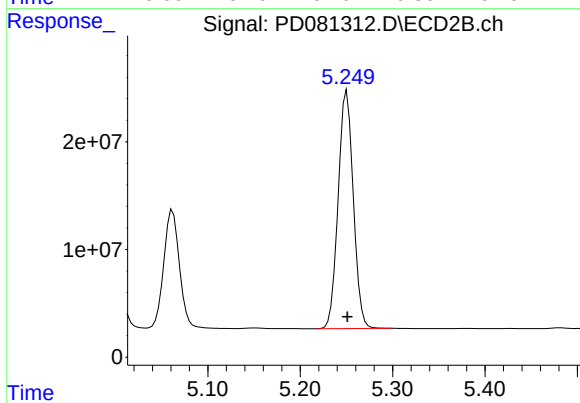

#12 4,4'-DDE


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 251936844
Conc: 81.41 ng/ml

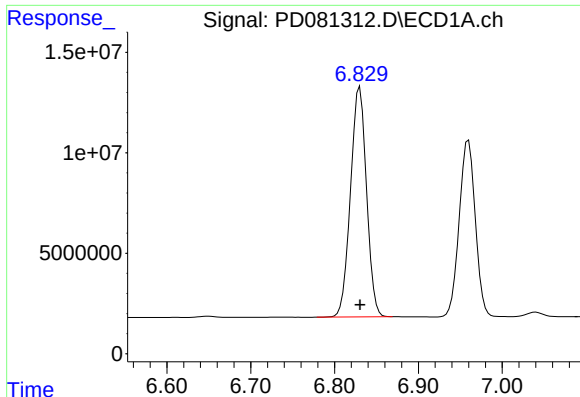

#15 Endosulfan II


R.T.: 6.830 min
Delta R.T.: 0.000 min
Response: 152291607
Conc: 79.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

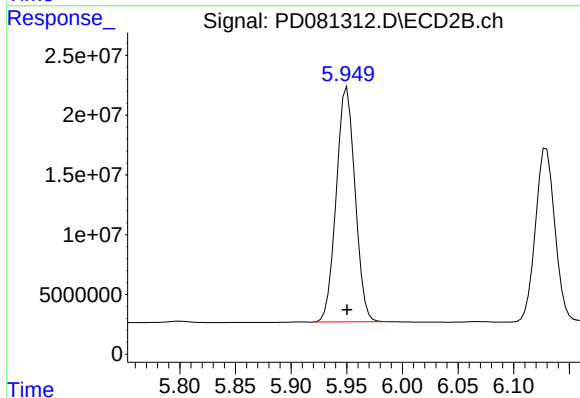


#15 Endosulfan II

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 230722484
Conc: 80.09 ng/ml

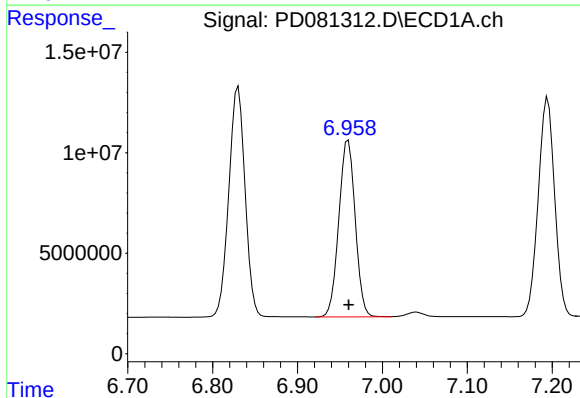


#18 Endrin aldehyde

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 117892613
Conc: 79.06 ng/ml

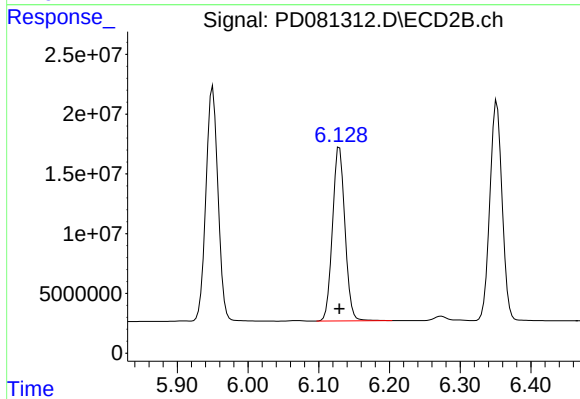

#18 Endrin aldehyde


R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 177855744
Conc: 78.31 ng/ml

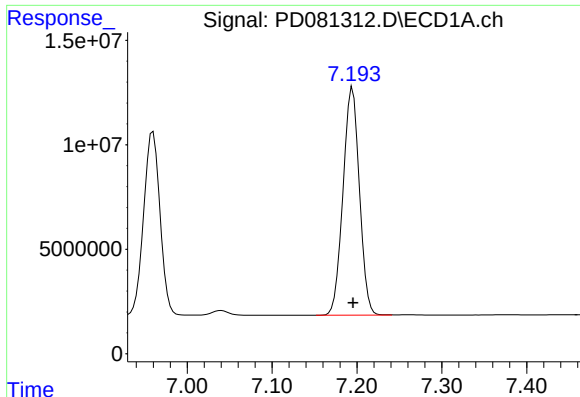

#19 Endosulfan Sulfate


R.T.: 7.195 min
Delta R.T.: 0.000 min
Response: 146118189
Conc: 79.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

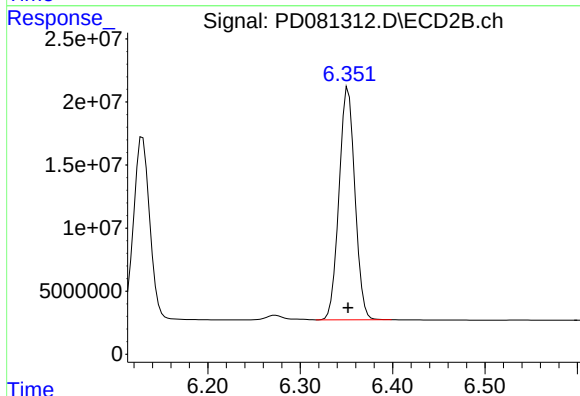


#19 Endosulfan Sulfate

R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 220115564
Conc: 78.81 ng/ml

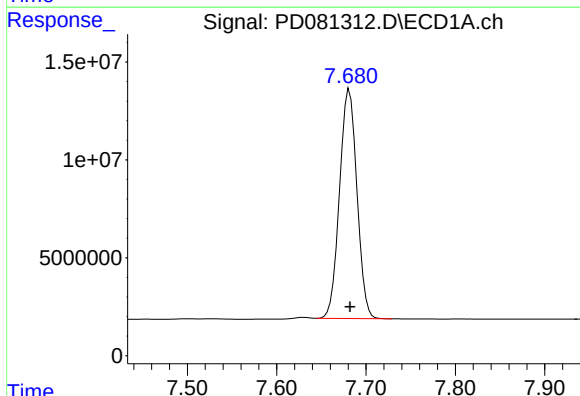


#21 Endrin ketone

R.T.: 7.681 min
Delta R.T.: 0.000 min
Response: 158587542
Conc: 79.89 ng/ml

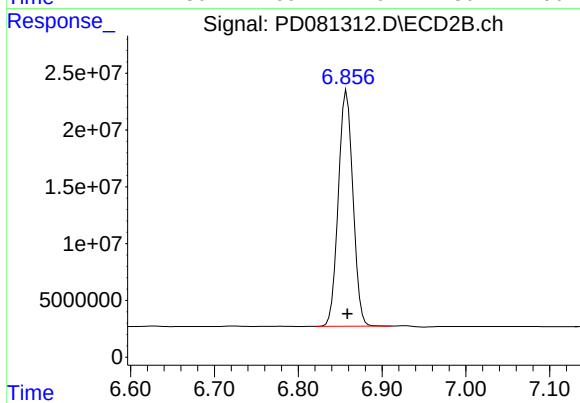

#21 Endrin ketone

R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 251576158
Conc: 79.15 ng/ml

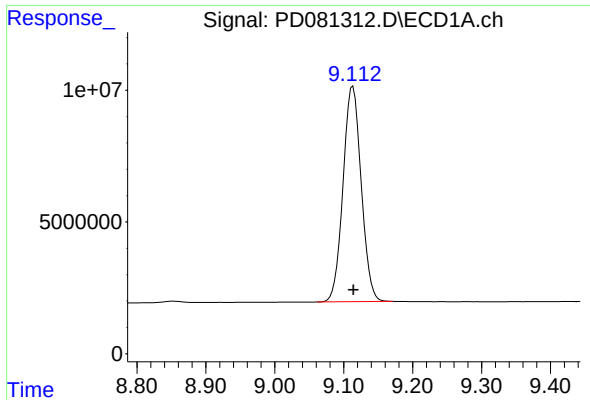

#27 Decachlorobiphenyl


R.T.: 9.113 min

Delta R.T.: 0.000 min

Response: 149754176

Conc: 76.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB4027

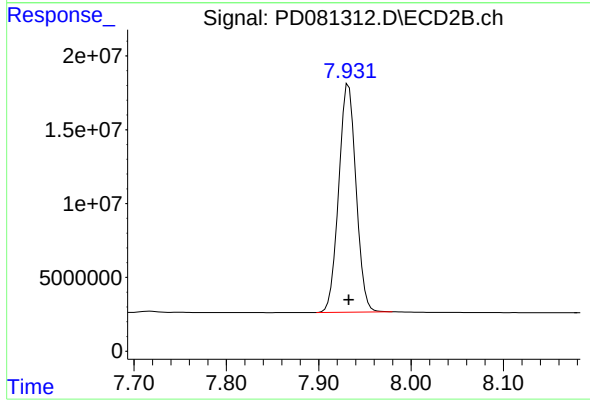

#27 Decachlorobiphenyl

R.T.: 7.932 min

Delta R.T.: 0.000 min

Response: 201602166

Conc: 77.74 ng/ml