

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
 Data File : PD081307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 20:19
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 04:30:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 13 04:30:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	14117828	25262444	10.288	10.055
27)	SA Decachlor...	9.114	7.933	40608295	53140776	20.195	20.071
Target Compounds							
2)	A alpha-BHC	4.022	3.296	22528887	38710349	10.362	10.014
3)	MA gamma-BHC...	4.356	3.626	22606300	36733230	10.314	9.992
4)	MA Heptachlor	4.949	3.966	24893879	35742839	10.213	10.037
9)	A Endosulfan I	6.106	5.118	21921414	31527620	10.122	10.073
13)	MA Dieldrin	6.382	5.383	44768082	67349027	20.162	20.049
14)	MA Endrin	6.612	5.658	36130513	58337448	19.811	20.001
16)	A 4,4'-DDD	6.743	5.804	32643404	52258291	20.022	20.075
17)	MA 4,4'-DDT	7.058	6.056	34153374	52118569	19.851	20.036
20)	A Methoxychlor	7.534	6.630	95905169	143.0E6	99.752	100.605

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
Data File : PD081307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 20:19
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 04:30:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 13 04:30:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

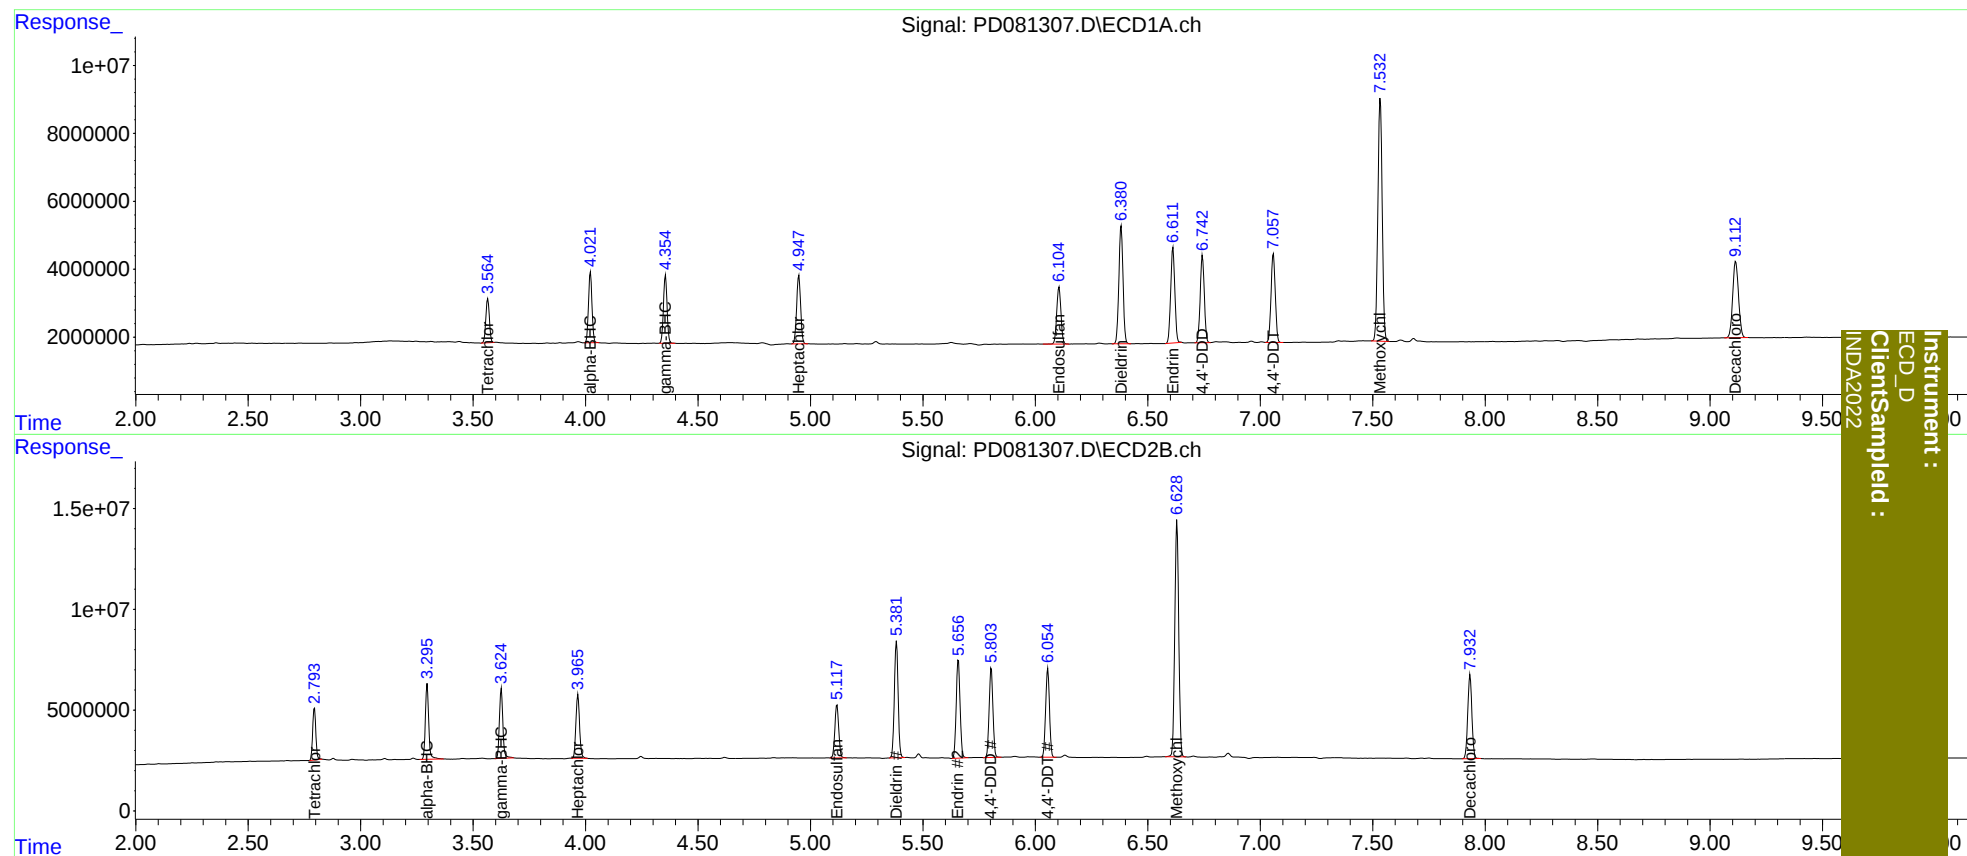

Instrument :
ECD_D
ClientSampled :
INDA2022