

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
 Data File : PD081311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 21:12
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4026

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 04:33:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 13 04:33:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	54603572	97546360	39.843	39.112
27)	SA Decachlor...	9.115	7.933	150.4E6	201.0E6	76.024	76.892
Target Compounds							
2)	A alpha-BHC	4.022	3.296	96919356	163.0E6	43.337	41.596
3)	MA gamma-BHC...	4.356	3.625	94977501	150.3E6	42.448	40.663
4)	MA Heptachlor	4.949	3.966	98957906	143.6E6	40.447	40.235
9)	A Endosulfan I	6.106	5.118	83843601	123.1E6	39.027	39.496
13)	MA Dieldrin	6.382	5.382	182.5E6	277.6E6	81.625	81.955
14)	MA Endrin	6.612	5.658	147.3E6	237.1E6	80.578	80.977
16)	A 4,4'-DDD	6.744	5.804	133.9E6	213.5E6	81.605	81.488
17)	MA 4,4'-DDT	7.059	6.056	140.8E6	221.1E6	81.376	83.700
20)	A Methoxychlor	7.534	6.630	358.6E6	535.8E6	379.377	382.454

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
Data File : PD081311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 21:12
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 04:33:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 13 04:33:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

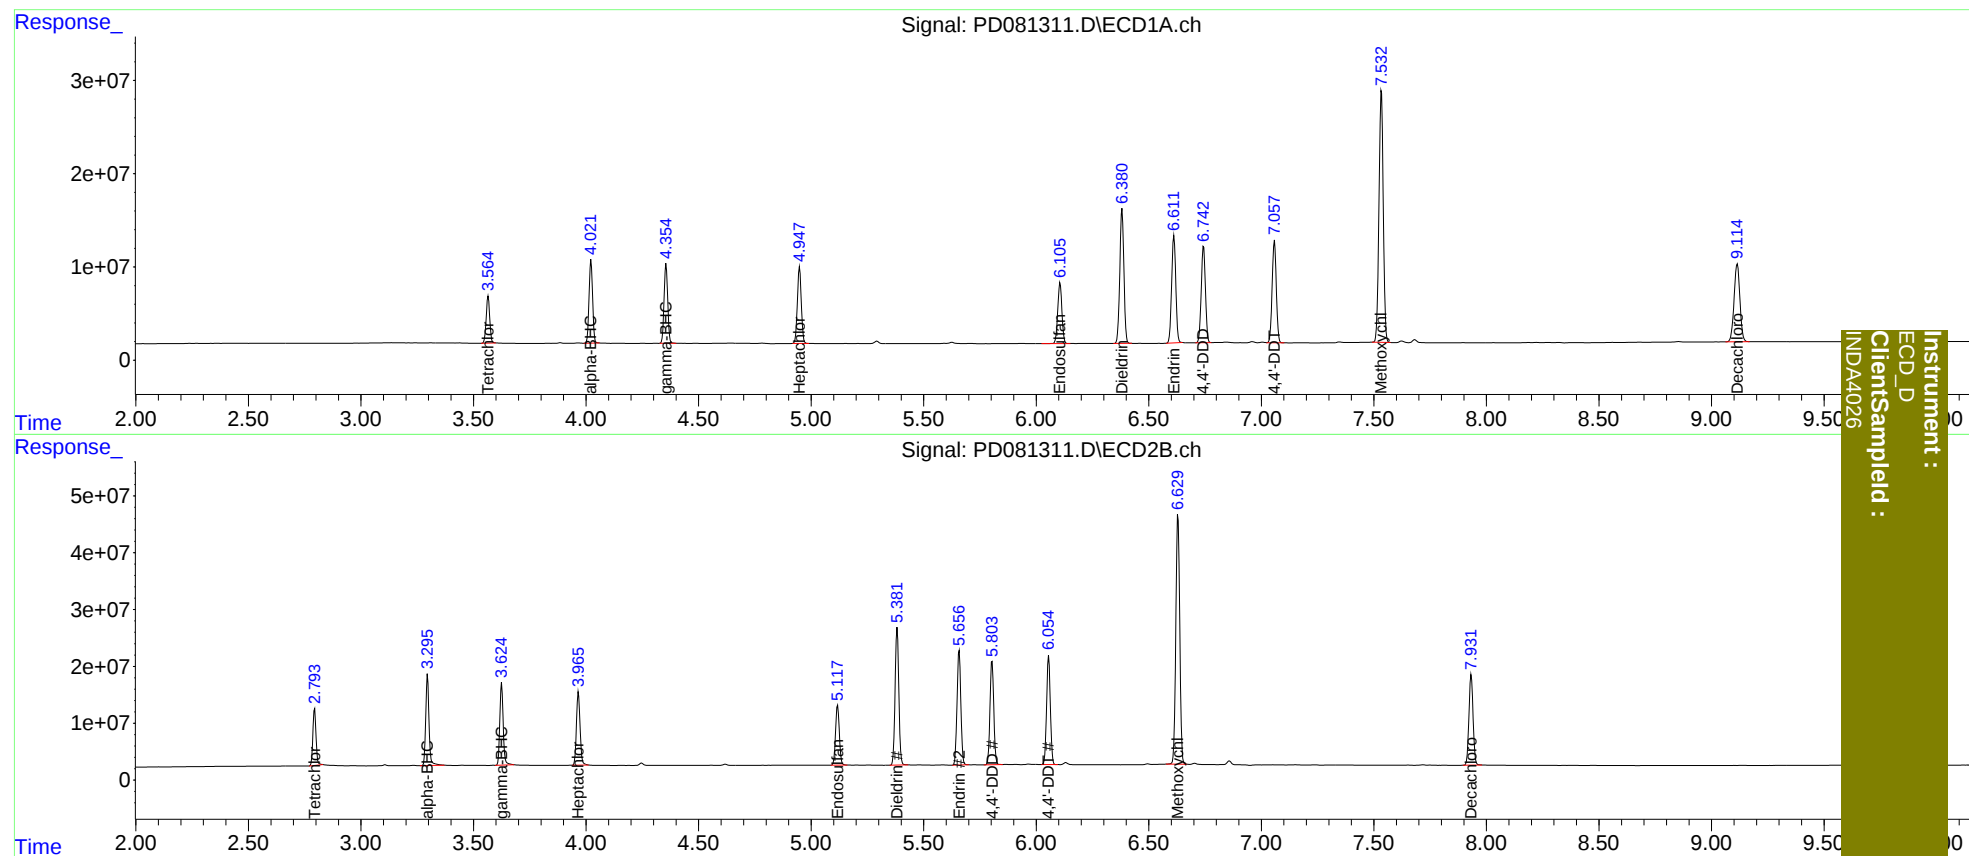

Instrument :
ECD_D
ClientSampled :
INDA4026