

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
 Data File : PD081313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 21:39
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 04:36:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 13 04:36:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	103.5E6	195.5E6	76.391	78.702
27)	SA Decachlor...	9.115	7.933	296.0E6	403.4E6	151.590	155.431
Target Compounds							
2)	A alpha-BHC	4.022	3.296	203.4E6	339.7E6	88.536	85.282
3)	MA gamma-BHC...	4.356	3.626	200.6E6	312.3E6	87.541	83.537
4)	MA Heptachlor	4.949	3.967	214.5E6	294.5E6	86.018	82.016
9)	A Endosulfan I	6.106	5.119	194.6E6	250.4E6	88.260	80.268
13)	MA Dieldrin	6.382	5.383	398.3E6	569.5E6	174.200	166.457
14)	MA Endrin	6.612	5.658	314.1E6	485.9E6	169.310	164.695
16)	A 4,4'-DDD	6.744	5.805	289.1E6	437.7E6	172.657	165.627
17)	MA 4,4'-DDT	7.058	6.056	318.4E6	458.7E6	178.632	170.713
20)	A Methoxychlor	7.533	6.630	781.9E6	1026.8E6	821.659	745.409

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021324\
Data File : PD081313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 21:39
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 04:36:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 13 04:36:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

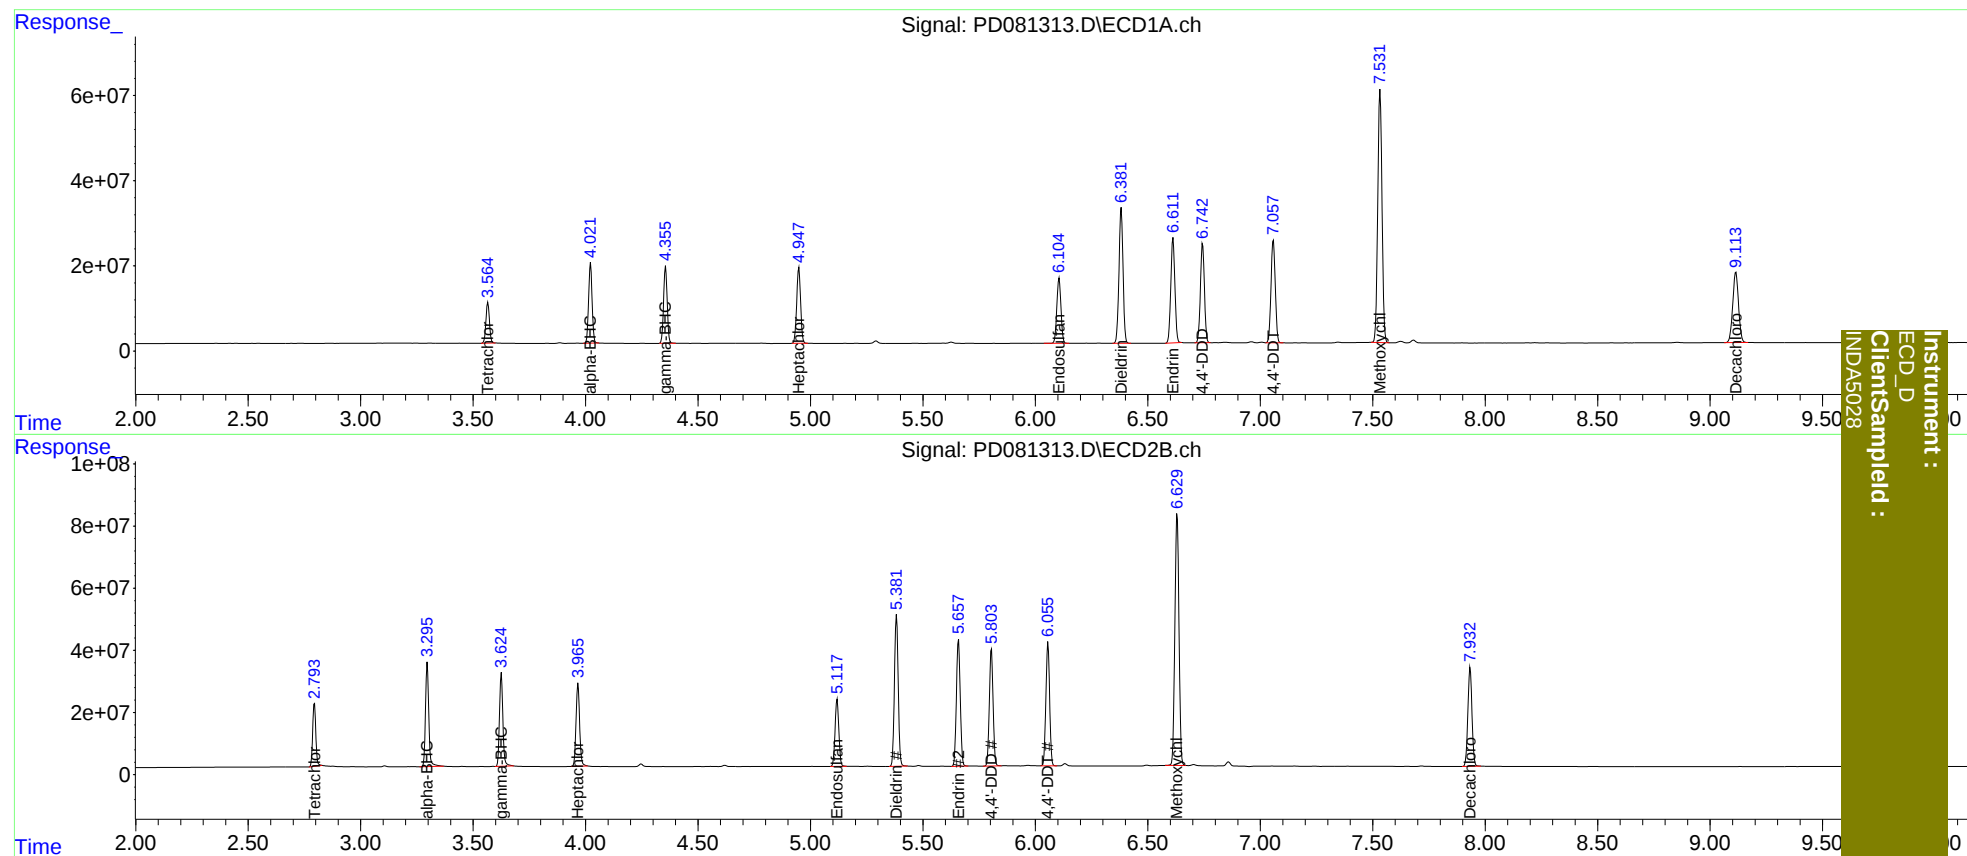

Instrument :
ECD_D
ClientSampled :
INDA5028