

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021419\
 Data File : PD051288.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Feb 2019 8:59
 Operator : AJ\SJ
 Sample : PIBLK43
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK43

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 03:01:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 03:30:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.224	4.045	28001340	590.3E6	20.066	20.702
27) SA Decachlor...	7.825	9.157	46191207	696.8E6	37.808	37.462
Target Compounds						
6) B beta-BHC	0.000	4.936f	0 51583512	N.D.	2.795	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021419\
Data File : PD051288.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Feb 2019 8:59
Operator : AJ\SJ
Sample : PIBLK43
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK43

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 03:01:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 25 03:30:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

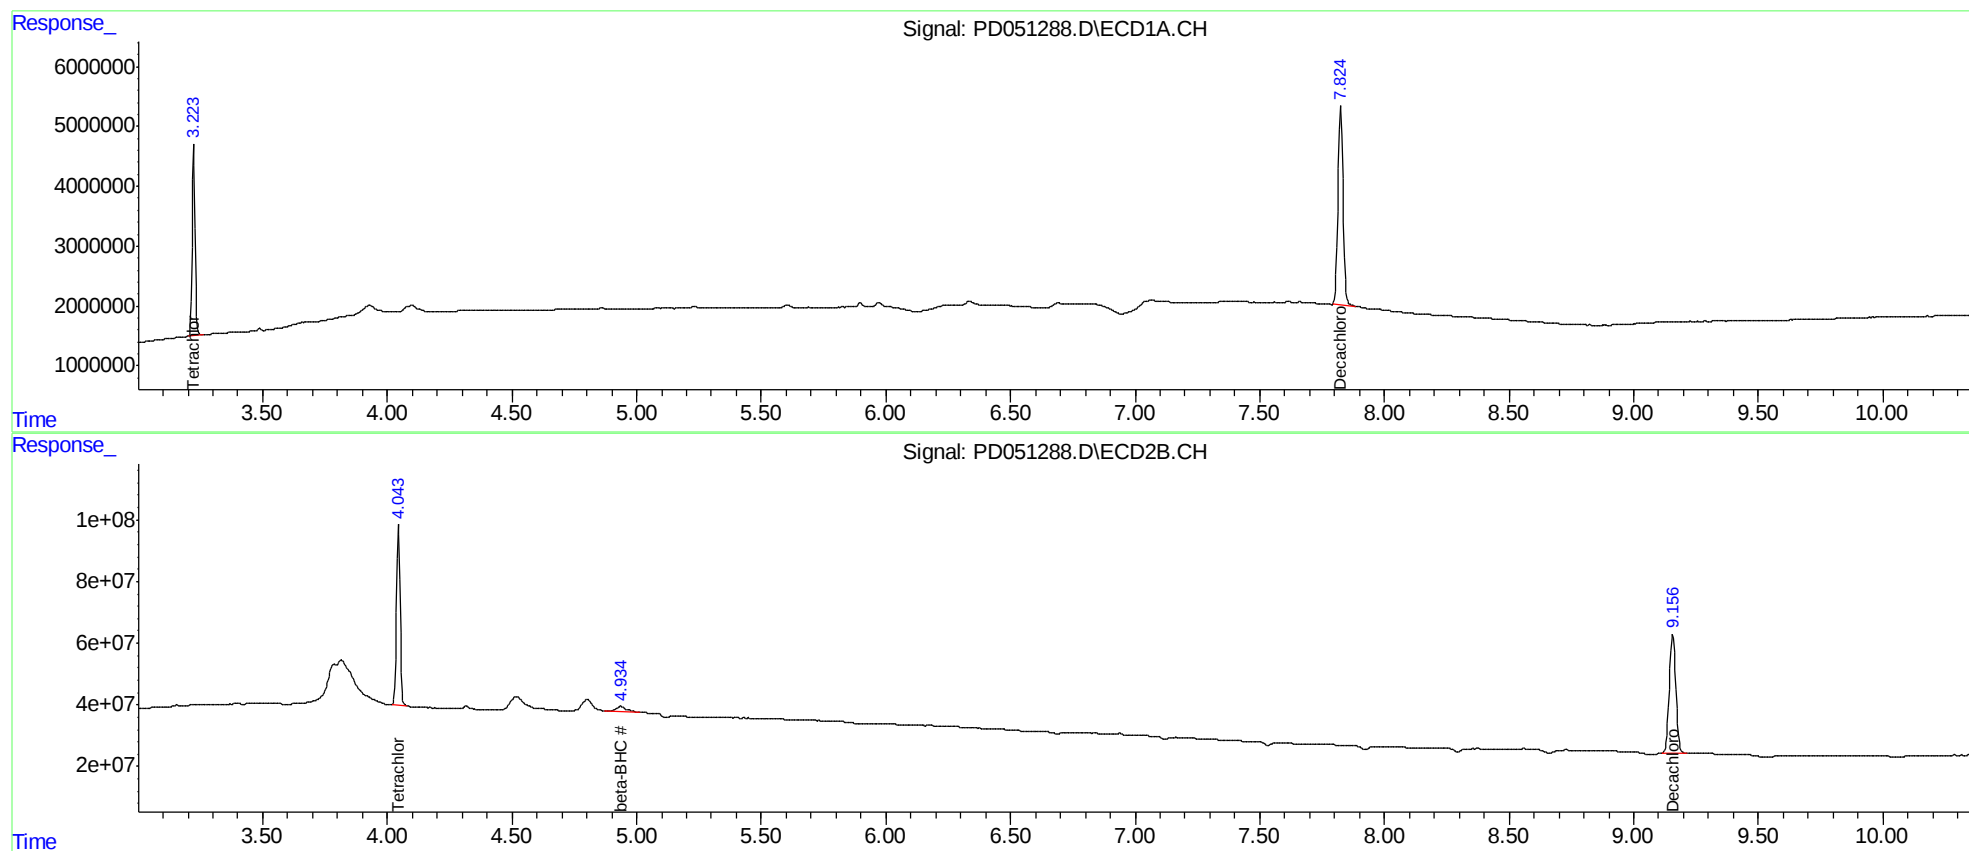


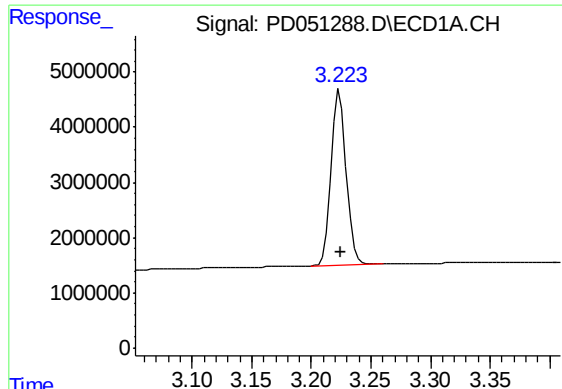

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 28001340
Conc: 20.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK43

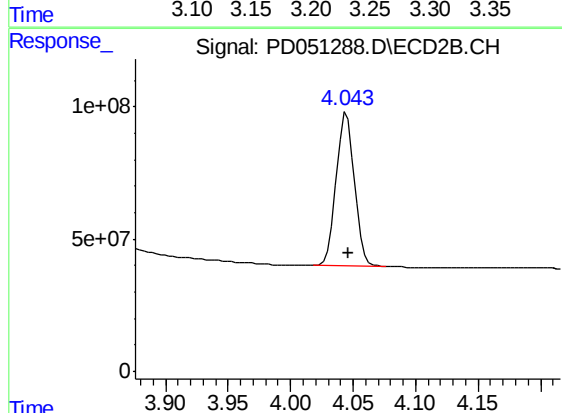


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 590256355
Conc: 20.70 ng/ml

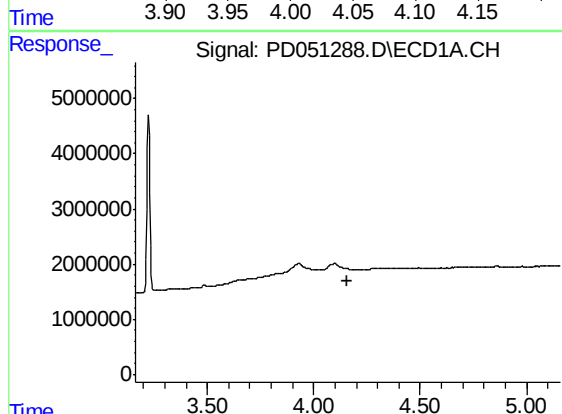


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.160 min
Response: 0
Conc: N.D.

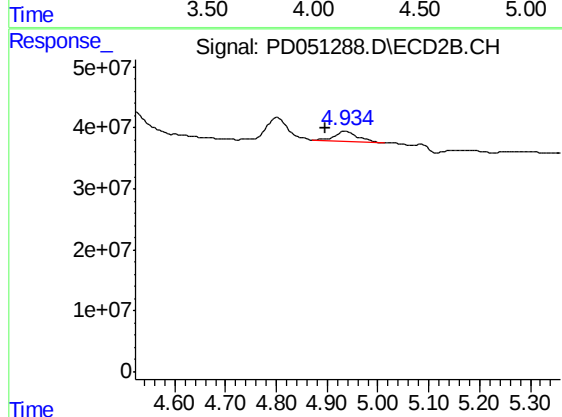

#6 beta-BHC


R.T.: 4.936 min
Delta R.T.: 0.040 min
Response: 51583512
Conc: 2.79 ng/ml

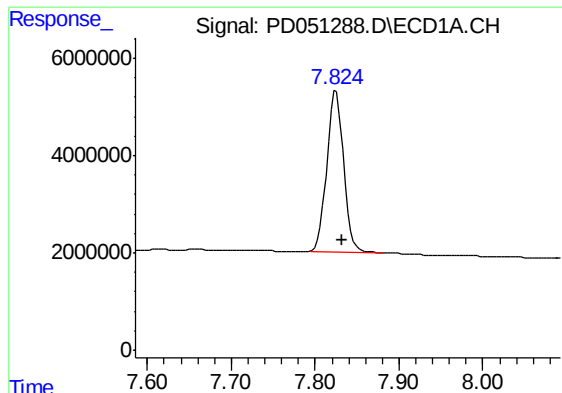

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.006 min
Response: 46191207
Conc: 37.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK43

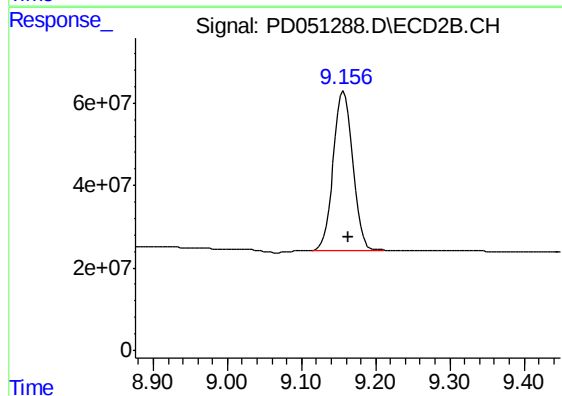

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: -0.007 min
Response: 696761807
Conc: 37.46 ng/ml