

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021420\
 Data File : PD057271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2020 09:03
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 01:17:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.815	0	21396349	N.D.	8.679
15) B	Endosulfa...	0.000	6.868	0	4890580	N.D.	2.088
16) A	4,4'-DDD	0.000	6.824f	0	59166213	N.D.	28.696


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021420\
Data File : PD057271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2020 09:03
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 01:17:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

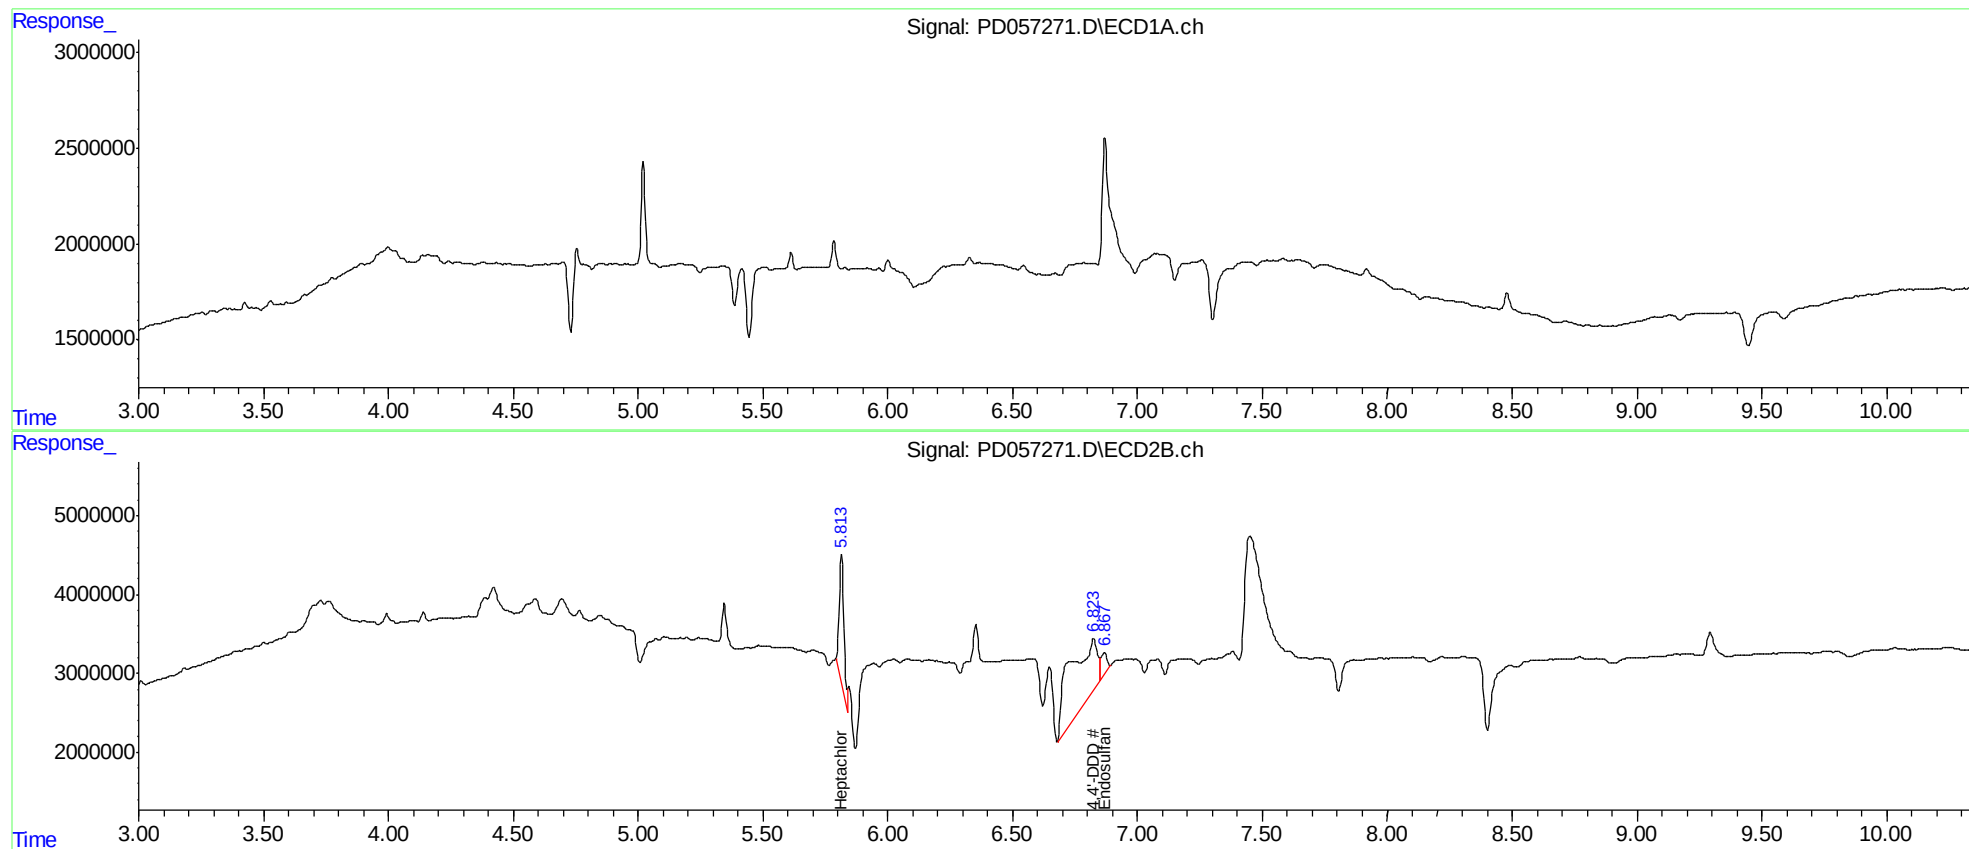


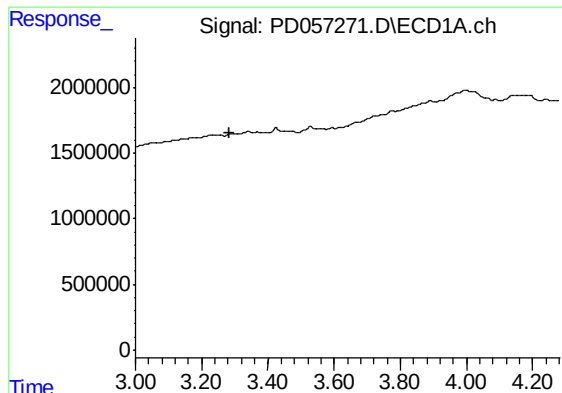

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

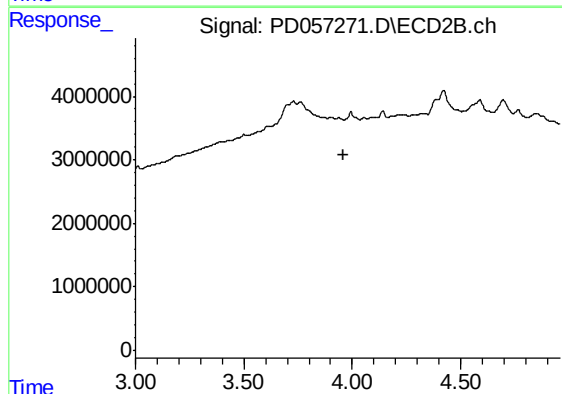


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.961 min
Response: 0
Conc: N.D.

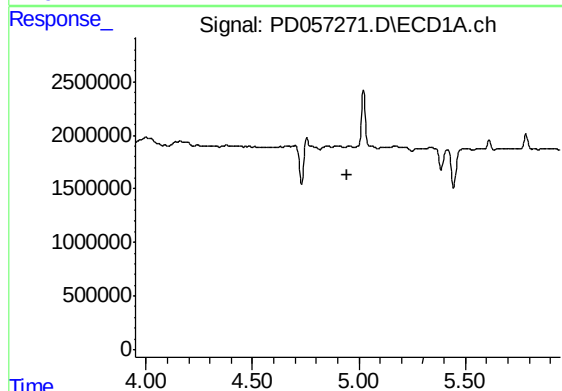


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.948 min
Response: 0
Conc: N.D.

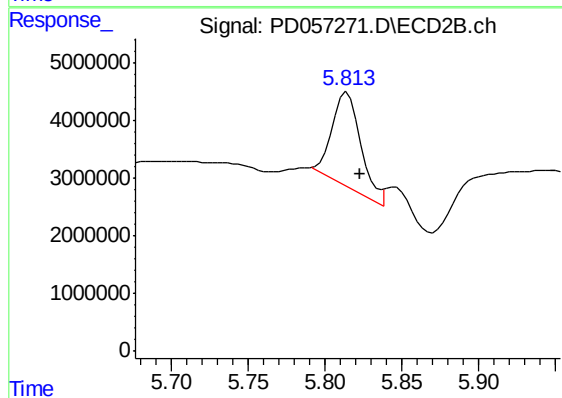

#8 Heptachlor epoxide


R.T.: 5.815 min
Delta R.T.: -0.009 min
Response: 21396349
Conc: 8.68 ng/ml

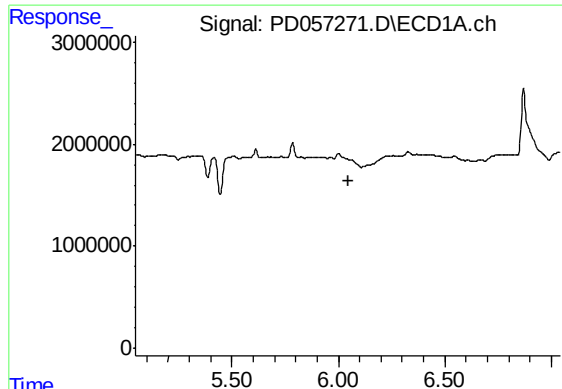

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

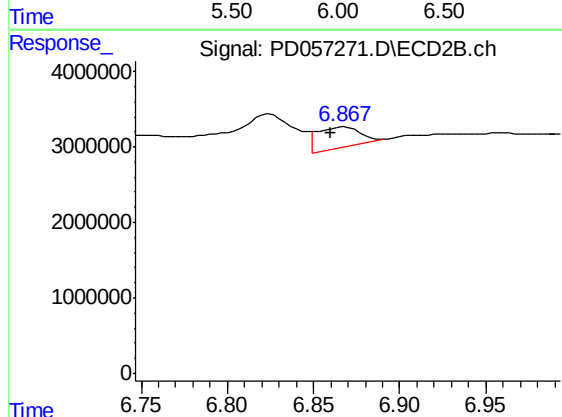


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.009 min
Response: 4890580
Conc: 2.09 ng/ml

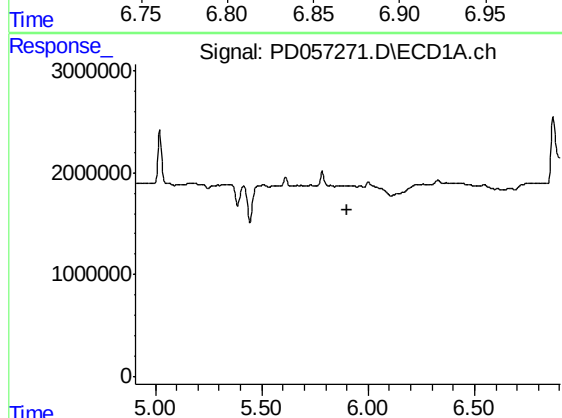


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.904 min
Response: 0
Conc: N.D.

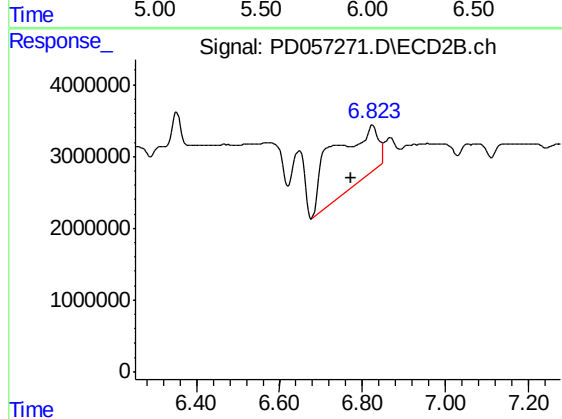

#16 4,4'-DDD


R.T.: 6.824 min
Delta R.T.: 0.051 min
Response: 59166213
Conc: 28.70 ng/ml

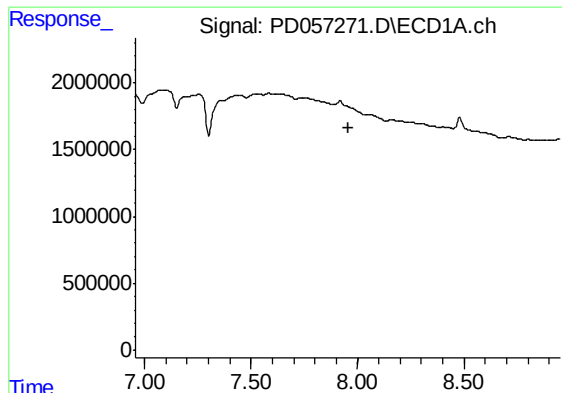

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

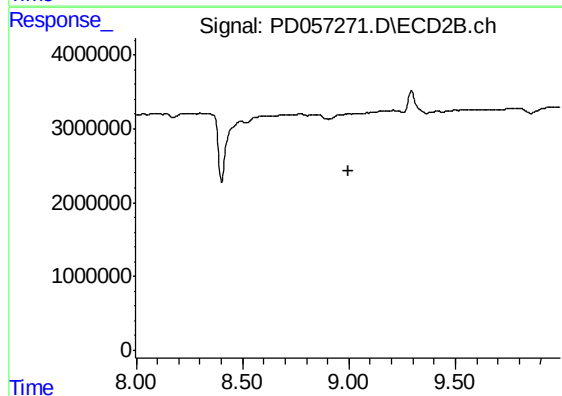

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.996 min
Response: 0
Conc: N.D.