

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021420\
 Data File : PD057304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2020 19:39
 Operator : AJ\MA
 Sample : L1423-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AY0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 01:27:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.283	3.959	12465185	31349879	15.006	16.823
27) SA Decachlor...	7.952	8.992	16893373	28723664	16.284	12.706
Target Compounds						
10) B trans-Chl...	0.000	6.041	0	9950095	N.D.	3.639


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021420\
Data File : PD057304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2020 19:39
Operator : AJ\MA
Sample : L1423-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C5AY0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 01:27:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

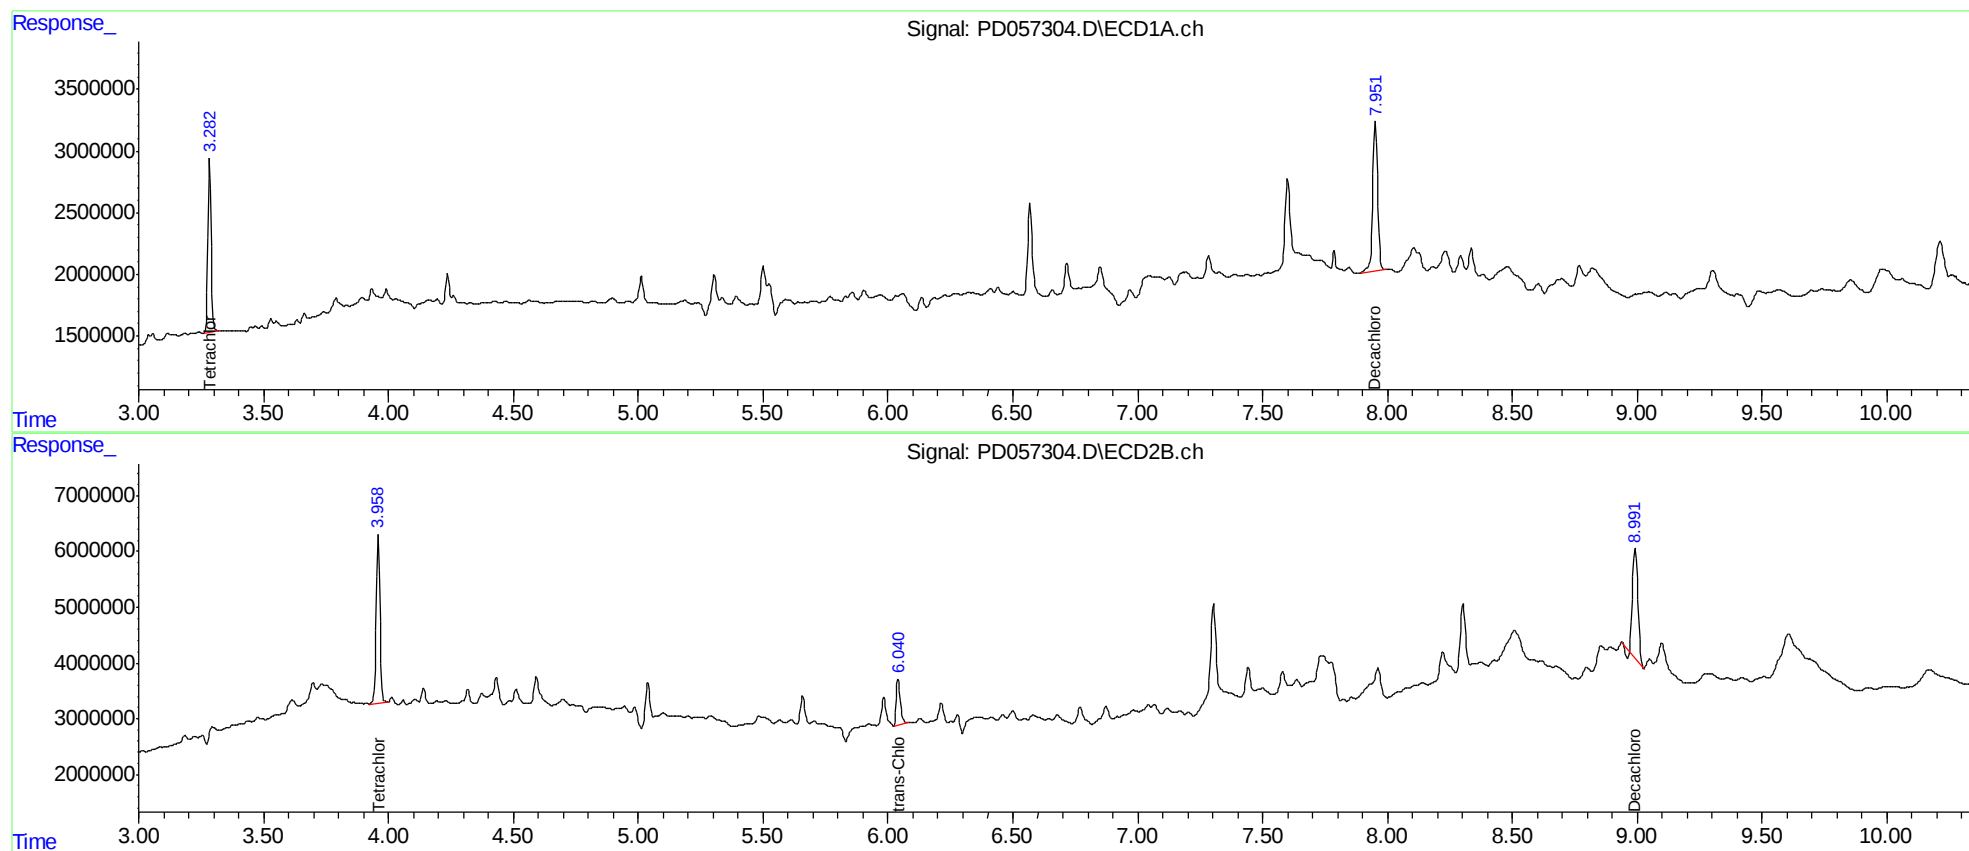


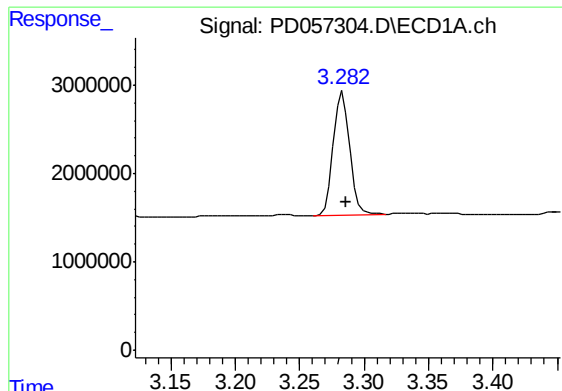

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: -0.003 min
Response: 12465185
Conc: 15.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AY0

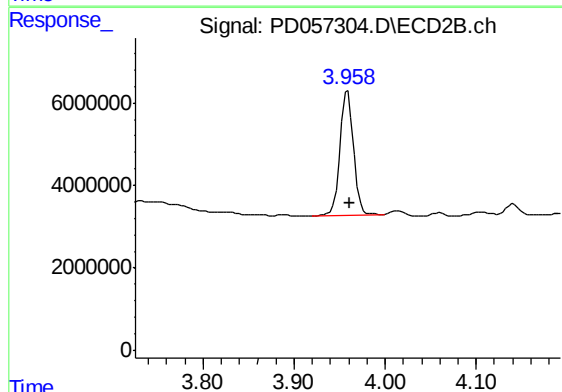


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 31349879
Conc: 16.82 ng/ml

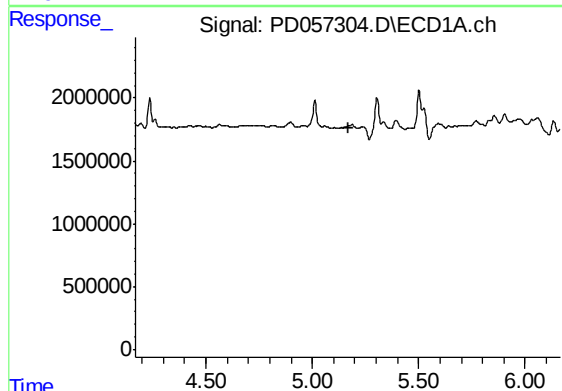


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

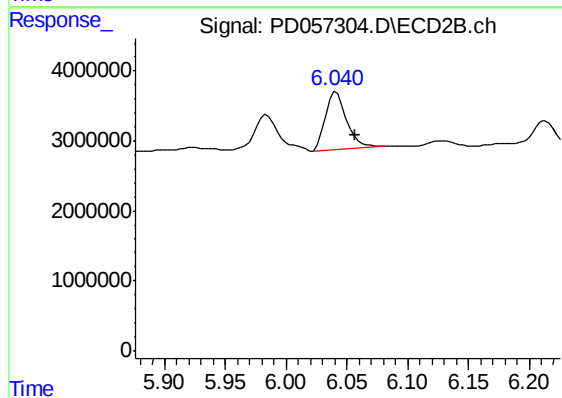

#10 trans-Chlordane


R.T.: 6.041 min
Delta R.T.: -0.015 min
Response: 9950095
Conc: 3.64 ng/ml

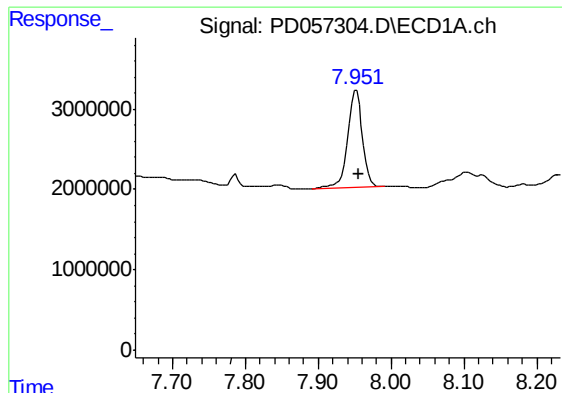

#27 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: -0.004 min
Response: 16893373
Conc: 16.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AY0

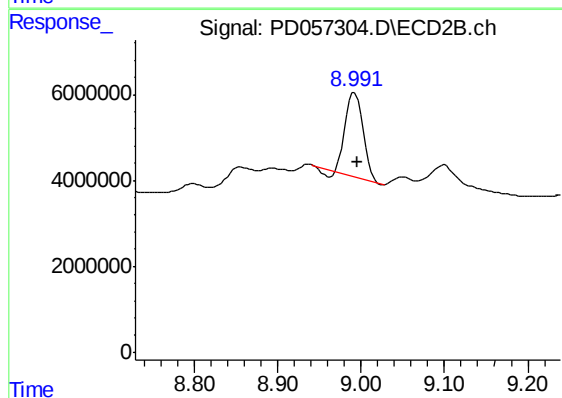

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: -0.004 min
Response: 28723664
Conc: 12.71 ng/ml