

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021420\
 Data File : PD057316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2020 22:28
 Operator : AJ\MA
 Sample : L1423-13
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AZ7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 01:29:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.284	3.959	11838390	30236424	14.251	16.226
27) SA Decachlor...	7.952	8.992	21142121	44656500	20.379	19.754
Target Compounds						
7) B delta-BHC	4.435	0.000	13620771	0	10.927	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021420\
Data File : PD057316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2020 22:28
Operator : AJ\MA
Sample : L1423-13
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C5AZ7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 01:29:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

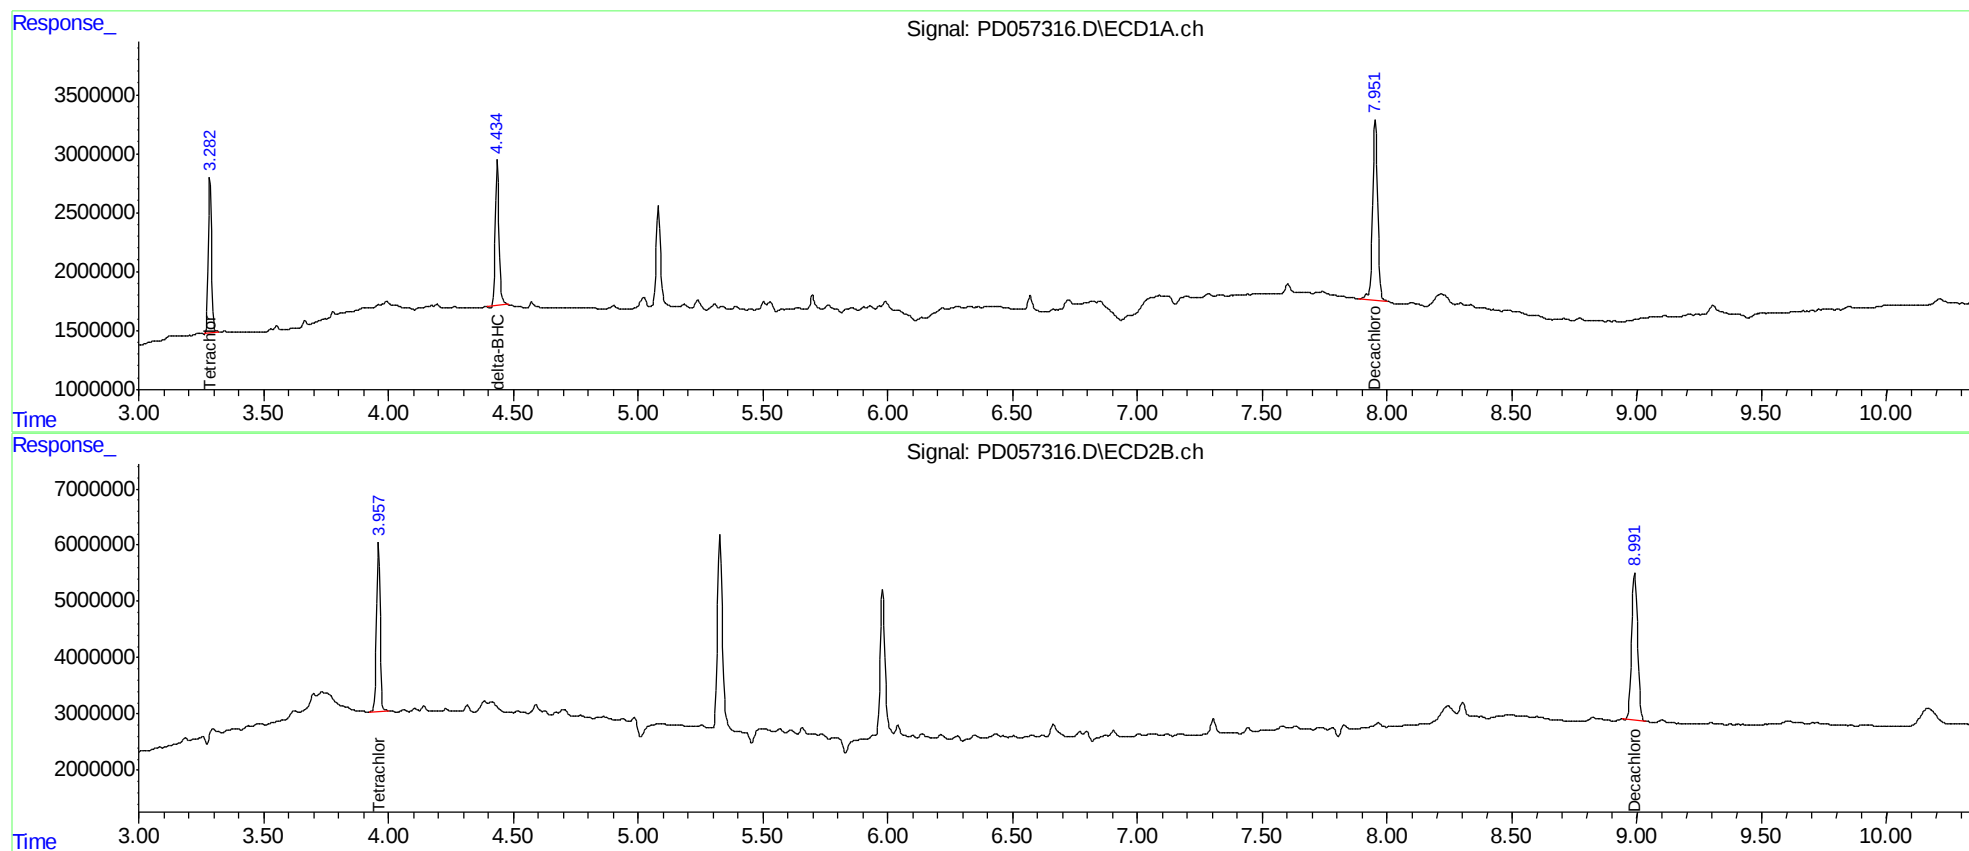


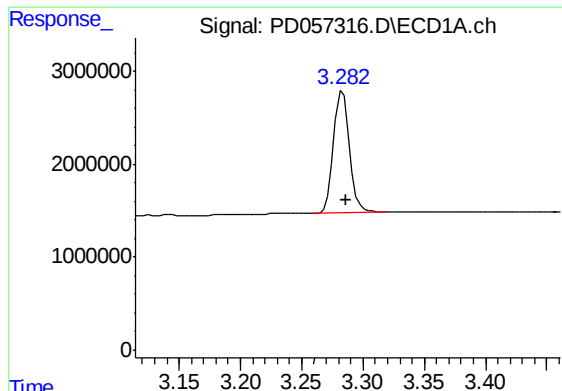

#1 Tetrachloro-m-xylene


R.T.: 3.284 min
Delta R.T.: -0.002 min
Response: 11838390
Conc: 14.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AZ7

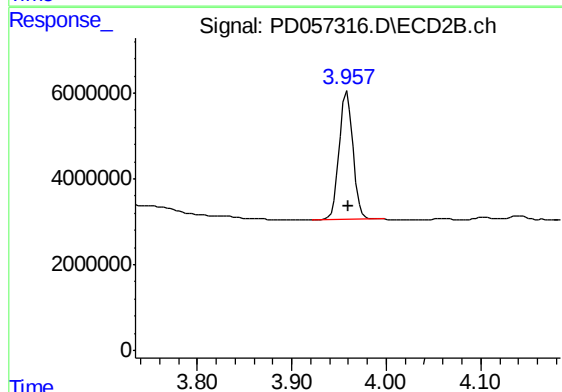


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 30236424
Conc: 16.23 ng/ml

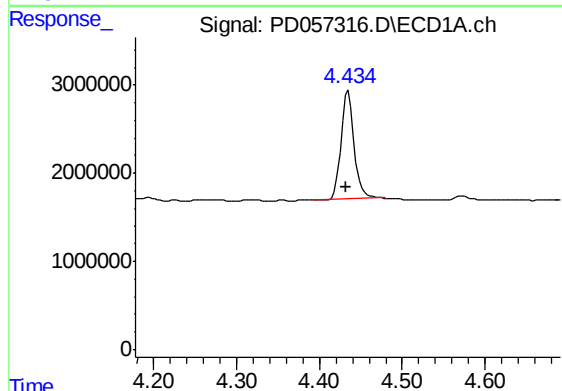


#7 delta-BHC

R.T.: 4.435 min
Delta R.T.: 0.003 min
Response: 13620771
Conc: 10.93 ng/ml

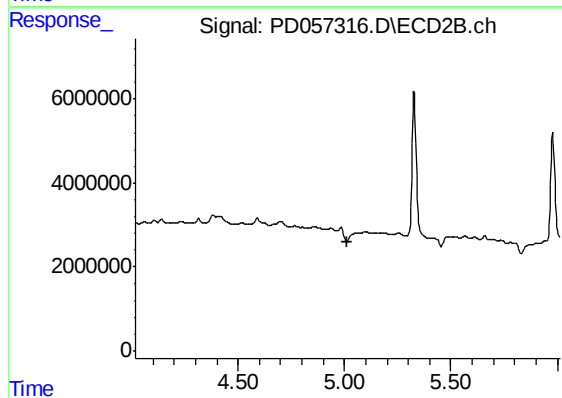

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.015 min
Response: 0
Conc: N.D.

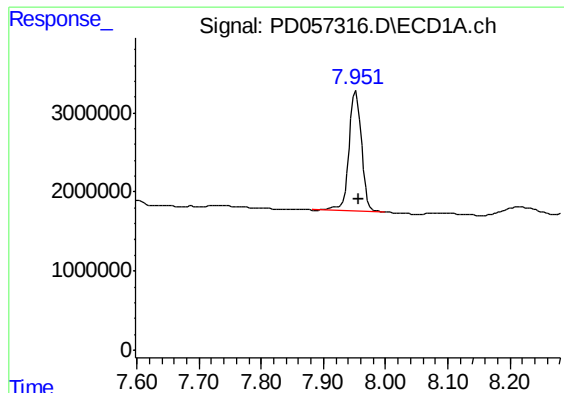

#27 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: -0.004 min
Response: 21142121
Conc: 20.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AZ7

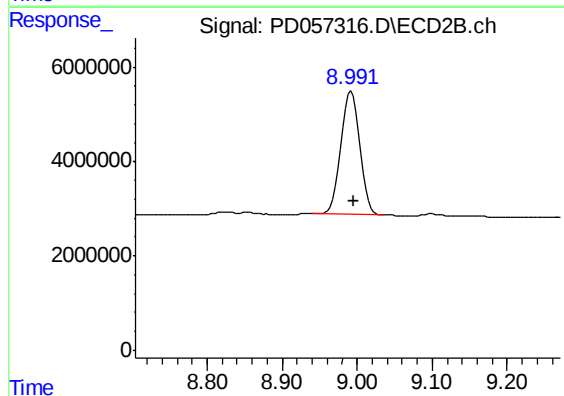

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: -0.004 min
Response: 44656500
Conc: 19.75 ng/ml