

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021521\
 Data File : PD061236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 09:22
 Operator : DD\AJ
 Sample : PIBLK15
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:47:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	28077575	181.5E6	27.663	25.362
27)	SA Decachlor...	8.274	9.103	53036497	286.7E6	42.091	42.223
Target Compounds							
3)	MA gamma-BHC...	0.000	4.694	0	403110	N.D.	<MDL
6)	B beta-BHC	4.434f	4.875	698152	108336	1.120	<MDL #
7)	B delta-BHC	0.000	5.058f	0	3774189	N.D.	0.370
8)	B Heptachlo...	5.159f	5.841f	153282	12609507	0.113	1.455 #
9)	A Endosulfan I	0.000	6.250	0	122248	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.231	0	246260	N.D.	<MDL
14)	MA Endrin	6.011f	6.684f	363700	3690558	0.293	0.500 #
17)	MA 4,4'-DDT	0.000	7.111f	0	4955700	N.D.	0.682
18)	B Endrin al...	0.000	7.111f	0	4955700	N.D.	0.836
19)	B Endosulfa...	6.761f	0.000	268640	0	0.257	N.D. #
20)	A Methoxychlor	7.038f	7.547f	1907741	-138723	3.056	N.D. #
23)	Toxaphene-2	0.000	6.684	0	3690558	N.D.	56.117
24)	Toxaphene-3	0.000	7.111	0	4955700	N.D.	51.728


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021521\
Data File : PD061236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2021 09:22
Operator : DD\AJ
Sample : PIBLK15
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 04:47:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

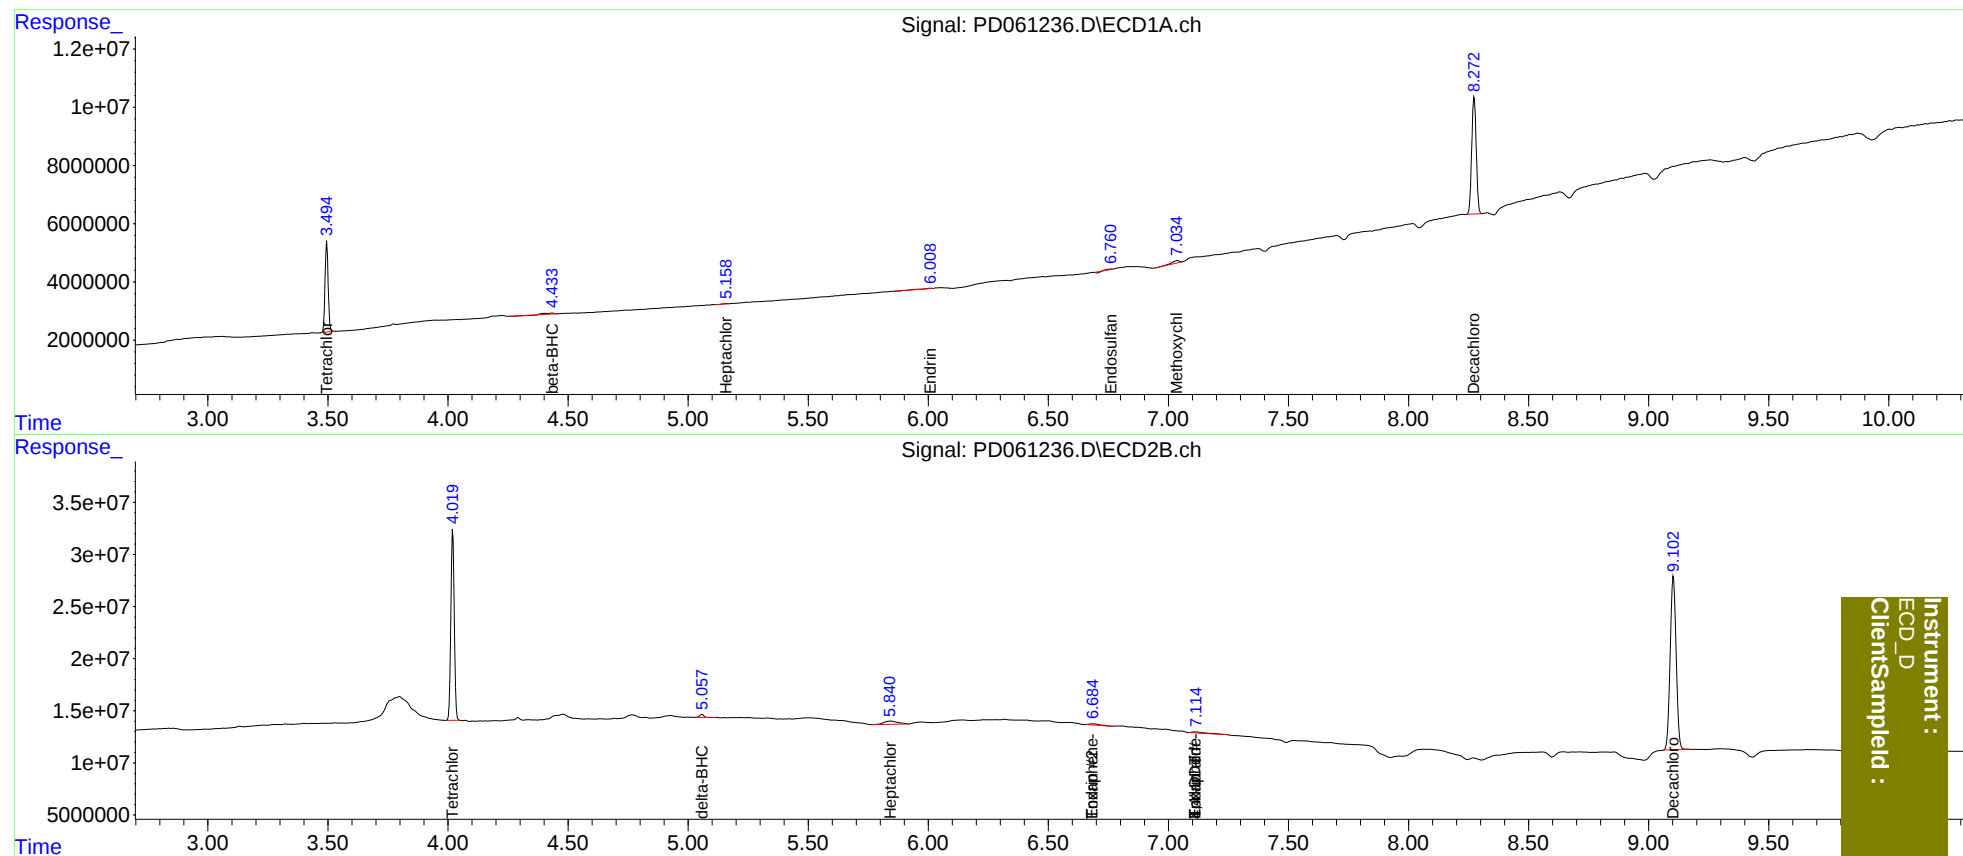


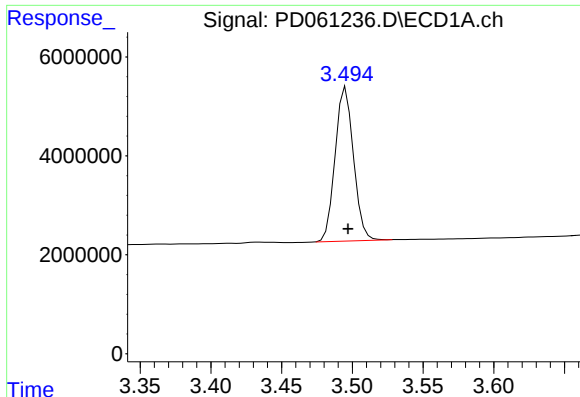

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: -0.001 min
Response: 28077575
Conc: 27.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

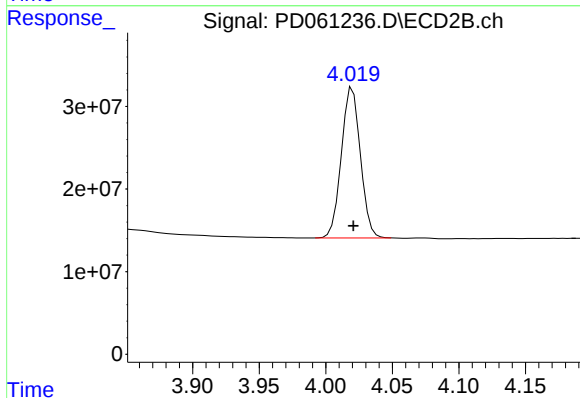


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 181488538
Conc: 25.36 ng/ml

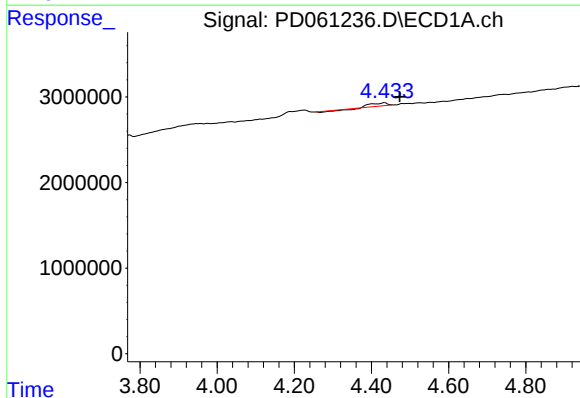


#6 beta-BHC

R.T.: 4.434 min
Delta R.T.: -0.039 min
Response: 698152
Conc: 1.12 ng/ml

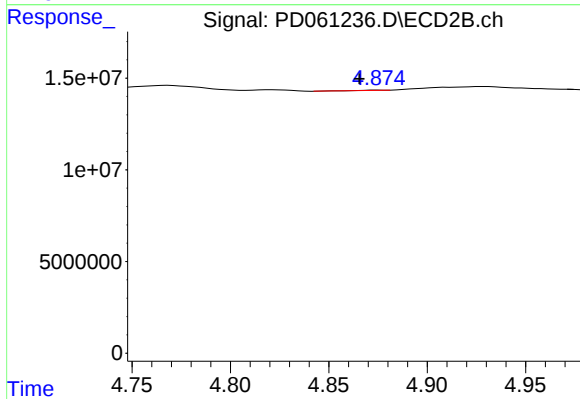

#6 beta-BHC


R.T.: 4.875 min
Delta R.T.: 0.010 min
Response: 108336
Conc: N.D.

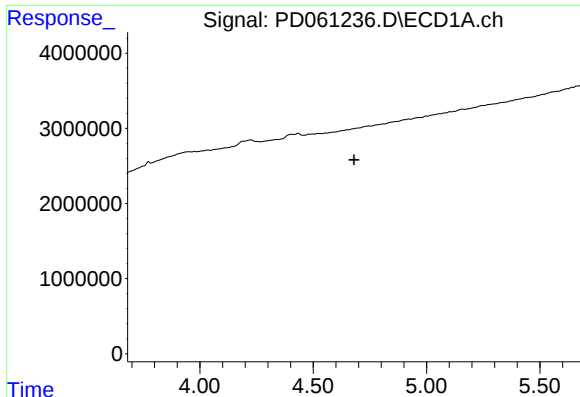

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

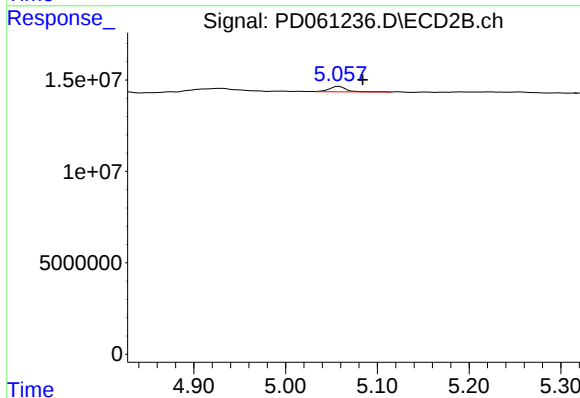


#7 delta-BHC

R.T.: 5.058 min
Delta R.T.: -0.026 min
Response: 3774189
Conc: 0.37 ng/ml

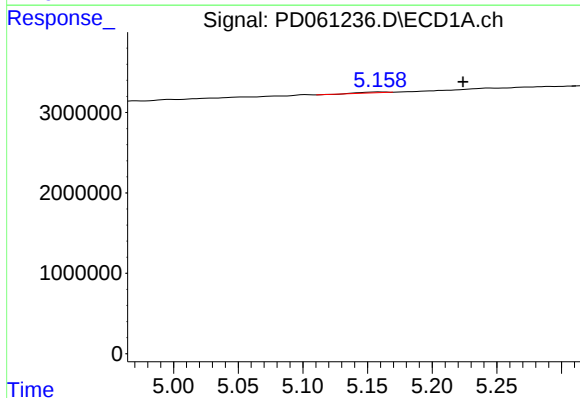


#8 Heptachlor epoxide

R.T.: 5.159 min
Delta R.T.: -0.065 min
Response: 153282
Conc: 0.11 ng/ml

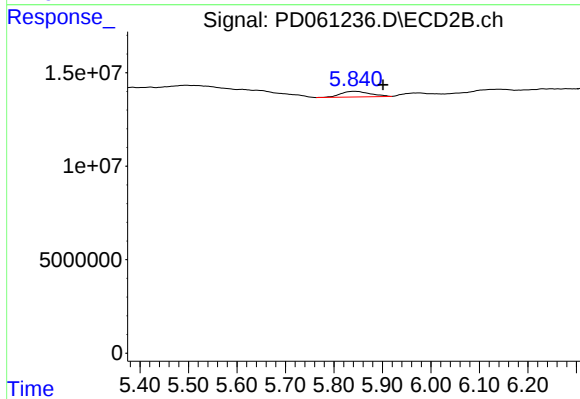

#8 Heptachlor epoxide


R.T.: 5.841 min
Delta R.T.: -0.060 min
Response: 12609507
Conc: 1.46 ng/ml

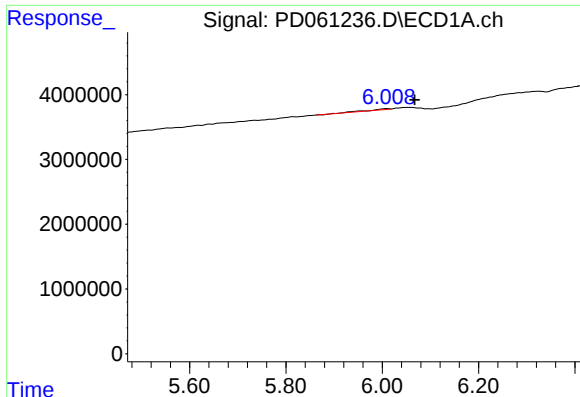

#14 Endrin


R.T.: 6.011 min
Delta R.T.: -0.057 min
Response: 363700
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

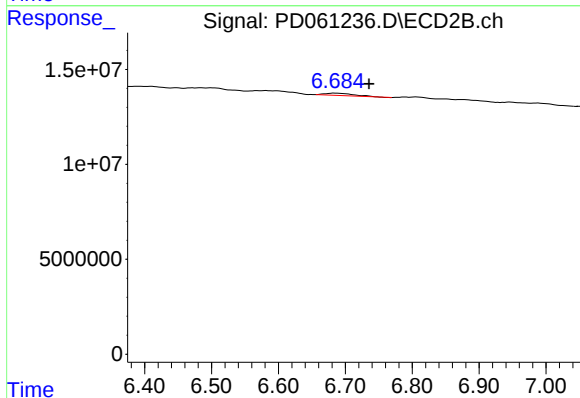


#14 Endrin

R.T.: 6.684 min
Delta R.T.: -0.051 min
Response: 3690558
Conc: 0.50 ng/ml

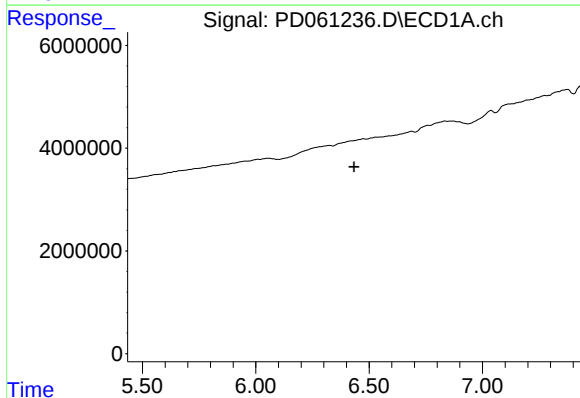


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

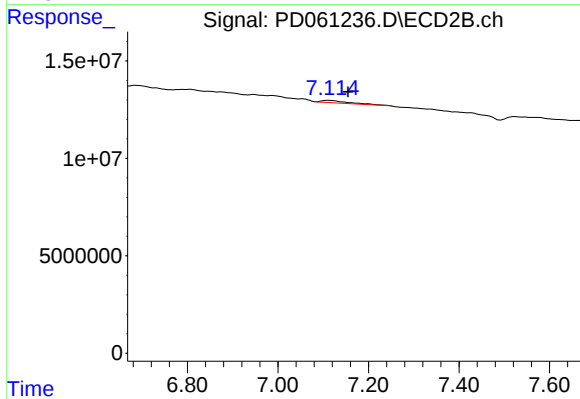

#17 4,4'-DDT


R.T.: 7.111 min
Delta R.T.: -0.043 min
Response: 4955700
Conc: 0.68 ng/ml

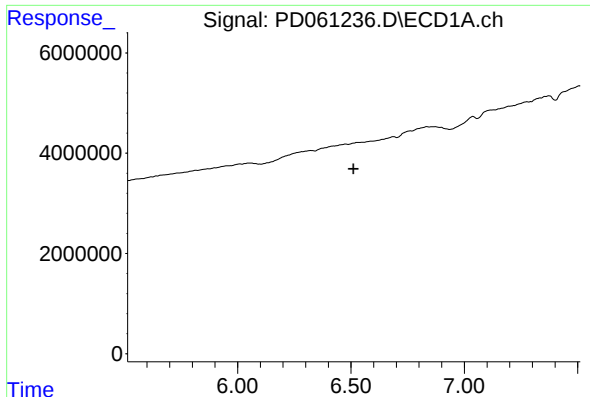

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

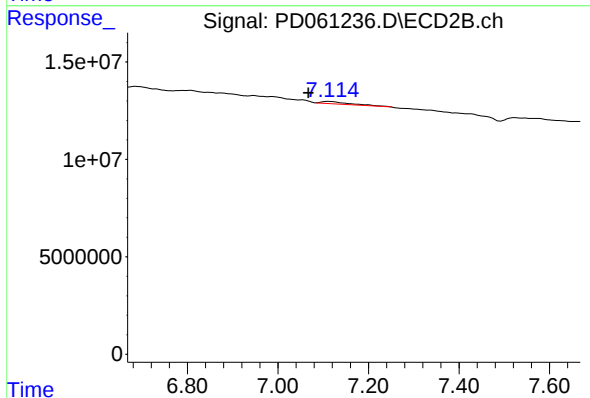


#18 Endrin aldehyde

R.T.: 7.111 min
Delta R.T.: 0.044 min
Response: 4955700
Conc: 0.84 ng/ml

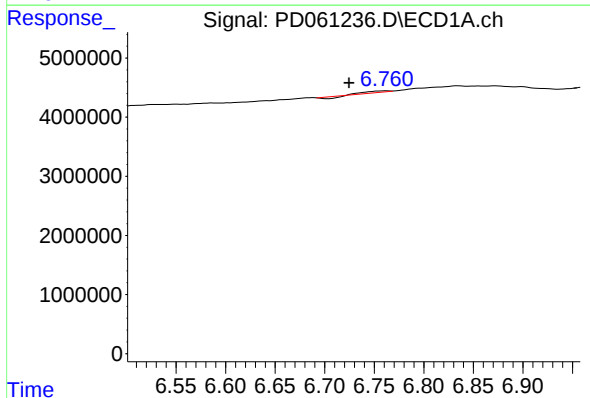


#19 Endosulfan Sulfate

R.T.: 6.761 min
Delta R.T.: 0.037 min
Response: 268640
Conc: 0.26 ng/ml

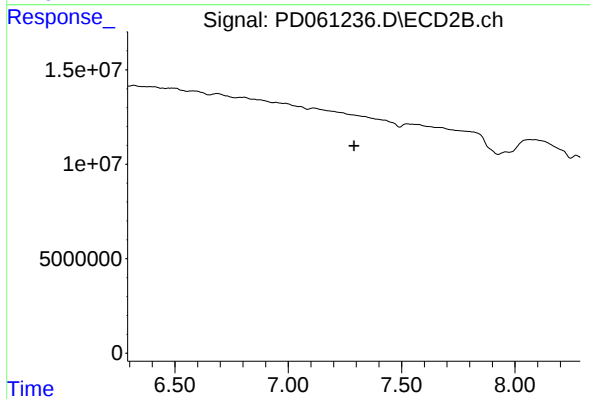

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.291 min
Response: 0
Conc: N.D.

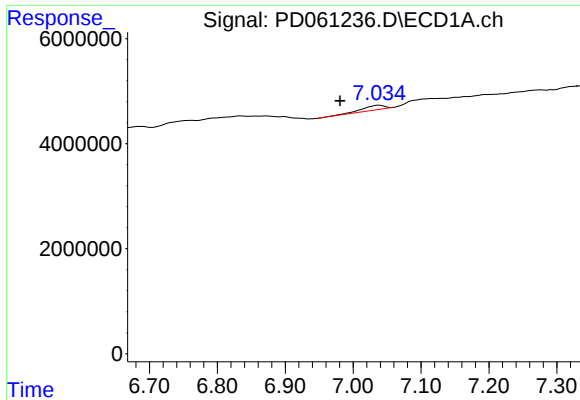

#20 Methoxychlor


R.T.: 7.038 min
Delta R.T.: 0.057 min
Response: 1907741
Conc: 3.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

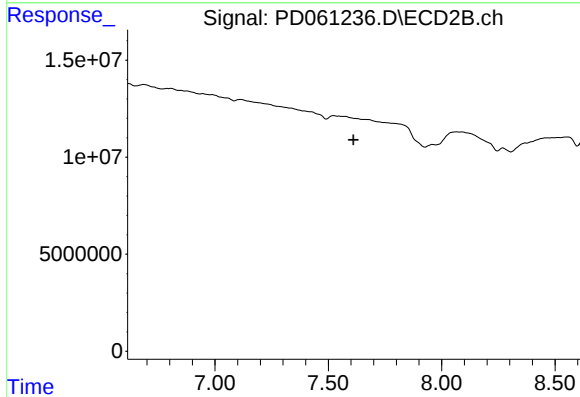


#20 Methoxychlor

R.T.: 7.547 min
Delta R.T.: -0.064 min
Response: -138723
Conc: N.D.

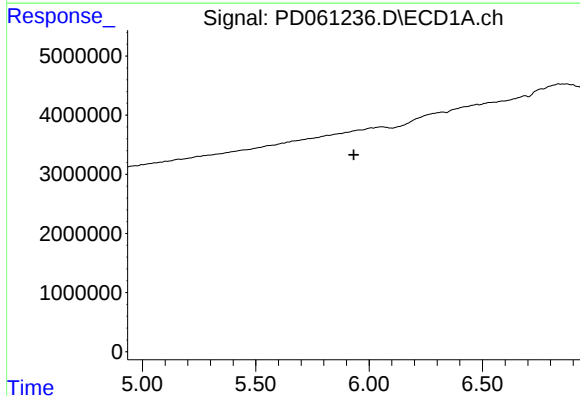


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.933 min
Response: 0
Conc: N.D.

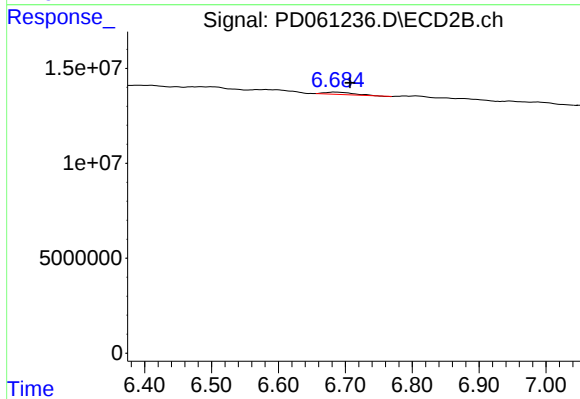

#23 Toxaphene-2


R.T.: 6.684 min
Delta R.T.: -0.023 min
Response: 3690558
Conc: 56.12 ng/ml

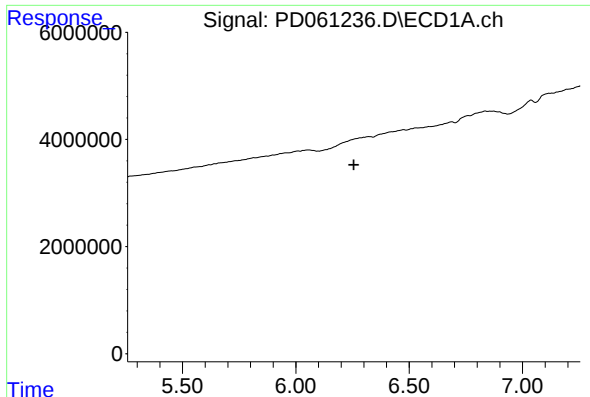

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

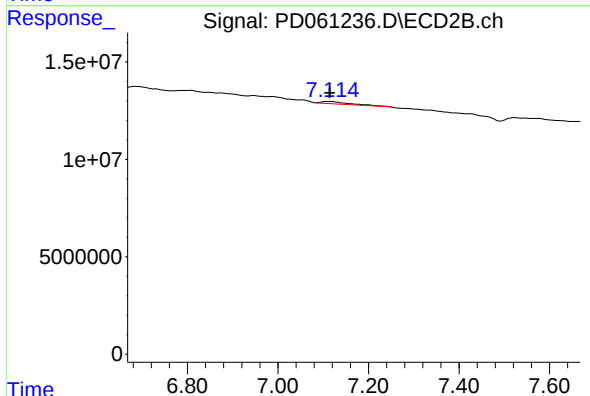


#24 Toxaphene-3

R.T.: 7.111 min
Delta R.T.: -0.003 min
Response: 4955700
Conc: 51.73 ng/ml

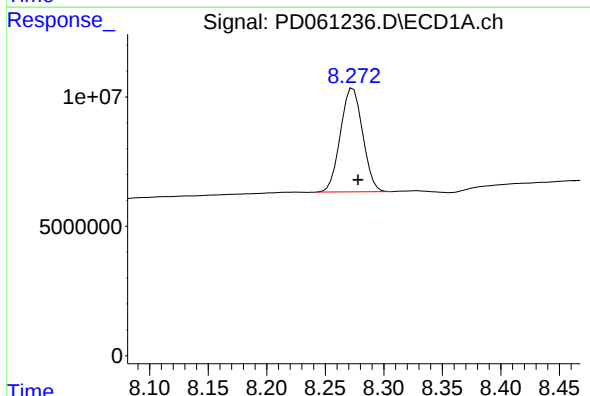

#27 Decachlorobiphenyl

R.T.: 8.274 min
Delta R.T.: -0.004 min
Response: 53036497
Conc: 42.09 ng/ml

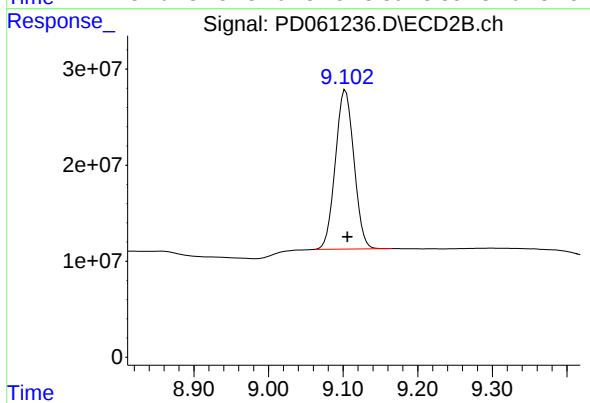

#27 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: -0.003 min
Response: 286728498
Conc: 42.22 ng/ml