

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021521\
 Data File : PD061242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 12:43
 Operator : DD\AJ
 Sample : INDA308
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 ECD_D
 LabSampleId :
 INDA308

Manual Integrations
 APPROVED

Ankita
 2/16/2021 10:03:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:49:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

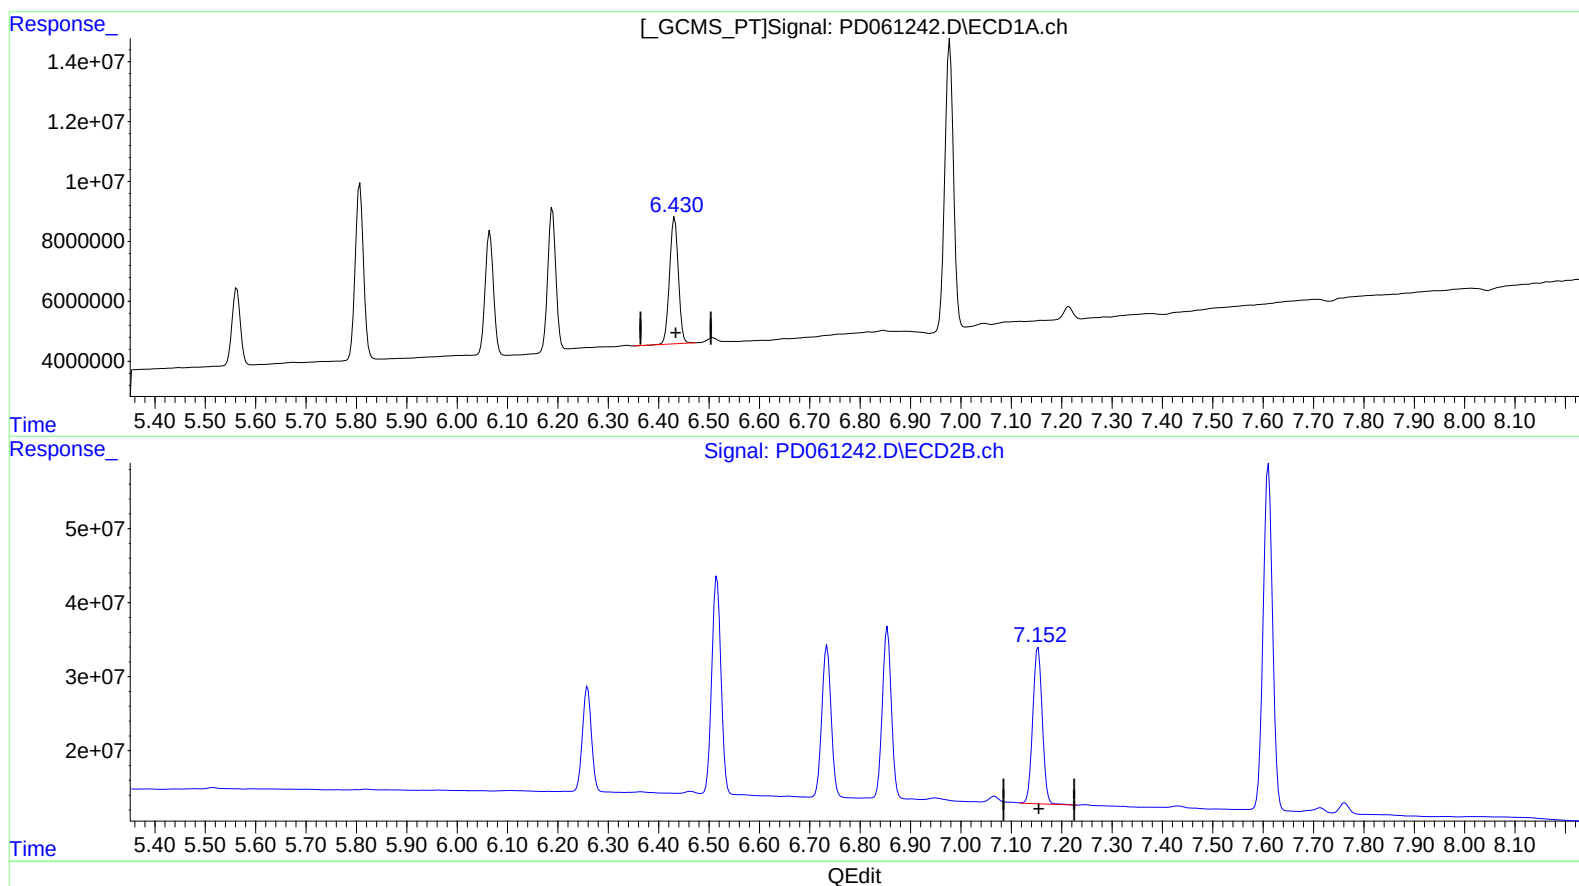

(17) 4,4'-DDT (MA)

6.432min 41.964 ng/ml

response 51383356

(17) 4,4'-DDT #2 (MA)

7.153min 38.244 ng/ml

response 277713557

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021521\
 Data File : PD061242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 12:43
 Operator : DD\AJ
 Sample : INDA308
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 ECD_D
 LabSampleId :
 INDA308

Manual Integrations
 APPROVED

Ankita
 2/16/2021 10:03:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:49:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

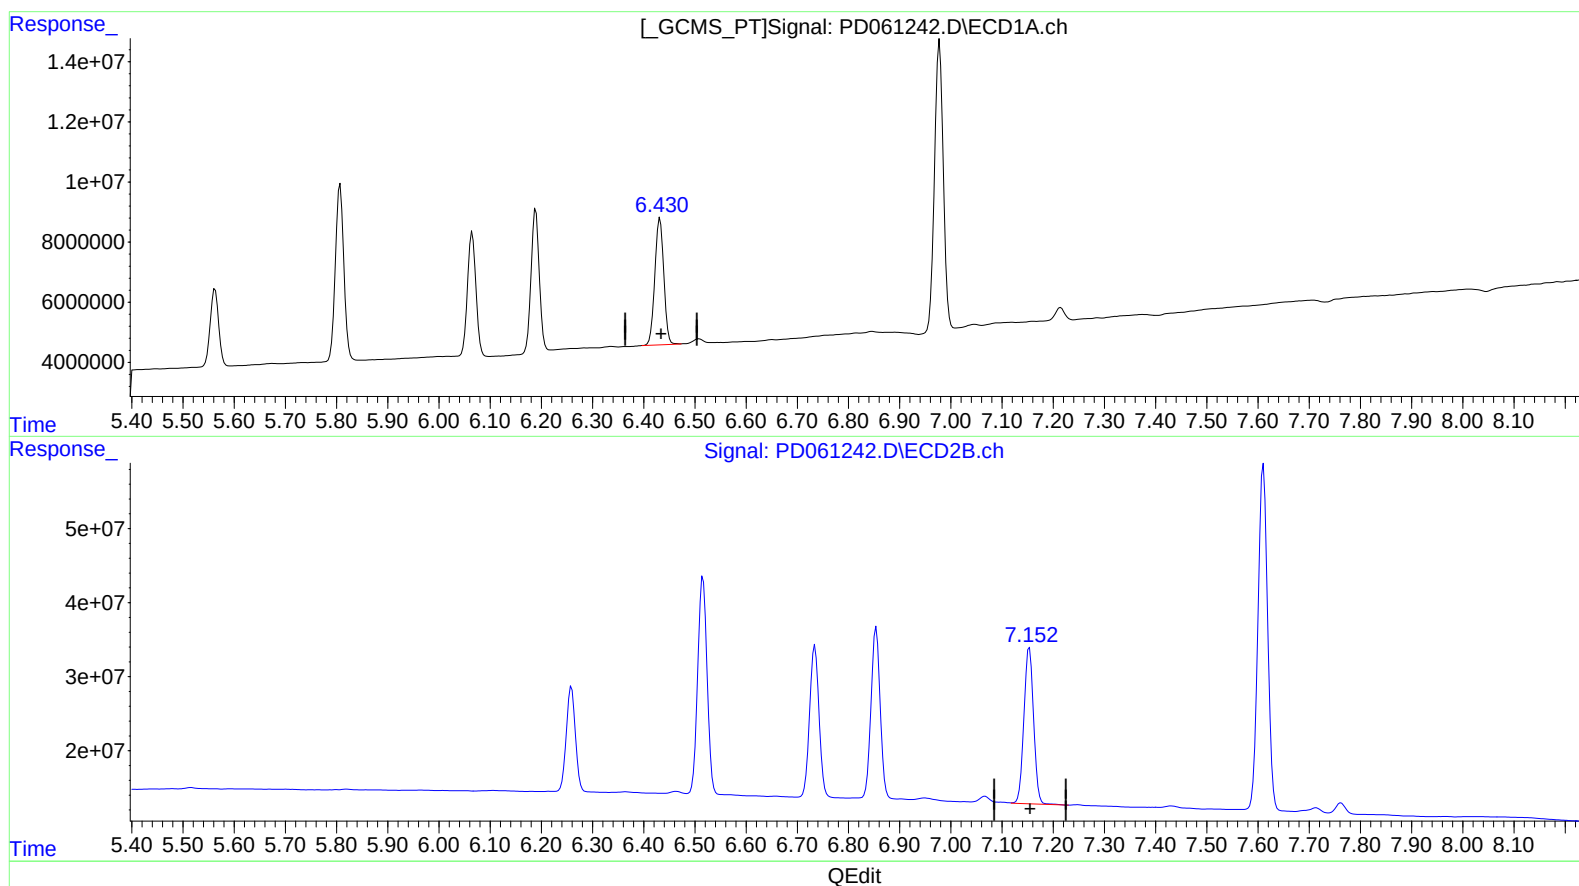

(17) 4,4'-DDT (MA)
 6.430min 41.959 ng/ml m
 response 51376941

(17) 4,4'-DDT #2 (MA)
 7.153min 38.244 ng/ml
 response 277713557

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021521\
 Data File : PD061242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 12:43
 Operator : DD\AJ
 Sample : INDA308
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA308

Manual Integrations
 APPROVED

Ankita
 2/16/2021 10:03:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:49:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.020	23679509	152.8E6	23.330	21.349
27) SA Decachlor...	8.275	9.103	51631854	258.9E6	40.977	38.122
Target Compounds						
2) A alpha-BHC	3.936	4.411	37252066	231.8E6	24.988	20.950
3) MA gamma-BHC...	4.221	4.696	34803838	215.5E6	23.788	21.240
4) MA Heptachlor	4.526	5.208	32875499	220.3E6	21.754	20.890
9) A Endosulfan I	5.563	6.259	29879169	174.5E6	22.784	20.249
13) MA Dieldrin	5.807	6.516	67838509	374.2E6	46.199	40.255
14) MA Endrin	6.065	6.734	47566321	264.6E6	38.266	35.812
16) A 4,4'-DDD	6.189	6.854	54362468	289.9E6	46.315	40.741
17) MA 4,4'-DDT	6.430	7.153	51376941	277.7E6	41.959m	38.244
20) A Methoxychlor	6.978	7.611	116.9E6	613.2E6	187.283	185.777

17
 2/21/21

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.