

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021523\
 Data File : PD073966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2023 09:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 20:21:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	9.034f	0.000	26981	0	<MDL	N.D. #
Target Compounds							
3)	MA gamma-BHC...	4.388f	0.000	182709	0	<MDL	N.D. #
4)	MA Heptachlor	4.888f	0.000	235513	0	<MDL	N.D. #
5)	MB Aldrin	0.000	4.210	0	327879	N.D.	0.193
6)	B beta-BHC	0.000	3.865f	0	76352	N.D.	<MDL
7)	B delta-BHC	4.790	4.157	1168111	96996	0.357	<MDL #
8)	B Heptachlo...	5.710	4.678f	6948711	159210	2.136	0.102 #
9)	A Endosulfan I	6.134f	0.000	326228	0	0.106	N.D. #
15)	B Endosulfa...	6.802	0.000	176880	0	<MDL	N.D. #
20)	A Methoxychlor	7.453f	0.000	642459	0	0.432	N.D. #
21)	B Endrin ke...	7.672	0.000	612301	0	0.192	N.D. #
22)	Toxaphene-1	6.283	0.000	334158	0	14.849	N.D. #
23)	Toxaphene-2	6.510f	0.000	328942	0	11.176	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021523\
Data File : PD073966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2023 09:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 20:21:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

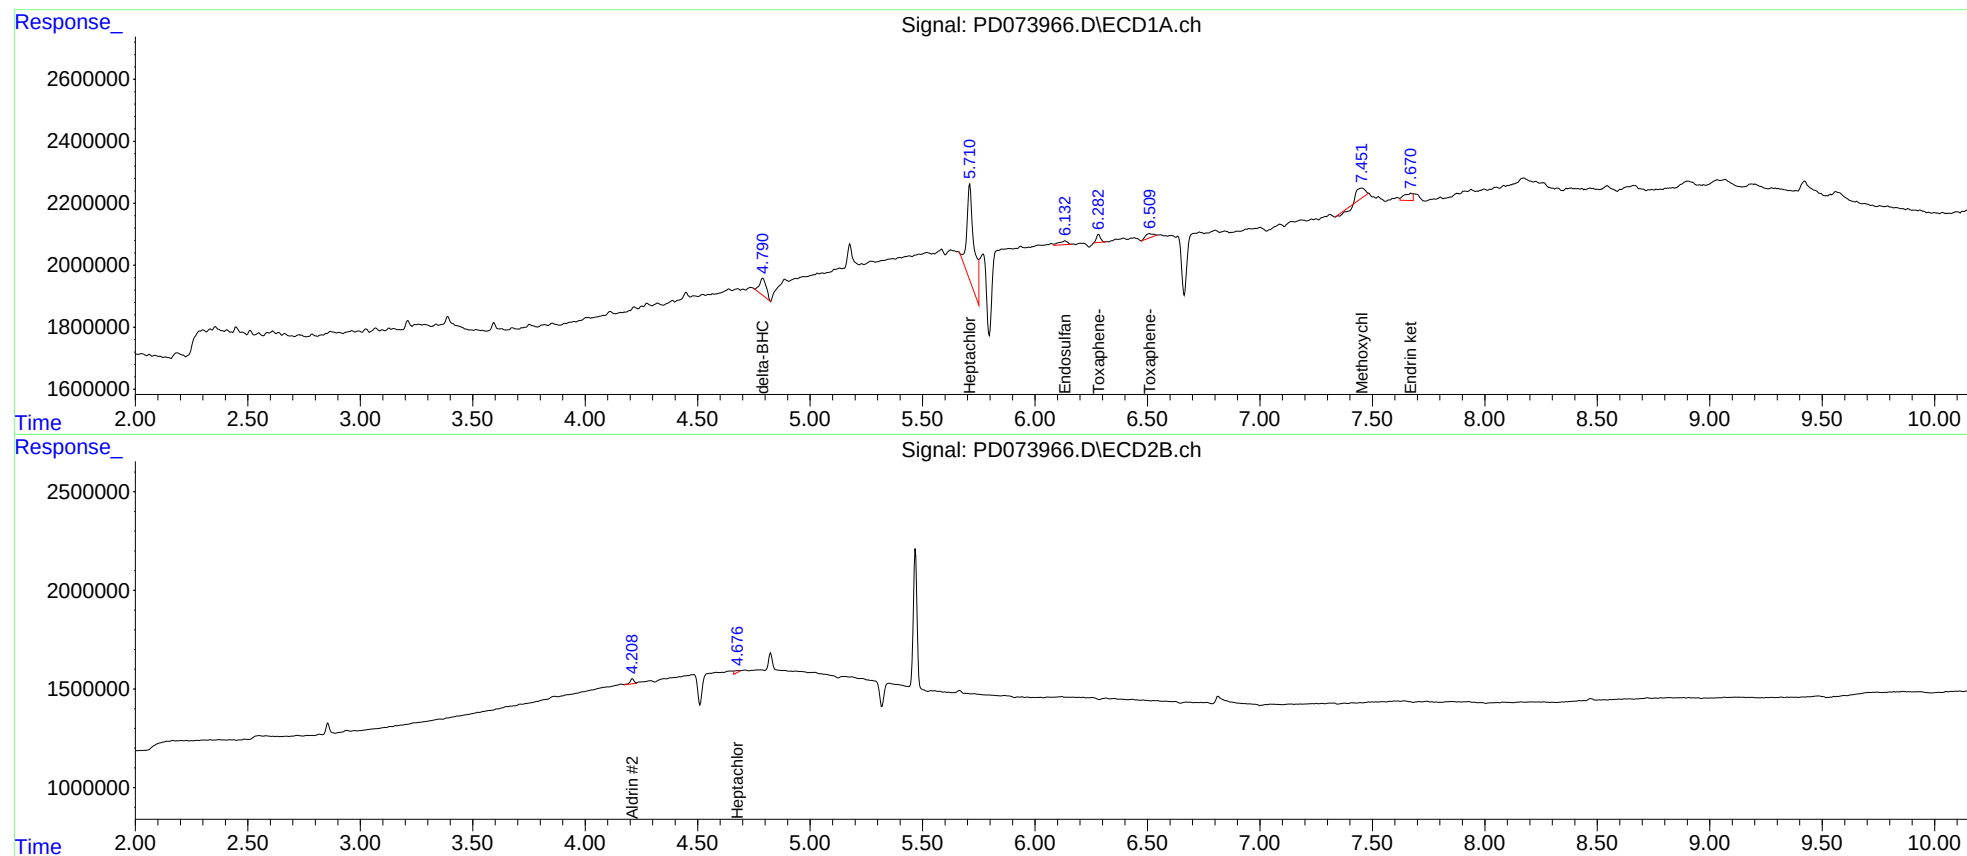

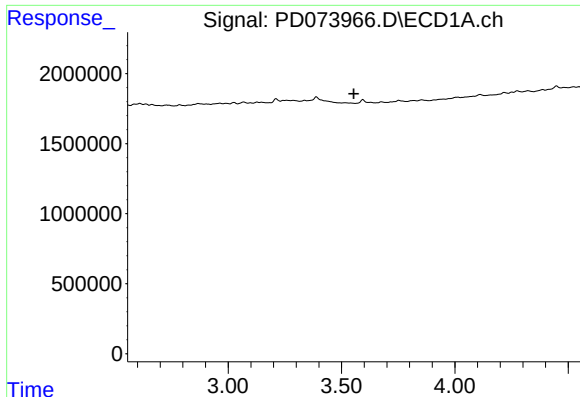


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.554 min
Response: 0
Conc: N.D.

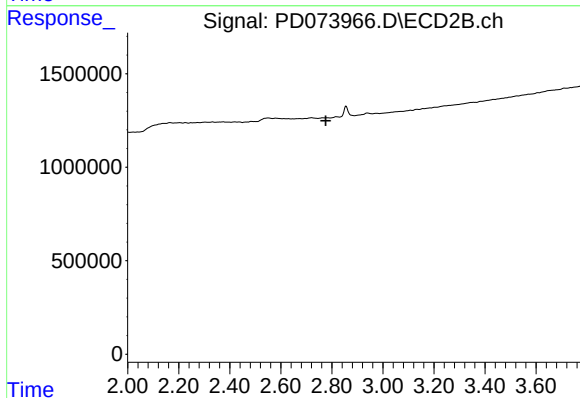


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.776 min
Response: 0
Conc: N.D.

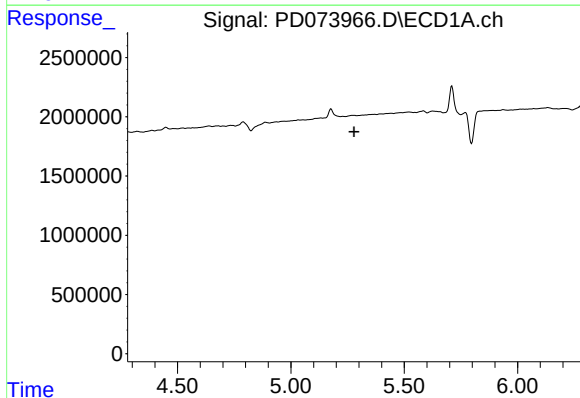


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.279 min
Response: 0
Conc: N.D.

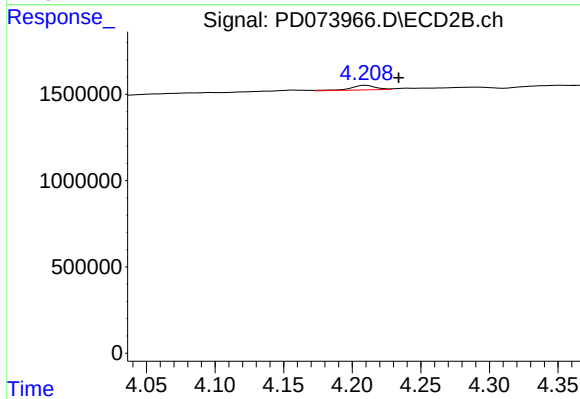


#5 Aldrin

R.T.: 4.210 min
Delta R.T.: -0.024 min
Response: 327879
Conc: 0.19 ng/ml

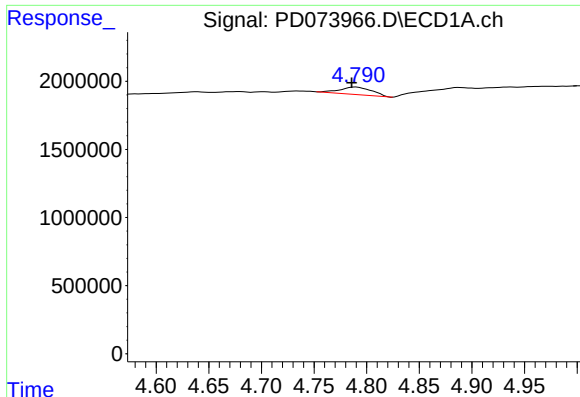


#7 delta-BHC

R.T.: 4.790 min
Delta R.T.: 0.004 min
Response: 1168111
Conc: 0.36 ng/ml

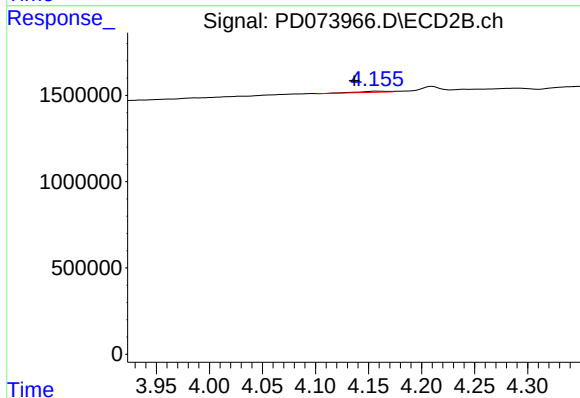


#7 delta-BHC

R.T.: 4.157 min
Delta R.T.: 0.020 min
Response: 96996
Conc: N.D.

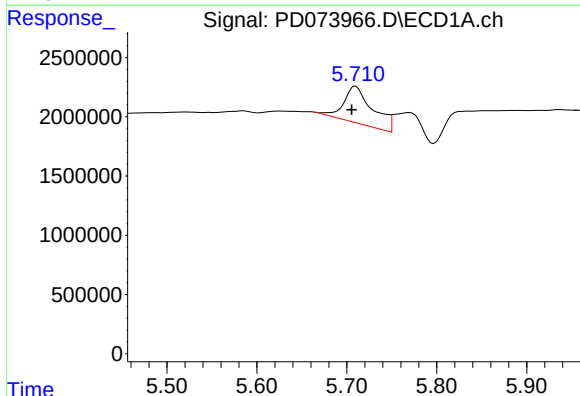


#8 Heptachlor epoxide

R.T.: 5.710 min
Delta R.T.: 0.004 min
Response: 6948711
Conc: 2.14 ng/ml

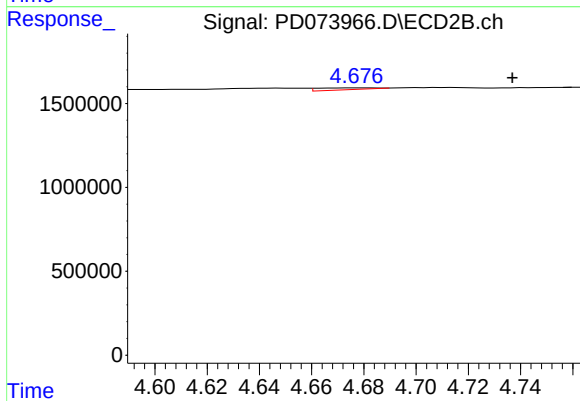


#8 Heptachlor epoxide

R.T.: 4.678 min
Delta R.T.: -0.059 min
Response: 159210
Conc: 0.10 ng/ml

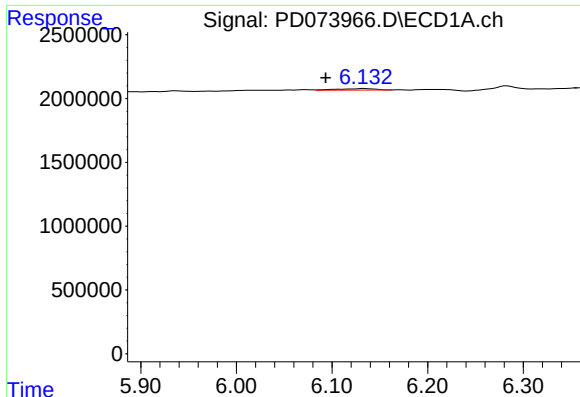


#9 Endosulfan I

R.T.: 6.134 min
Delta R.T.: 0.040 min
Response: 326228
Conc: 0.11 ng/ml

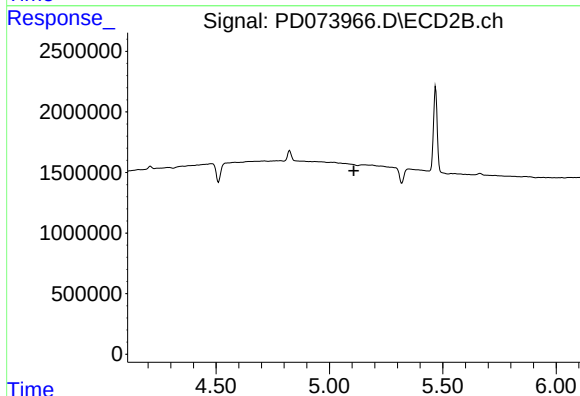


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.107 min
Response: 0
Conc: N.D.

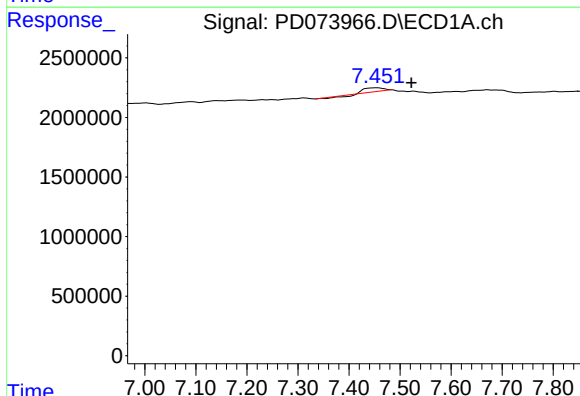


#20 Methoxychlor

R.T.: 7.453 min
Delta R.T.: -0.069 min
Response: 642459
Conc: 0.43 ng/ml

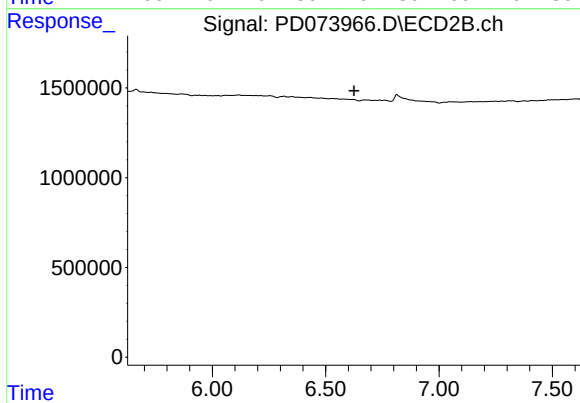


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.625 min
Response: 0
Conc: N.D.

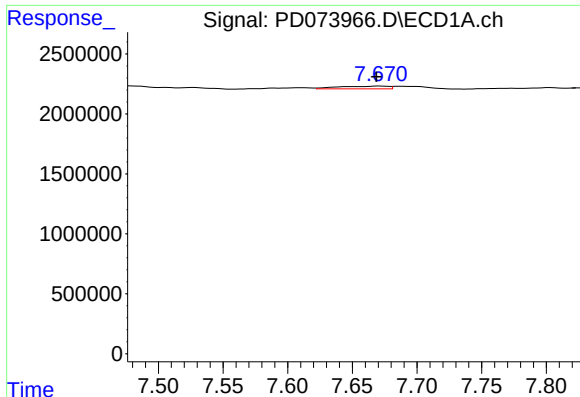


#21 Endrin ketone

R.T.: 7.672 min
Delta R.T.: 0.003 min
Response: 612301
Conc: 0.19 ng/ml

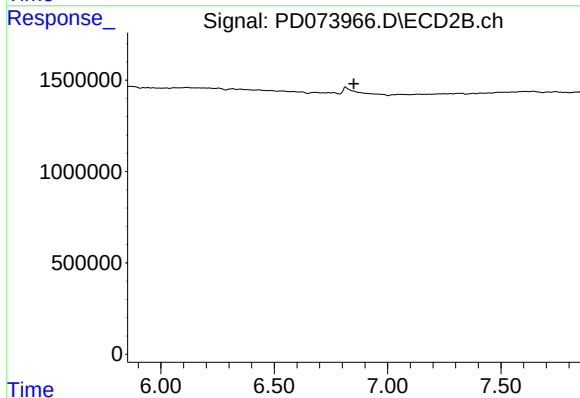


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.851 min
Response: 0
Conc: N.D.

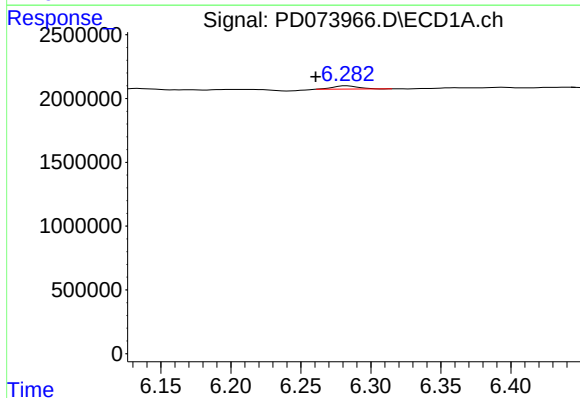


#22 Toxaphene-1

R.T.: 6.283 min
Delta R.T.: 0.022 min
Response: 334158
Conc: 14.85 ng/ml

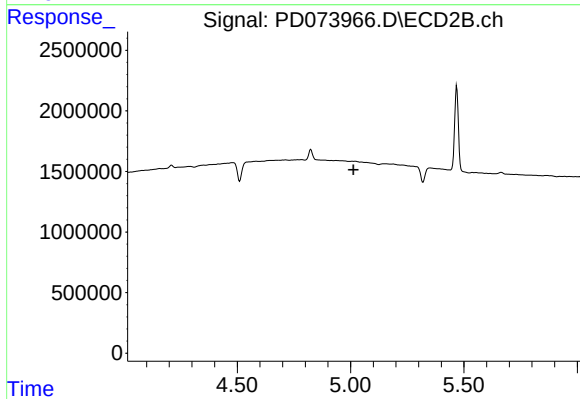


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.013 min
Response: 0
Conc: N.D.

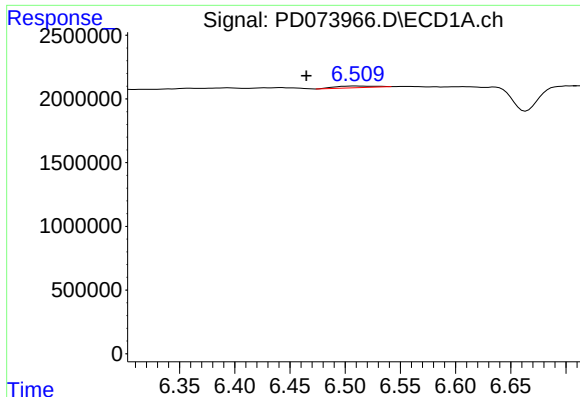


#23 Toxaphene-2

R.T.: 6.510 min
Delta R.T.: 0.045 min
Response: 328942
Conc: 11.18 ng/ml

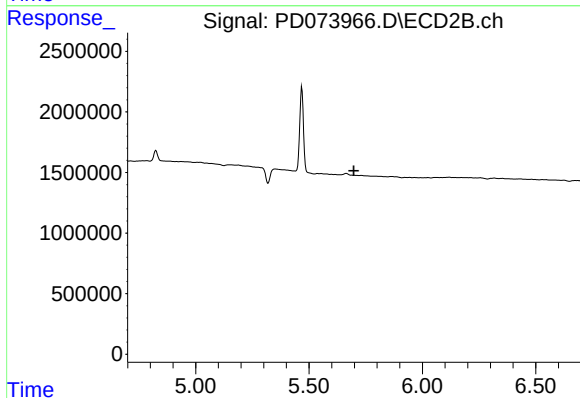


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 5.698 min
Response: 0
Conc: N.D.

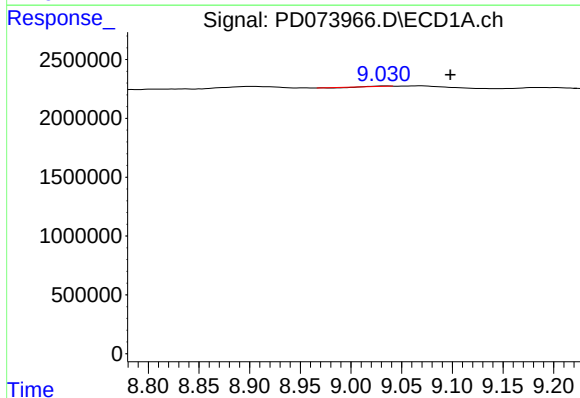

#27 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.065 min
Response: 26981
Conc: N.D.

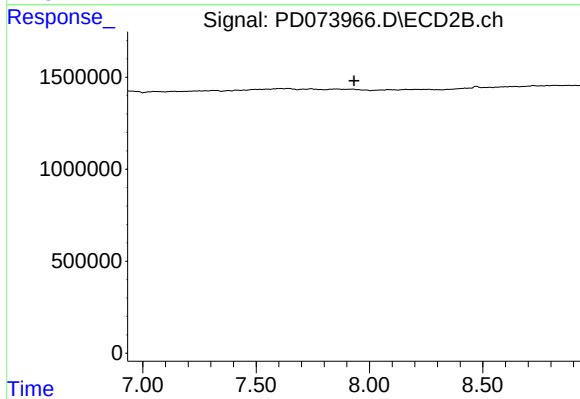

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.932 min
Response: 0
Conc: N.D.