

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
 Data File : PD081373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 10:17
 Operator : AR\AJ
 Sample : P1300-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6Z6MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 21:46:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.794	28500728	52875860	20.847	21.568
27)	SA Decachlor...	9.114	7.932	47037394	64315180	24.380	25.926
Target Compounds							
2)	A alpha-BHC	4.022	3.296	119.3E6	208.3E6	51.072	54.173
3)	MA gamma-BHC...	4.355	3.625	115.4E6	190.1E6	49.946	52.496
4)	MA Heptachlor	4.948	3.966	130.0E6	186.0E6	52.992	52.430
5)	MB Aldrin	5.292	4.246	129.5E6	178.2E6	54.773	52.624
6)	B beta-BHC	4.550	3.920	49407318	78760083	47.543	46.612
7)	B delta-BHC	4.799	4.151	126.0E6	193.0E6	53.213	51.533
8)	B Heptachlo...	5.718	4.748	124.5E6	167.0E6	54.964	52.045
9)	A Endosulfan I	6.105	5.117	118.9E6	156.3E6	56.450	52.209
10)	B trans-Chl...	5.974	4.997	123.0E6	165.8E6	56.176	53.140
11)	B cis-Chlor...	6.054	5.062	125.8E6	167.1E6	55.868	52.164
12)	B 4,4'-DDE	6.225	5.250	240.4E6	321.5E6	112.002	108.728
13)	MA Dieldrin	6.380	5.382	229.0E6	346.9E6	103.131	105.612
14)	MA Endrin	6.611	5.657	190.6E6	309.6E6	101.536	107.758
15)	B Endosulfa...	6.829	5.950	202.1E6	300.6E6	104.673	106.490
16)	A 4,4'-DDD	6.743	5.804	174.1E6	271.2E6	104.813	107.609
17)	MA 4,4'-DDT	7.058	6.055	196.5E6	279.4E6	113.081	108.195
18)	B Endrin al...	6.960	6.129	148.0E6	215.4E6	99.099	99.422
19)	B Endosulfa...	7.194	6.351	194.7E6	282.9E6	106.359	105.467
20)	A Methoxychlor	7.532	6.629	470.6E6	656.8E6	512.995	491.608
21)	B Endrin ke...	7.680	6.857	210.0E6	325.8E6	108.604	108.641

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
Data File : PD081373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 10:17
Operator : AR\AJ
Sample : P1300-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 21:46:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

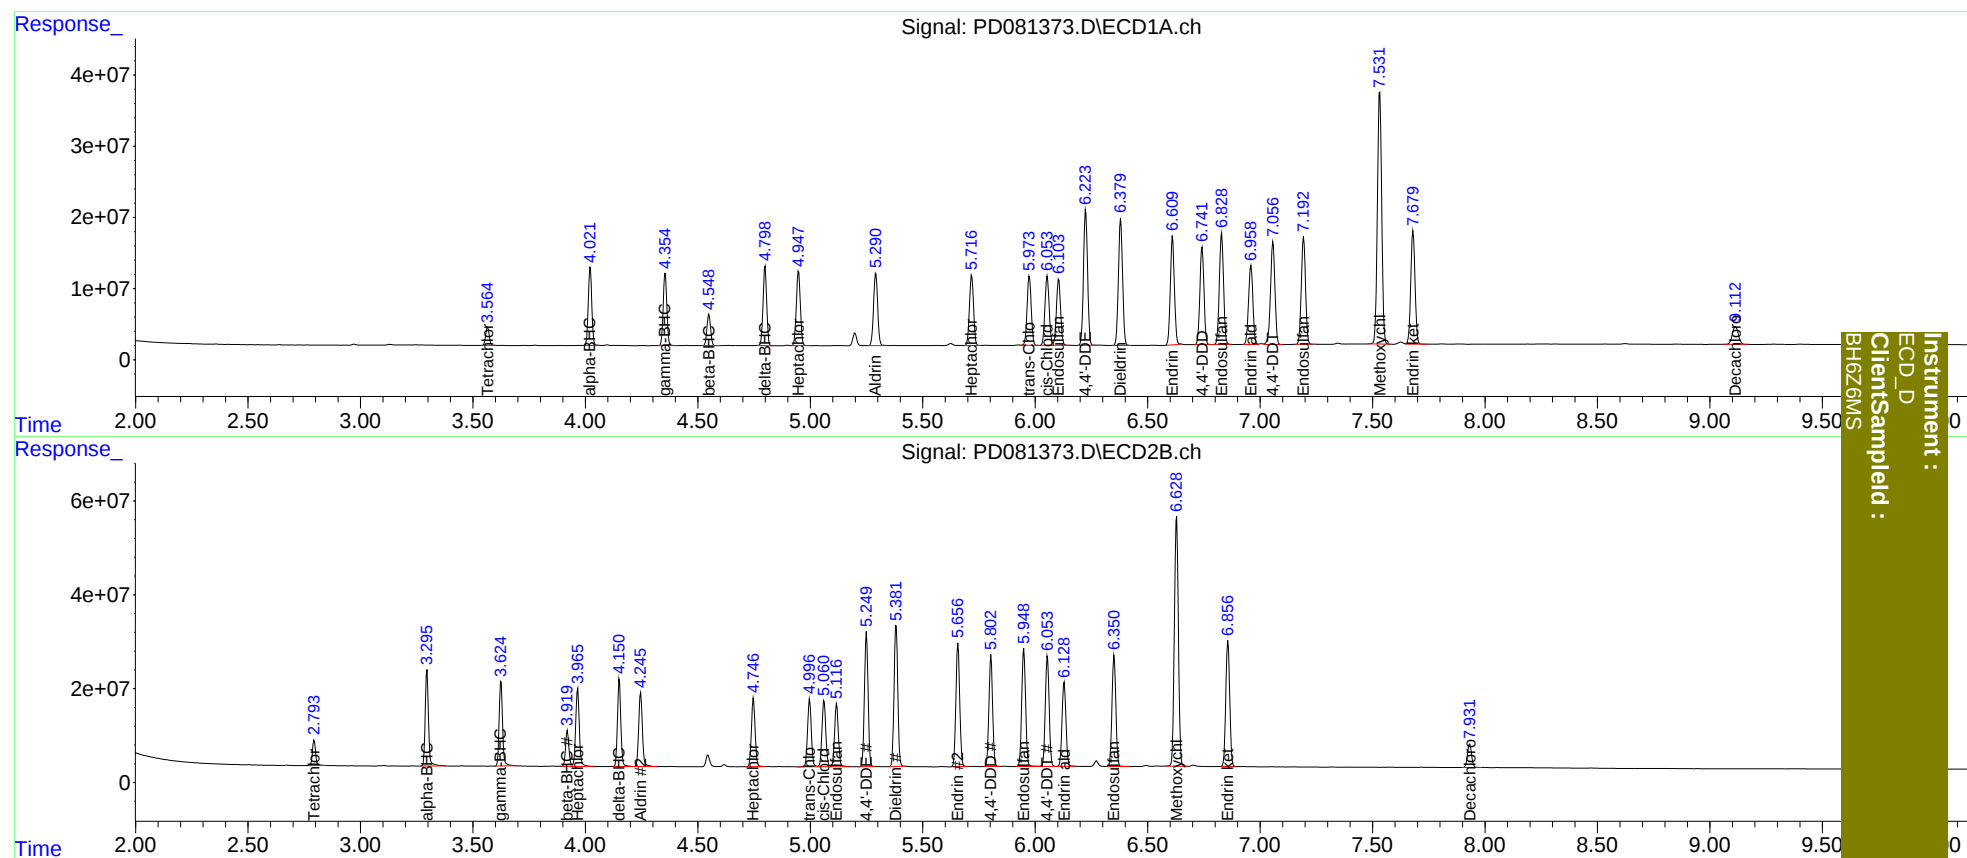

Instrument :
ECD_D
ClientSampled :
BH6Z6MS