

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
 Data File : PD081388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 13:37
 Operator : AR\AJ
 Sample : P1286-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6X5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :Ankita Jodhani 02/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 15:52:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.794	17784623	33622158	13.009	13.715
2)	SA Decachlor...	9.111	7.931	26046046	33019820	13.500m	13.311
Target Compounds							
9)	A Endosulfan I	6.136	5.145	4711743	11082136	2.238m	3.701 #
16)	A 4,4'-DDD	6.736	5.803	3705773	3858379	2.231	1.531m#
17)	MA 4,4'-DDT	7.060	6.052	1639352	3356915	0.944m	1.300 #
19)	B Endosulfa...	7.200	6.344	1466411	1835609	0.801m	0.684m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
Data File : PD081388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 13:37
Operator : AR\AJ
Sample : P1286-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 15:52:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

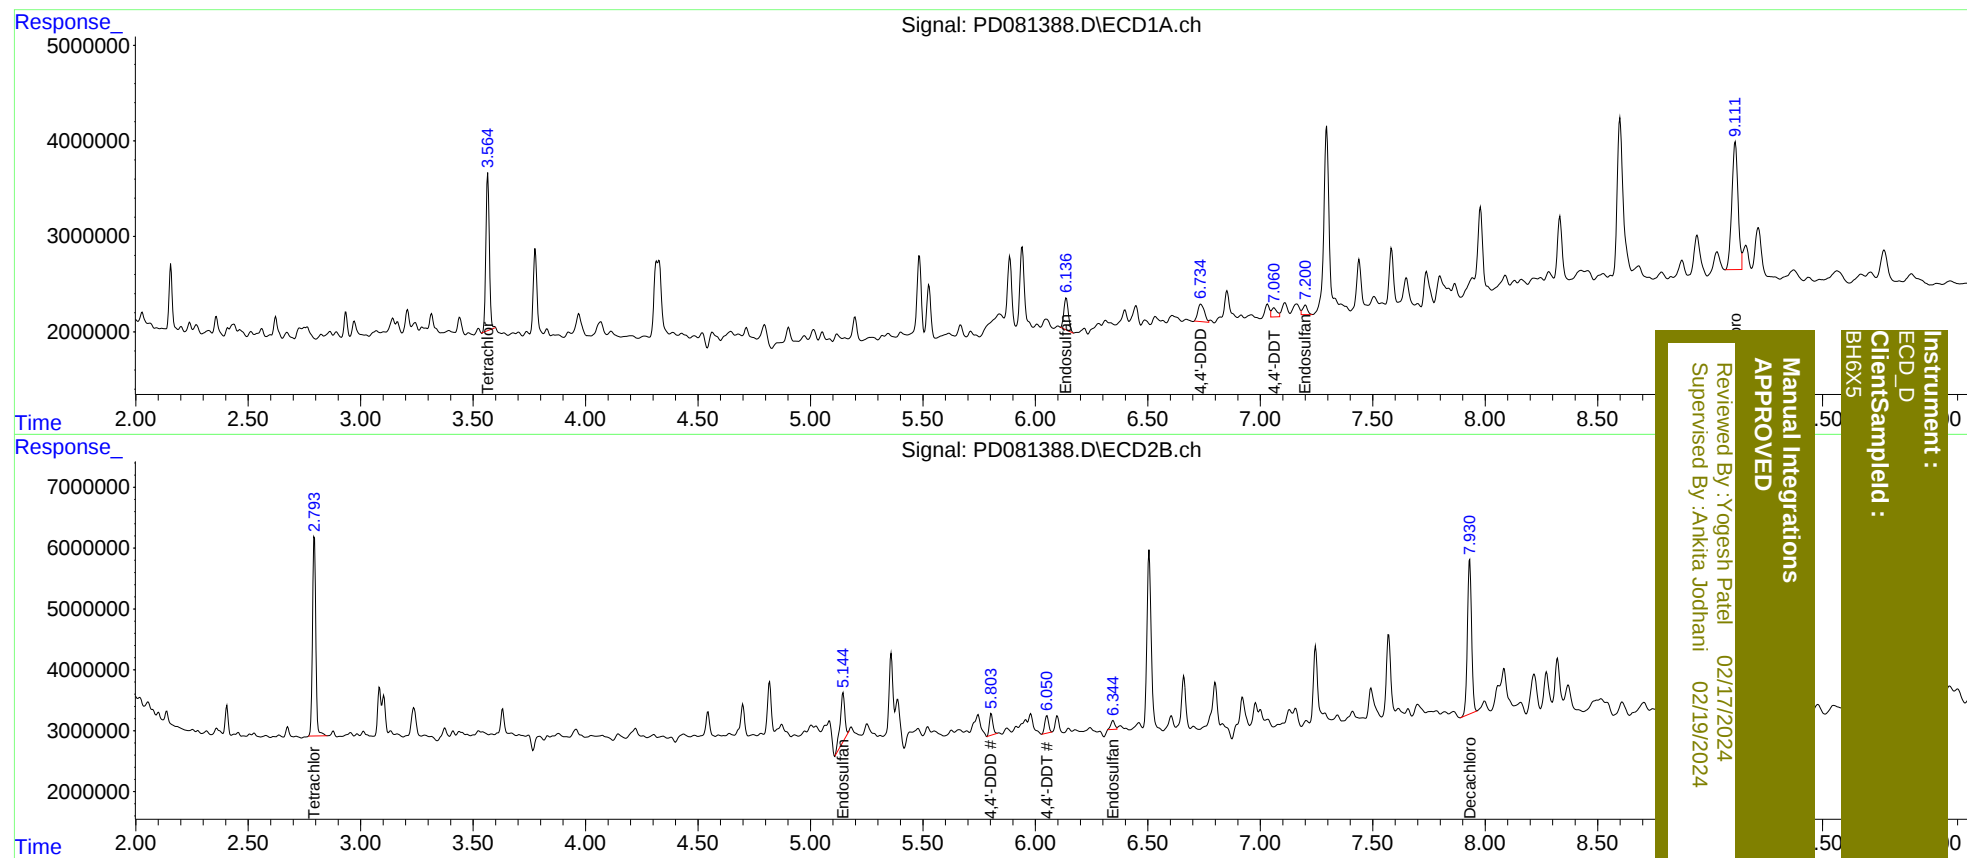

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 02/17/2024
Supervised By : Ankita Jodhani 02/19/2024

Instrument :
ECD_D
ClientSampled :
BH6X5